

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW023006.D
 Acq On : 12 May 2022 17:05
 Operator : SY/VA
 Sample : N2766-16
 Misc : 6.75g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4G6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 13 01:13:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	314657	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	285474	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	130465	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	91171	14.123	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.480%
7) Chloroethane-d5	2.885	69	76278	18.162	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.640%
11) 1,1-Dichloroethene-d2	4.013	63	90690	10.872	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.480%#
21) 2-Butanone-d5	7.074	46	50278	40.962	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.920%
24) Chloroform-d	7.647	84	176331	19.128	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	76.520%
26) 1,2-Dichloroethane-d4	8.305	65	103288m	20.428	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.720%
32) Benzene-d6	8.275	84	327695	19.915	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.680%
36) 1,2-Dichloropropane-d6	9.274	67	101395	21.937	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.760%
41) Toluene-d8	10.323	98	288942	18.178	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.720%
43) trans-1,3-Dichloroprop...	10.579	79	37493	17.617	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.480%
47) 2-Hexanone-d5	10.920	63	42444	48.103	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.200%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	97841	22.711	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.840%
66) 1,2-Dichlorobenzene-d4	13.847	152	89729	19.675	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.680%
Target Compounds					Qvalue	
42) Toluene	10.384	91	26770	1.420	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
Data File : VW023006.D
Acq On : 12 May 2022 17:05
Operator : SY/VA
Sample : N2766-16
Misc : 6.75g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW4G6

Quant Time: May 13 01:13:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 01:10:05 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2022
Supervised By : Mahesh Dadoda 05/16/2022

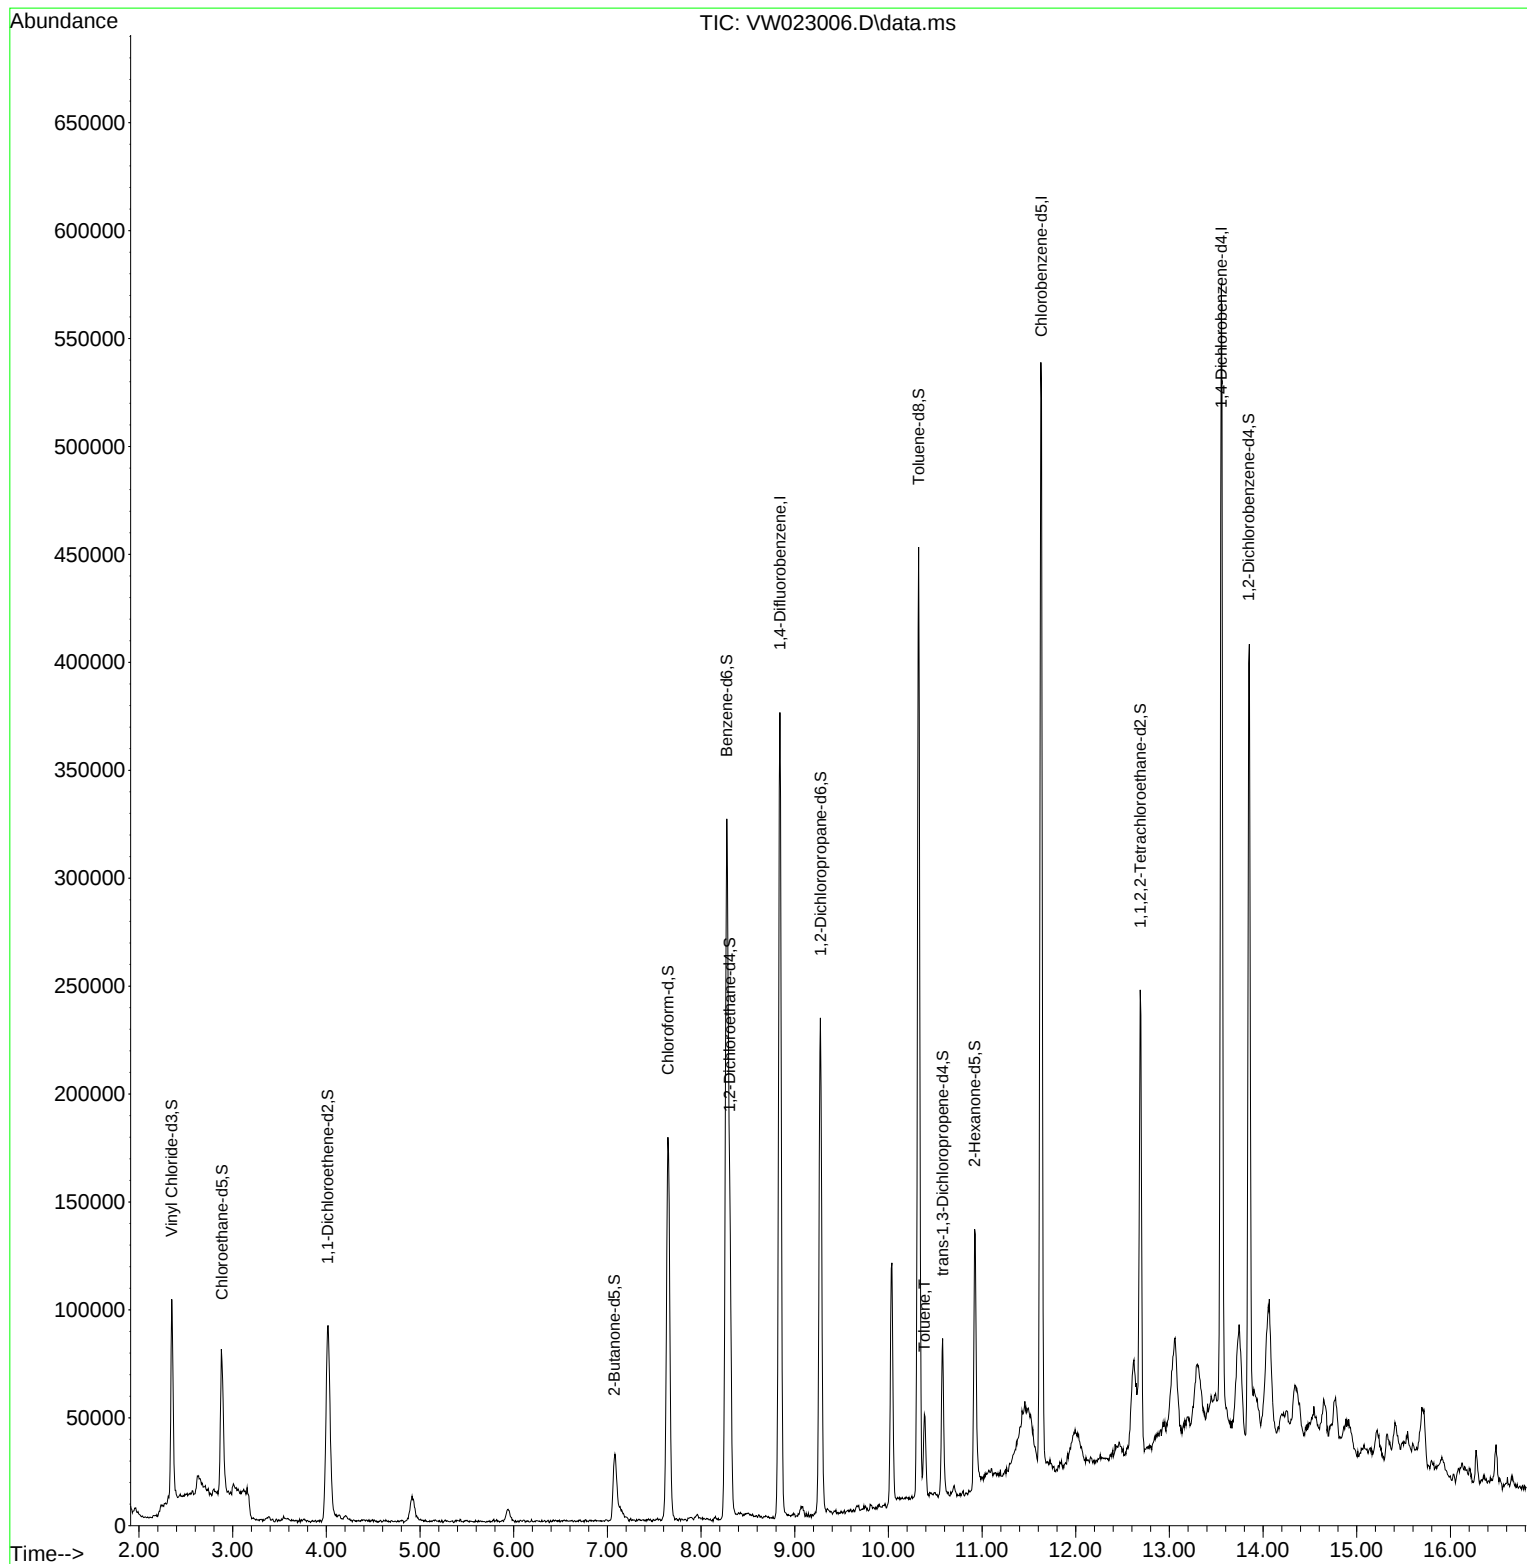

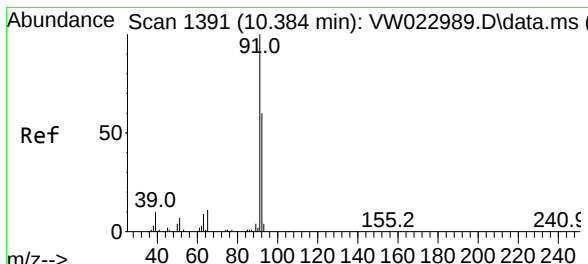

#42
Toluene
Concen: 1.420 ug/L
RT: 10.384 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW023006.D
Acq: 12 May 2022 17:05

Instrument : MSVOA_W
ClientSampleId : EW4G6

Tgt Ion: 91 Resp: 26770
Ion Ratio Lower Upper
91 100
92 55.3 41.6 77.2

Manual Integrations
APPROVED
Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

