

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW023010.D
 Acq On : 12 May 2022 18:42
 Operator : SY/VA
 Sample : N2767-10
 Misc : 6.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM5

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2022
 Supervised By : Mahesh Dadoda 05/16/2022

Quant Time: May 13 01:14:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	297951	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	275274	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	118332	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	98413	16.099	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	64.400%		
7) Chloroethane-d5	2.885	69	81561	20.509	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.040%		
11) 1,1-Dichloroethene-d2	4.013	63	96920	12.271	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	49.080%		
21) 2-Butanone-d5	7.080	46	68052	58.552	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	117.100%		
24) Chloroform-d	7.646	84	192972	22.106	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.440%		
26) 1,2-Dichloroethane-d4	8.305	65	111009	23.186	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.760%		
32) Benzene-d6	8.274	84	333792	21.037	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	84.160%		
36) 1,2-Dichloropropane-d6	9.274	67	109828	24.642	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.560%		
41) Toluene-d8	10.323	98	301513	19.672	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	78.680%		
43) trans-1,3-Dichloroprop...	10.579	79	41092	20.024	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.080%		
47) 2-Hexanone-d5	10.920	63	53666	63.075	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	126.140%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	111775	26.906	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	107.640%		
66) 1,2-Dichlorobenzene-d4	13.853	152	90739	21.936	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	87.760%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	4586m	5.270	ug/L	
16) Methylene chloride	4.927	84	16617	3.811	ug/L	94
35) Methylcyclohexane	9.335	83	5478	0.748	ug/L	95
46) Tetrachloroethene	10.865	164	3277	0.978	ug/L	83
52) Ethylbenzene	11.731	91	410297	20.293	ug/L	99
53) m,p-Xylene	11.835	106	678790	85.204	ug/L	97
54) o-Xylene	12.164	106	263585	34.479	ug/L	98
60) Isopropylbenzene	12.463	105	7116	0.439	ug/L #	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
Data File : VW023010.D
Acq On : 12 May 2022 18:42
Operator : SY/VA
Sample : N2767-10
Misc : 6.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BGPM5

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2022
Supervised By : Mahesh Dadoda 05/16/2022


Quant Time: May 13 01:14:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 01:10:05 2022
Response via : Initial Calibration

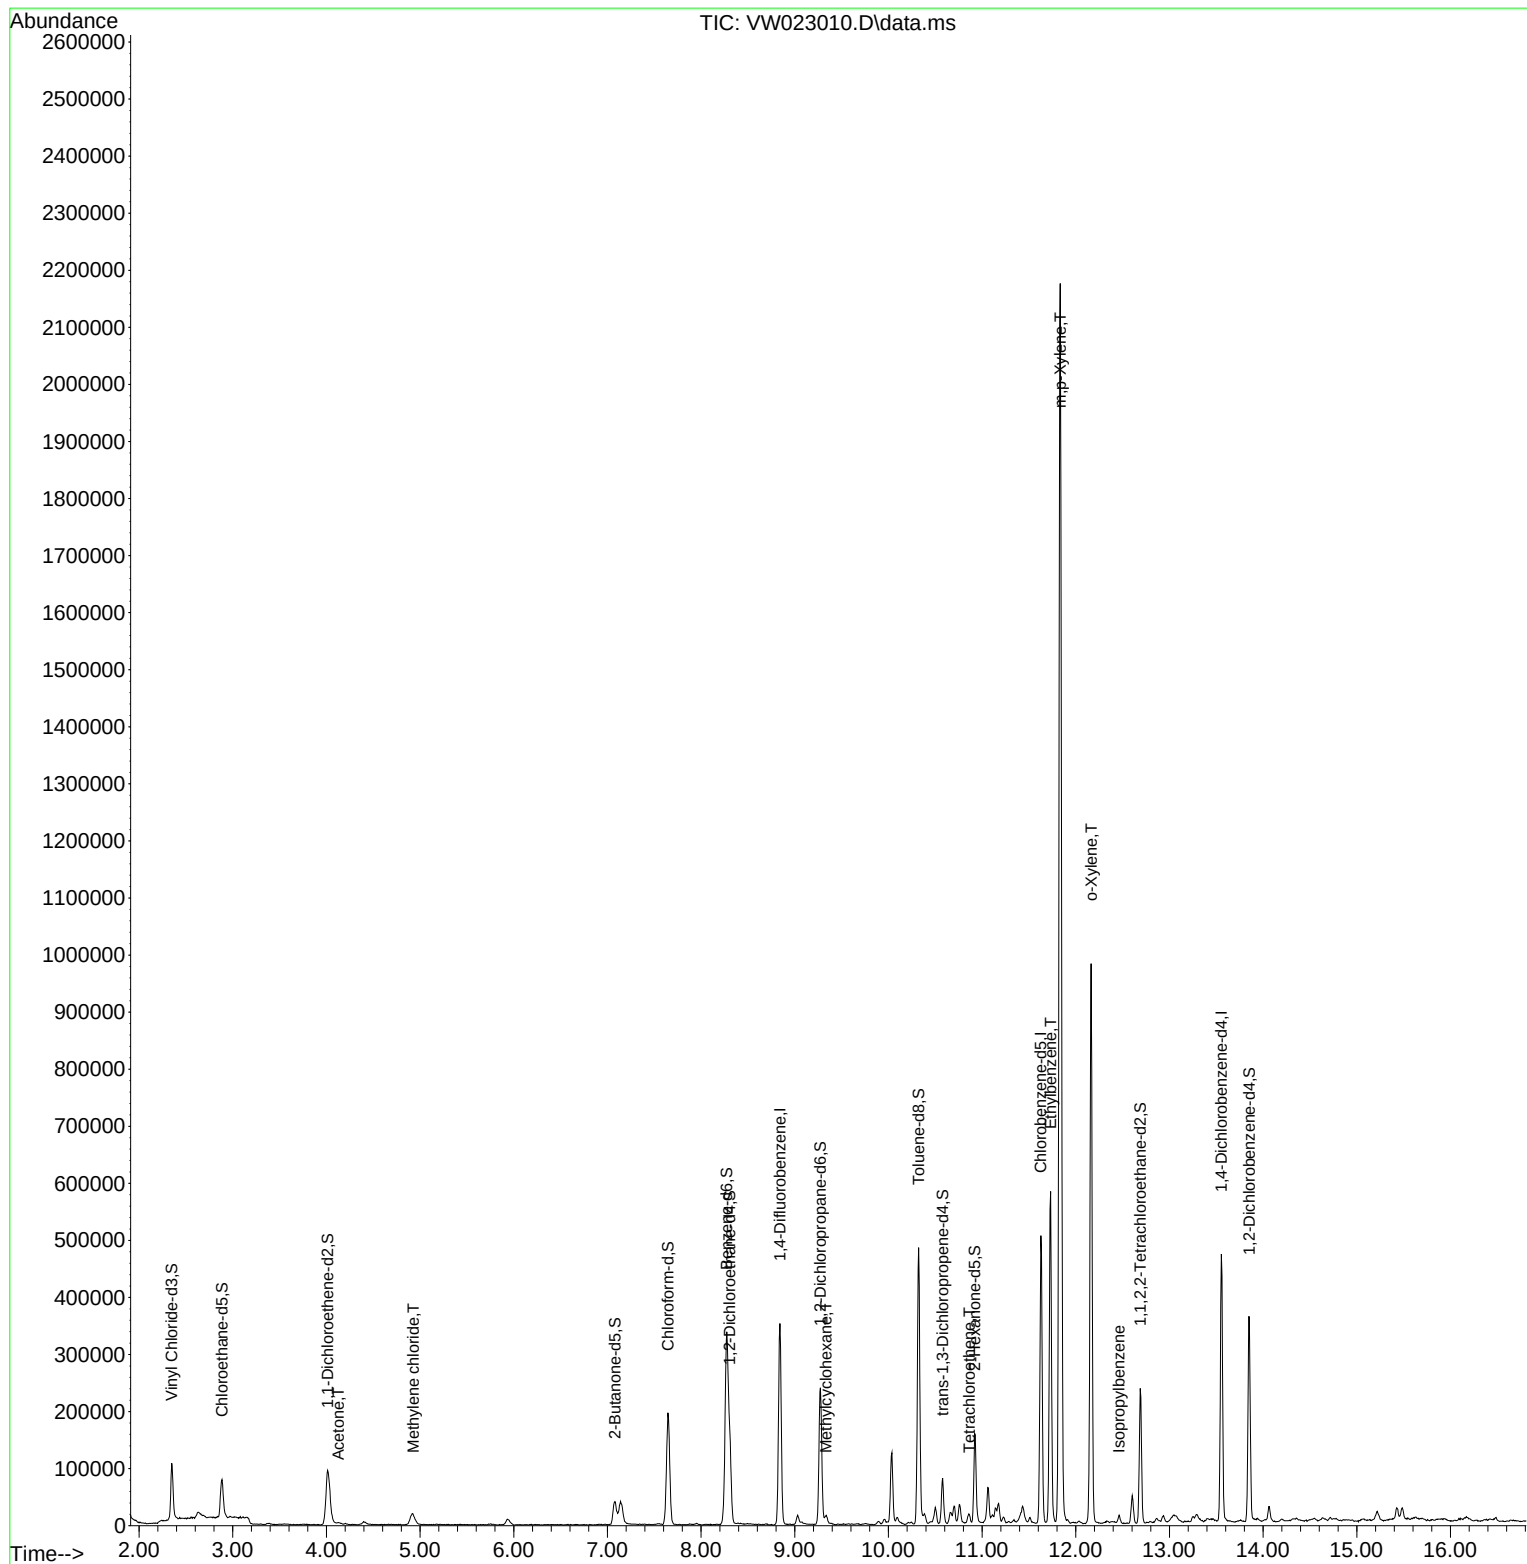

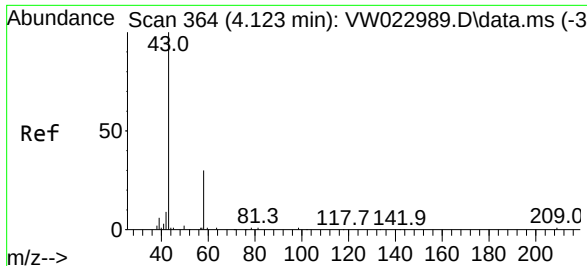

#13
Acetone
Concen: 5.270 ug/L m
RT: 4.129 min Scan# 364
Delta R.T. 0.006 min
Lab File: VW023010.D
Acq: 12 May 2022 18:42




Instrument :
MSVOA_W
ClientSampleId :
BGPM5

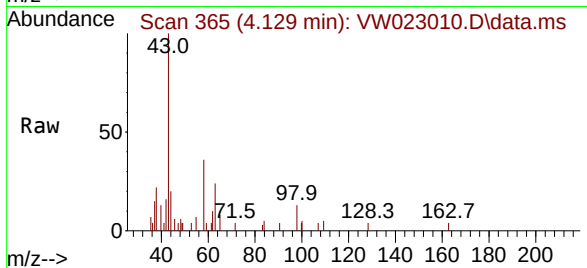

Tgt Ion: 43 Resp: 4580
Ion Ratio Lower Upper
43 100
58 13.0 0.0 64.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

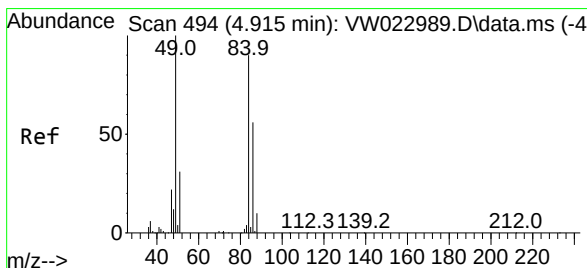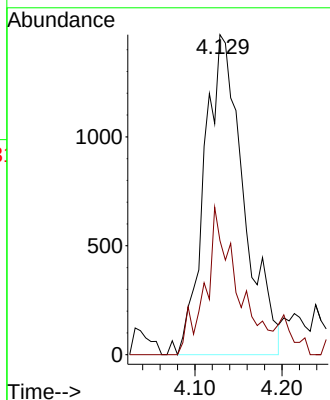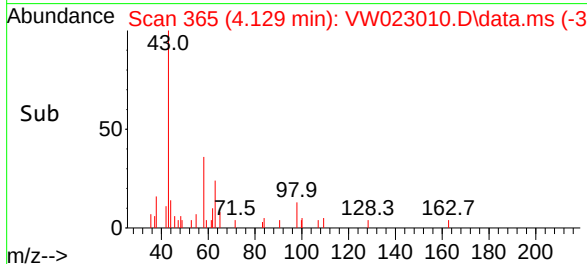

#16
Methylene chloride
Concen: 3.811 ug/L
RT: 4.927 min Scan# 496
Delta R.T. 0.012 min
Lab File: VW023010.D
Acq: 12 May 2022 18:42

Tgt Ion: 84 Resp: 16617
Ion Ratio Lower Upper
84 100
86 62.7 45.4 84.4
49 109.1 82.5 153.1

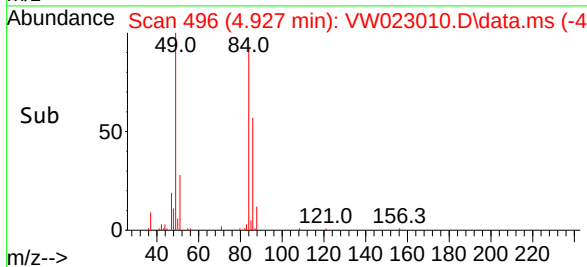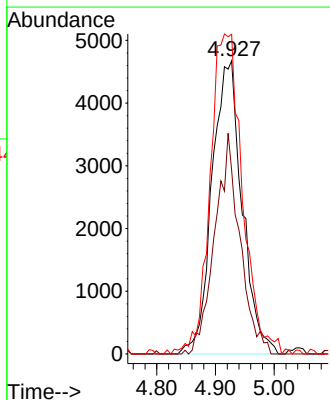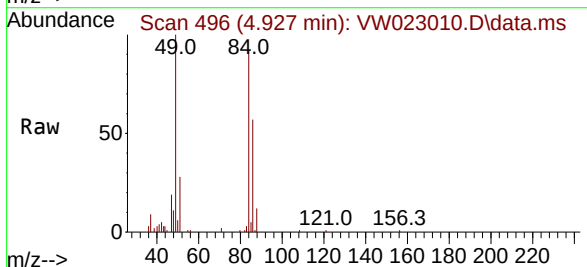

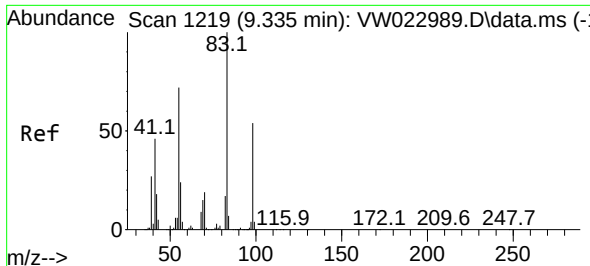





#35
Methylcyclohexane
Concen: 0.748 ug/L
RT: 9.335 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW023010.D
Acq: 12 May 2022 18:42

Instrument :
MSVOA_W
ClientSampleId :
BGPM5

Tgt Ion: 83 Resp: 5478
Ion Ratio Lower Upper
83 100
55 73.2 55.1 82.7
98 53.2 40.4 60.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

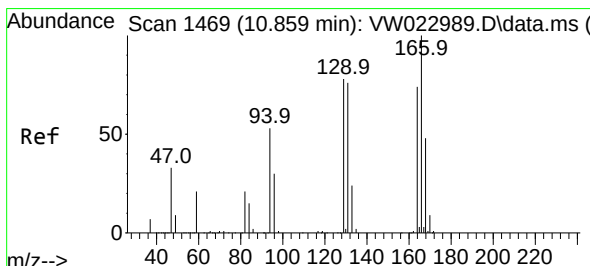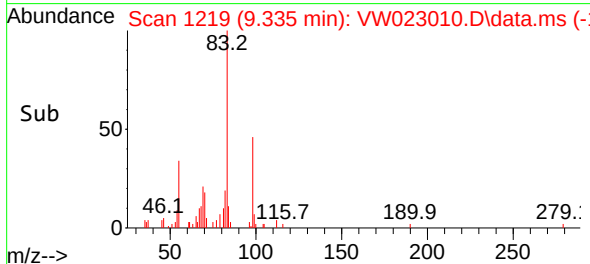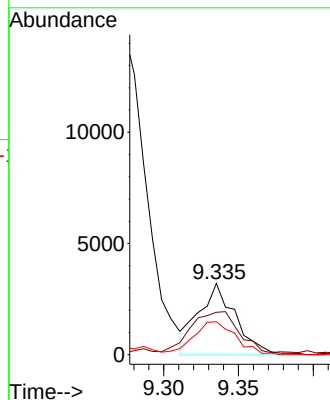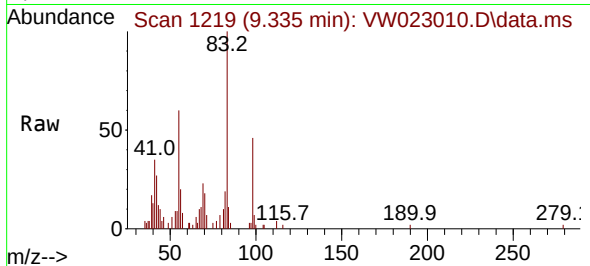

#46
Tetrachloroethene
Concen: 0.978 ug/L
RT: 10.865 min Scan# 1470
Delta R.T. 0.006 min
Lab File: VW023010.D
Acq: 12 May 2022 18:42

Tgt Ion:164 Resp: 3277
Ion Ratio Lower Upper
164 100
129 98.3 76.9 142.7
131 89.3 75.1 139.5
166 110.4 96.0 178.2

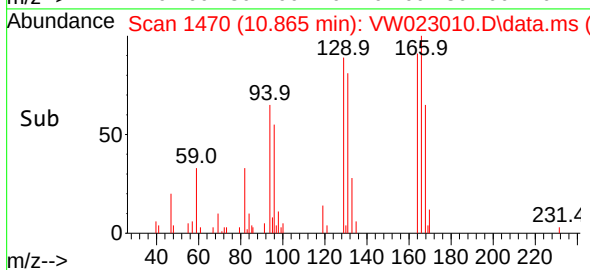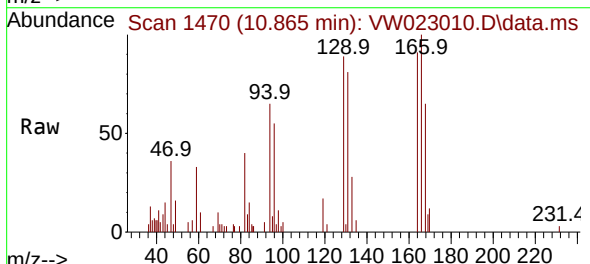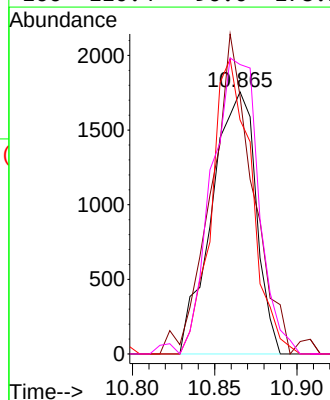

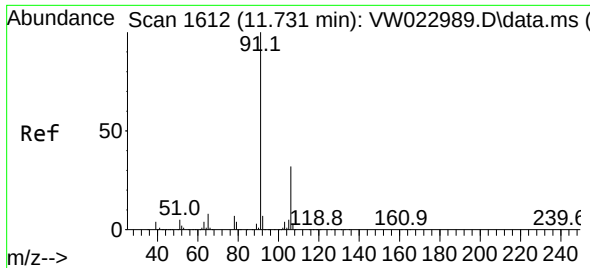





#52
Ethylbenzene
Concen: 20.293 ug/L
RT: 11.731 min Scan# 1612
Delta R.T. -0.000 min
Lab File: VW023010.D
Acq: 12 May 2022 18:42

Instrument :
MSVOA_W
ClientSampleId :
BGPM5

Tgt Ion: 91 Resp: 410297
Ion Ratio Lower Upper
91 100
106 31.1 22.3 41.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

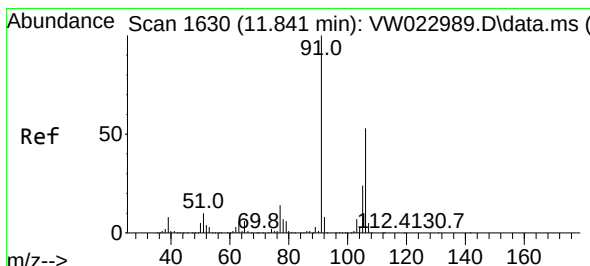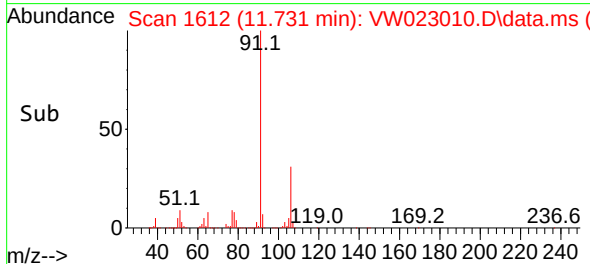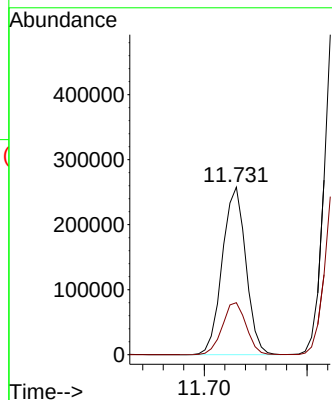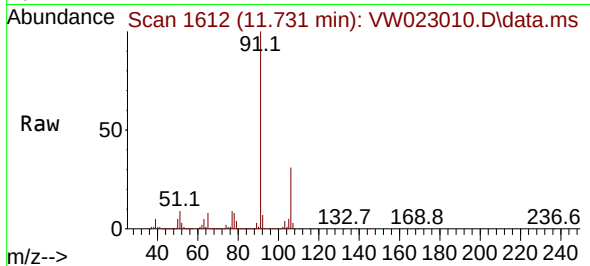

#53
m,p-Xylene
Concen: 85.204 ug/L
RT: 11.835 min Scan# 1629
Delta R.T. -0.006 min
Lab File: VW023010.D
Acq: 12 May 2022 18:42


Tgt Ion:106 Resp: 678790
Ion Ratio Lower Upper
106 100
91 199.7 136.8 254.0

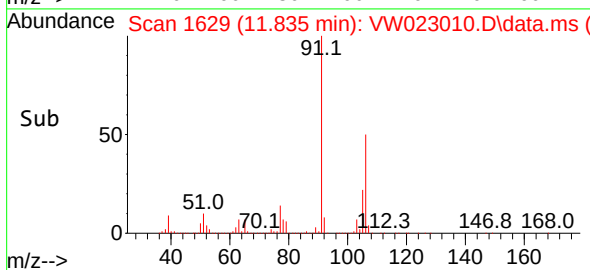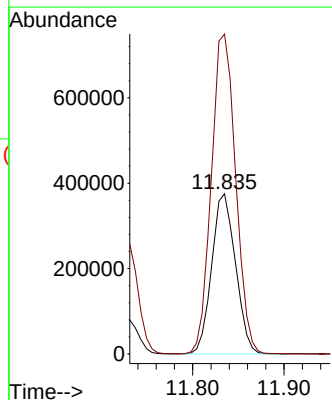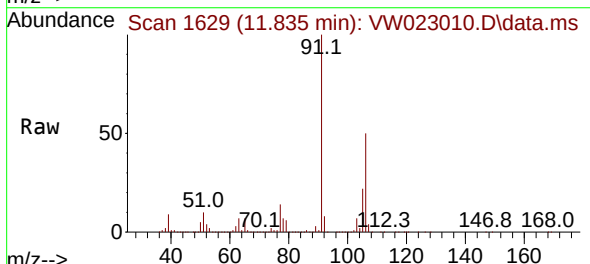

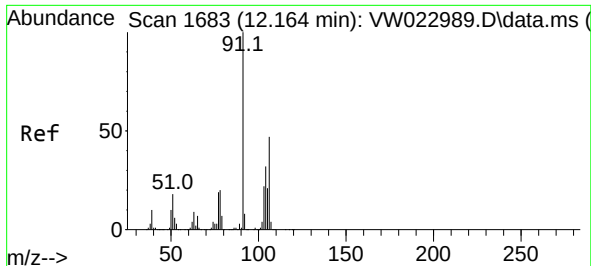

#54
o-Xylene
Concen: 34.479 ug/L
RT: 12.164 min Scan# 1683
Delta R.T. -0.000 min
Lab File: VW023010.D
Acq: 12 May 2022 18:42




Instrument :
MSVOA_W
ClientSampleId :
BGPM5

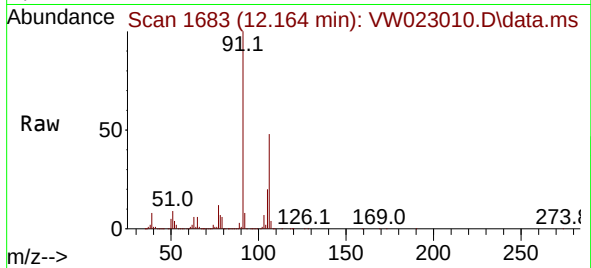


Tgt Ion:106 Resp: 26358
Ion Ratio Lower Upper
106 100
91 207.6 147.2 273.4

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

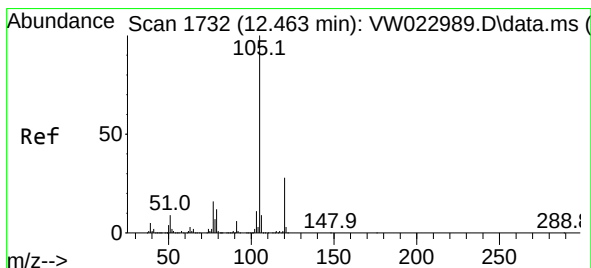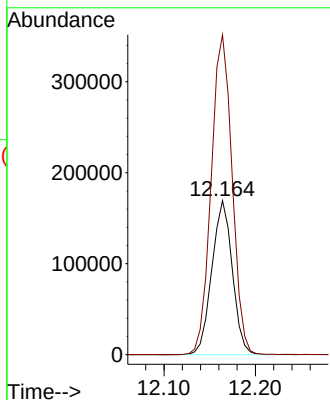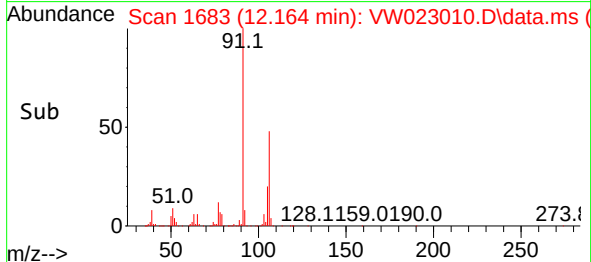

#60
Isopropylbenzene
Concen: 0.439 ug/L
RT: 12.463 min Scan# 1732
Delta R.T. -0.000 min
Lab File: VW023010.D
Acq: 12 May 2022 18:42

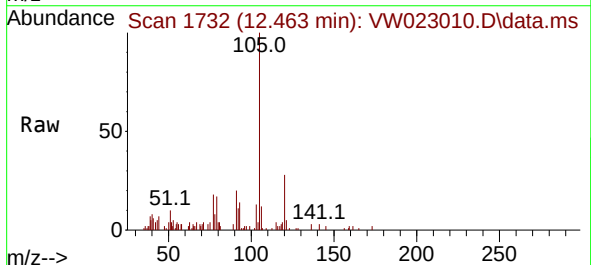

Tgt Ion:105 Resp: 7116
Ion Ratio Lower Upper
105 100
120 25.8 21.3 31.9
77 22.6 12.6 19.0#

