

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051223\
 Data File : VW025969.D
 Acq On : 12 May 2023 17:25
 Operator : SY/MD
 Sample : 02769-07
 Misc : 6.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBW04

Quant Time: May 14 22:50:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun May 14 22:48:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	767601	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	713632	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	319518	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	185836	17.085	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.320%
7) Chloroethane-d5	2.899	69	154250	19.128	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.520%
11) 1,1-Dichloroethene-d2	4.027	65	92493	16.981	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.920%
21) 2-Butanone-d5	7.075	46	226251	62.918	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.840%
24) Chloroform-d	7.648	84	444857	20.098	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.400%
26) 1,2-Dichloroethane-d4	8.300	65	284906	22.763	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.040%
32) Benzene-d6	8.270	84	847420	18.173	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	72.680%
36) 1,2-Dichloropropane-d6	9.270	67	302927	20.304	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.200%
41) Toluene-d8	10.324	98	741583	17.835	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.320%
43) trans-1,3-Dichloroprop...	10.574	79	122543	20.263	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.040%
47) 2-Hexanone-d5	10.922	63	160035	62.905	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.820%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	311668	27.408	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.640%
66) 1,2-Dichlorobenzene-d4	13.848	152	257526	22.110	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.440%
Target Compounds					Qvalue	
13) Acetone	4.118	43	99765	31.289	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051223\
Data File : VW025969.D
Acq On : 12 May 2023 17:25
Operator : SY/MD
Sample : 02769-07
Misc : 6.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBW04

Quant Time: May 14 22:50:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Sun May 14 22:48:01 2023
Response via : Initial Calibration

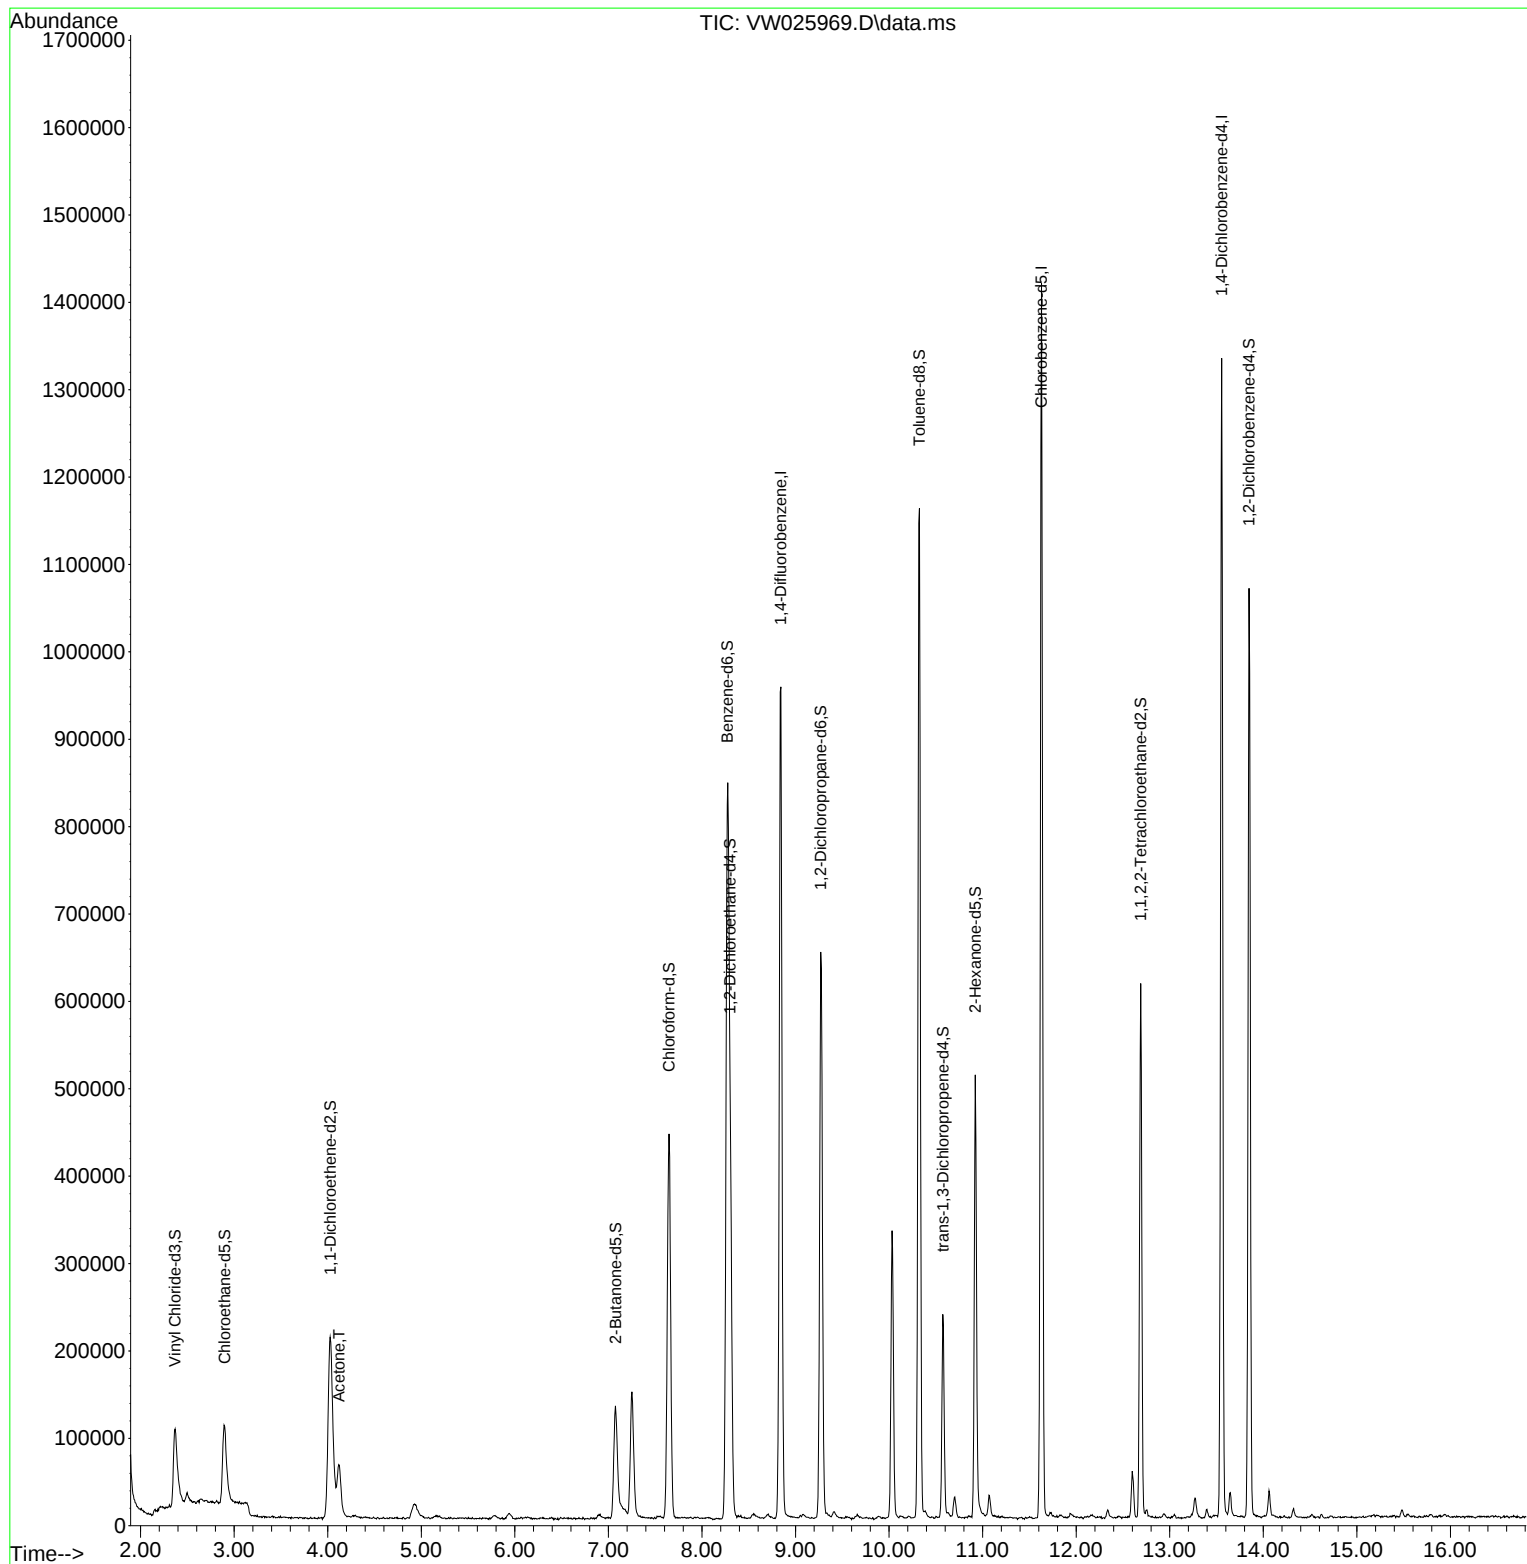

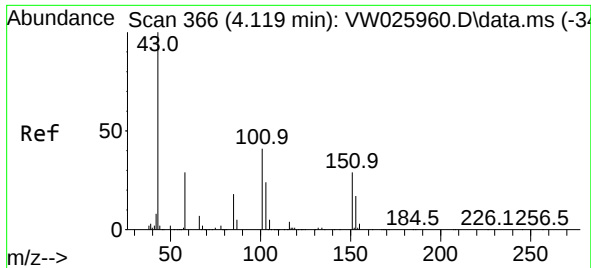

#13
 Acetone
 Concen: 31.289 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW025969.D
 Acq: 12 May 2023 17:25

Instrument :
 MSVOA_W
 ClientSampleId :
 GBW04

Tgt Ion: 43 Resp: 99765
 Ion Ratio Lower Upper
 43 100
 58 29.4 0.0 58.2

