

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051223\
 Data File : VW025968.D
 Acq On : 12 May 2023 17:01
 Operator : SY/MD
 Sample : 02769-06
 Misc : 5.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBW03

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2023
 Supervised By :Mahesh Dadoda 05/15/2023

Quant Time: May 14 22:50:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun May 14 22:48:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	959347	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	877167	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	406153	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	230788	16.976	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	67.920%		
7) Chloroethane-d5	2.893	69	191120	18.963	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.840%		
11) 1,1-Dichloroethene-d2	4.021	65	104311	15.323	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	61.280%		
21) 2-Butanone-d5	7.069	46	275056	61.202	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	122.400%		
24) Chloroform-d	7.648	84	562766	20.344	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	81.360%		
26) 1,2-Dichloroethane-d4	8.307	65	349387m	22.336	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	89.360%		
32) Benzene-d6	8.270	84	1106863	19.312	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	77.240%		
36) 1,2-Dichloropropane-d6	9.270	67	382410	20.853	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	83.400%		
41) Toluene-d8	10.319	98	953382	18.654	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	74.600%		
43) trans-1,3-Dichloroprop...	10.575	79	153589	20.662	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.640%		
47) 2-Hexanone-d5	10.922	63	198951	63.622	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	127.240%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	376144	26.911	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	107.640%		
66) 1,2-Dichlorobenzene-d4	13.849	152	326666	22.063	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	88.240%		
Target Compounds					Qvalue	
13) Acetone	4.119	43	71137	17.851	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051223\
Data File : VW025968.D
Acq On : 12 May 2023 17:01
Operator : SY/MD
Sample : 02769-06
Misc : 5.50g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBW03

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2023
Supervised By : Mahesh Dadoda 05/15/2023

Quant Time: May 14 22:50:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Sun May 14 22:48:01 2023
Response via : Initial Calibration

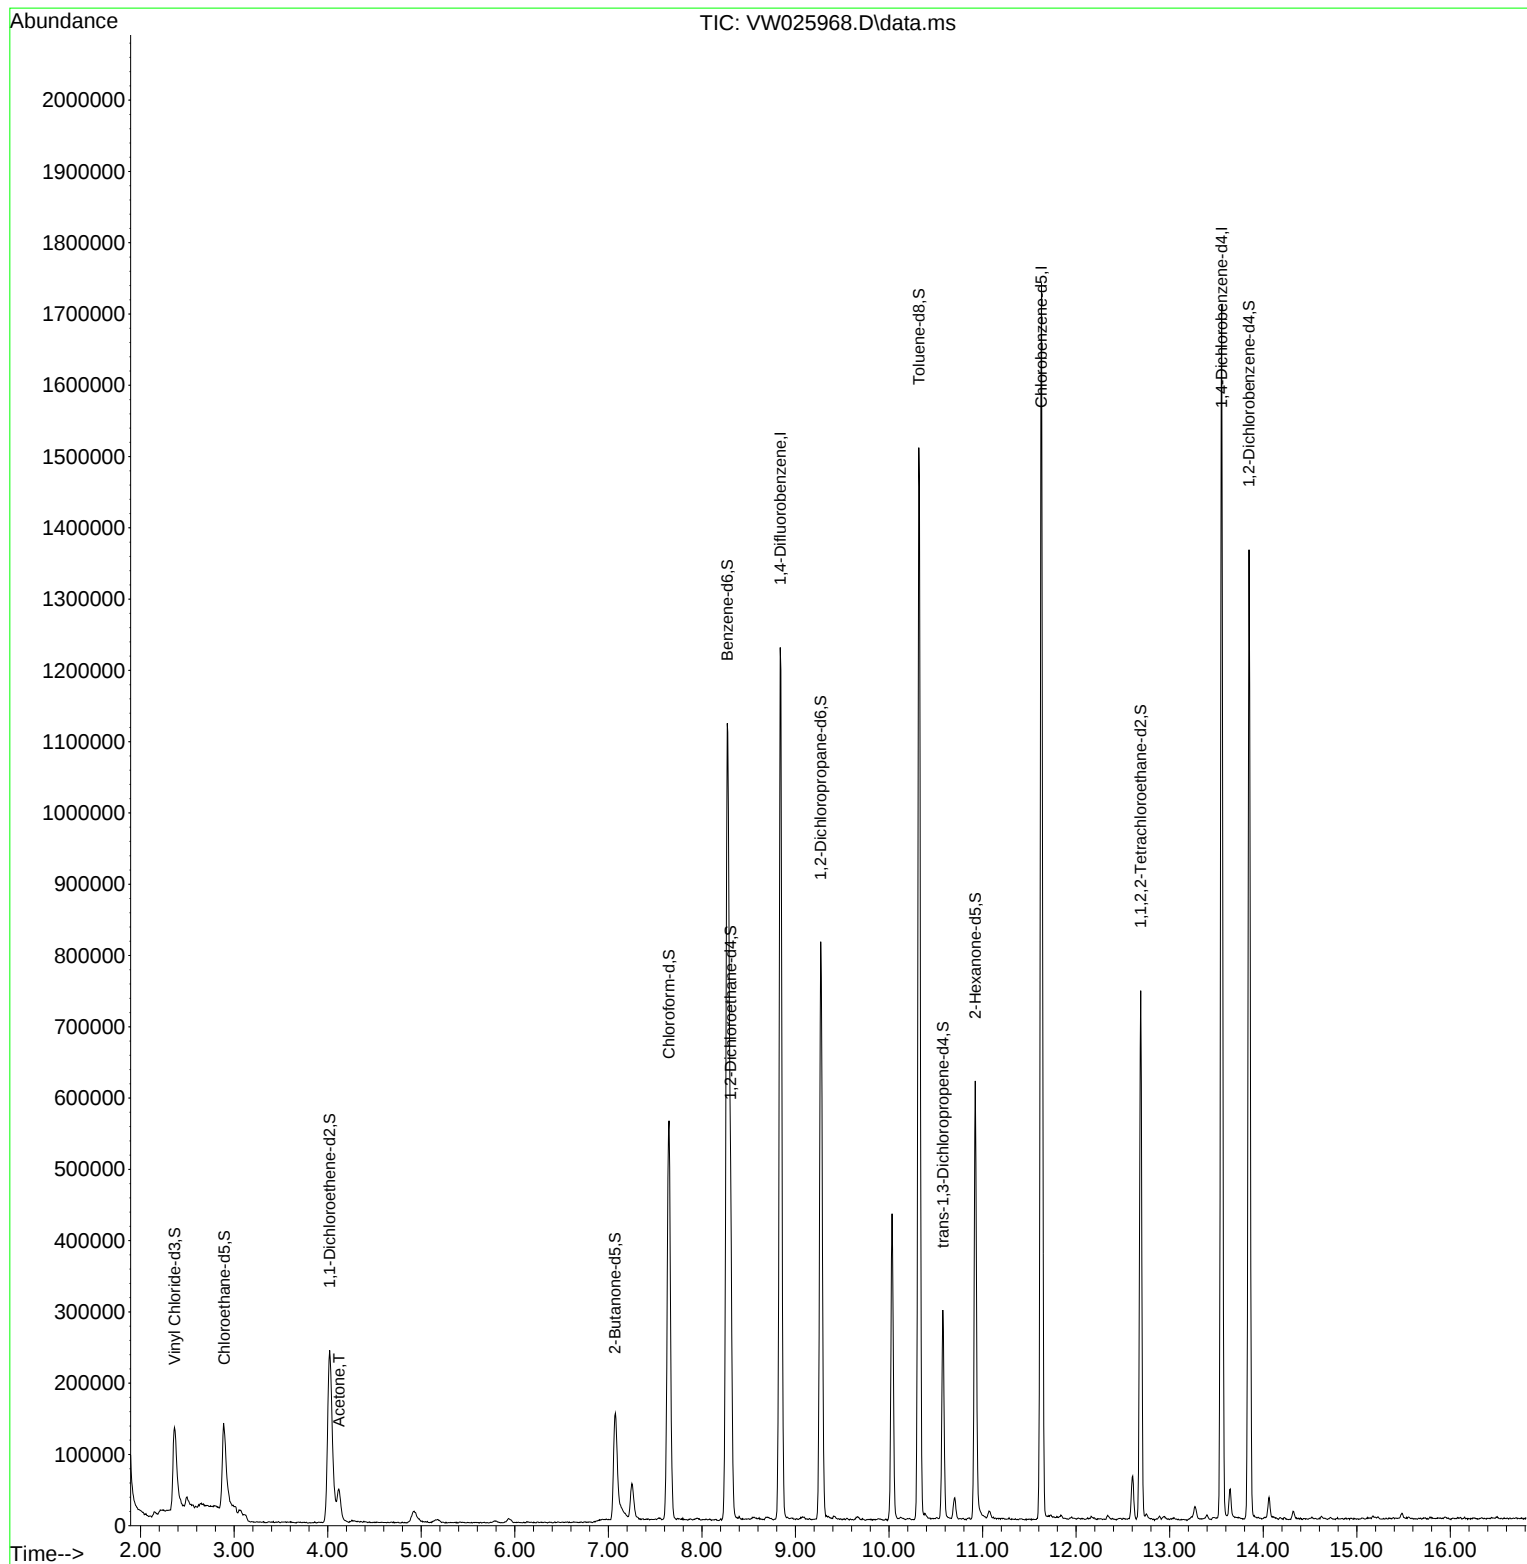

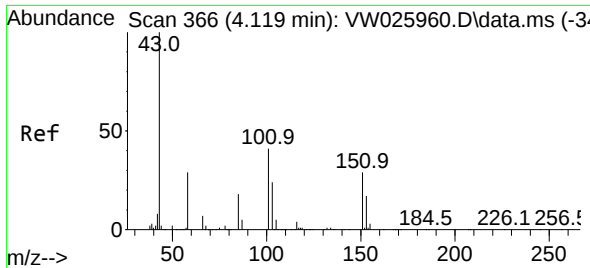

#13
Acetone
Concen: 17.851 ug/L
RT: 4.119 min Scan# 30
Delta R.T. 0.000 min
Lab File: VW025968.D
Acq: 12 May 2023 17:01

Instrument :
MSVOA_W
ClientSampleId :
GBW03

Tgt Ion: 43 Resp: 7113
Ion Ratio Lower Upper
43 100
58 29.2 0.0 58.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2023
Supervised By :Mahesh Dadoda 05/15/2023

