

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051223\
 Data File : VW025972.D
 Acq On : 12 May 2023 18:37
 Operator : SY/MD
 Sample : 02769-10
 Misc : 5.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBW07

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2023
 Supervised By :Mahesh Dadoda 05/15/2023

Quant Time: May 14 22:51:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun May 14 22:48:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	791130	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	737418	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	326498	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	190983	17.036	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	68.160%		
7) Chloroethane-d5	2.893	69	162587	19.562	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.240%		
11) 1,1-Dichloroethene-d2	4.027	65	93865	16.721	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	66.880%		
21) 2-Butanone-d5	7.075	46	298374	80.507	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	161.020%#		
24) Chloroform-d	7.648	84	461764	20.242	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	80.960%		
26) 1,2-Dichloroethane-d4	8.307	65	306982m	23.797	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.200%		
32) Benzene-d6	8.270	84	888732	18.444	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	73.760%		
36) 1,2-Dichloropropane-d6	9.276	67	316295	20.516	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	82.080%		
41) Toluene-d8	10.325	98	772938	17.989	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	71.960%		
43) trans-1,3-Dichloroprop...	10.575	79	129946	20.794	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.160%		
47) 2-Hexanone-d5	10.922	63	196527	74.757	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	149.520%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	369404	31.437	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	125.760%#		
66) 1,2-Dichlorobenzene-d4	13.848	152	271033	22.772	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.080%		
Target Compounds					Qvalue	
13) Acetone	4.118	43	97030	29.526	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051223\
Data File : VW025972.D
Acq On : 12 May 2023 18:37
Operator : SY/MD
Sample : 02769-10
Misc : 5.33g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBW07

Quant Time: May 14 22:51:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Sun May 14 22:48:01 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2023
Supervised By : Mahesh Dadoda 05/15/2023

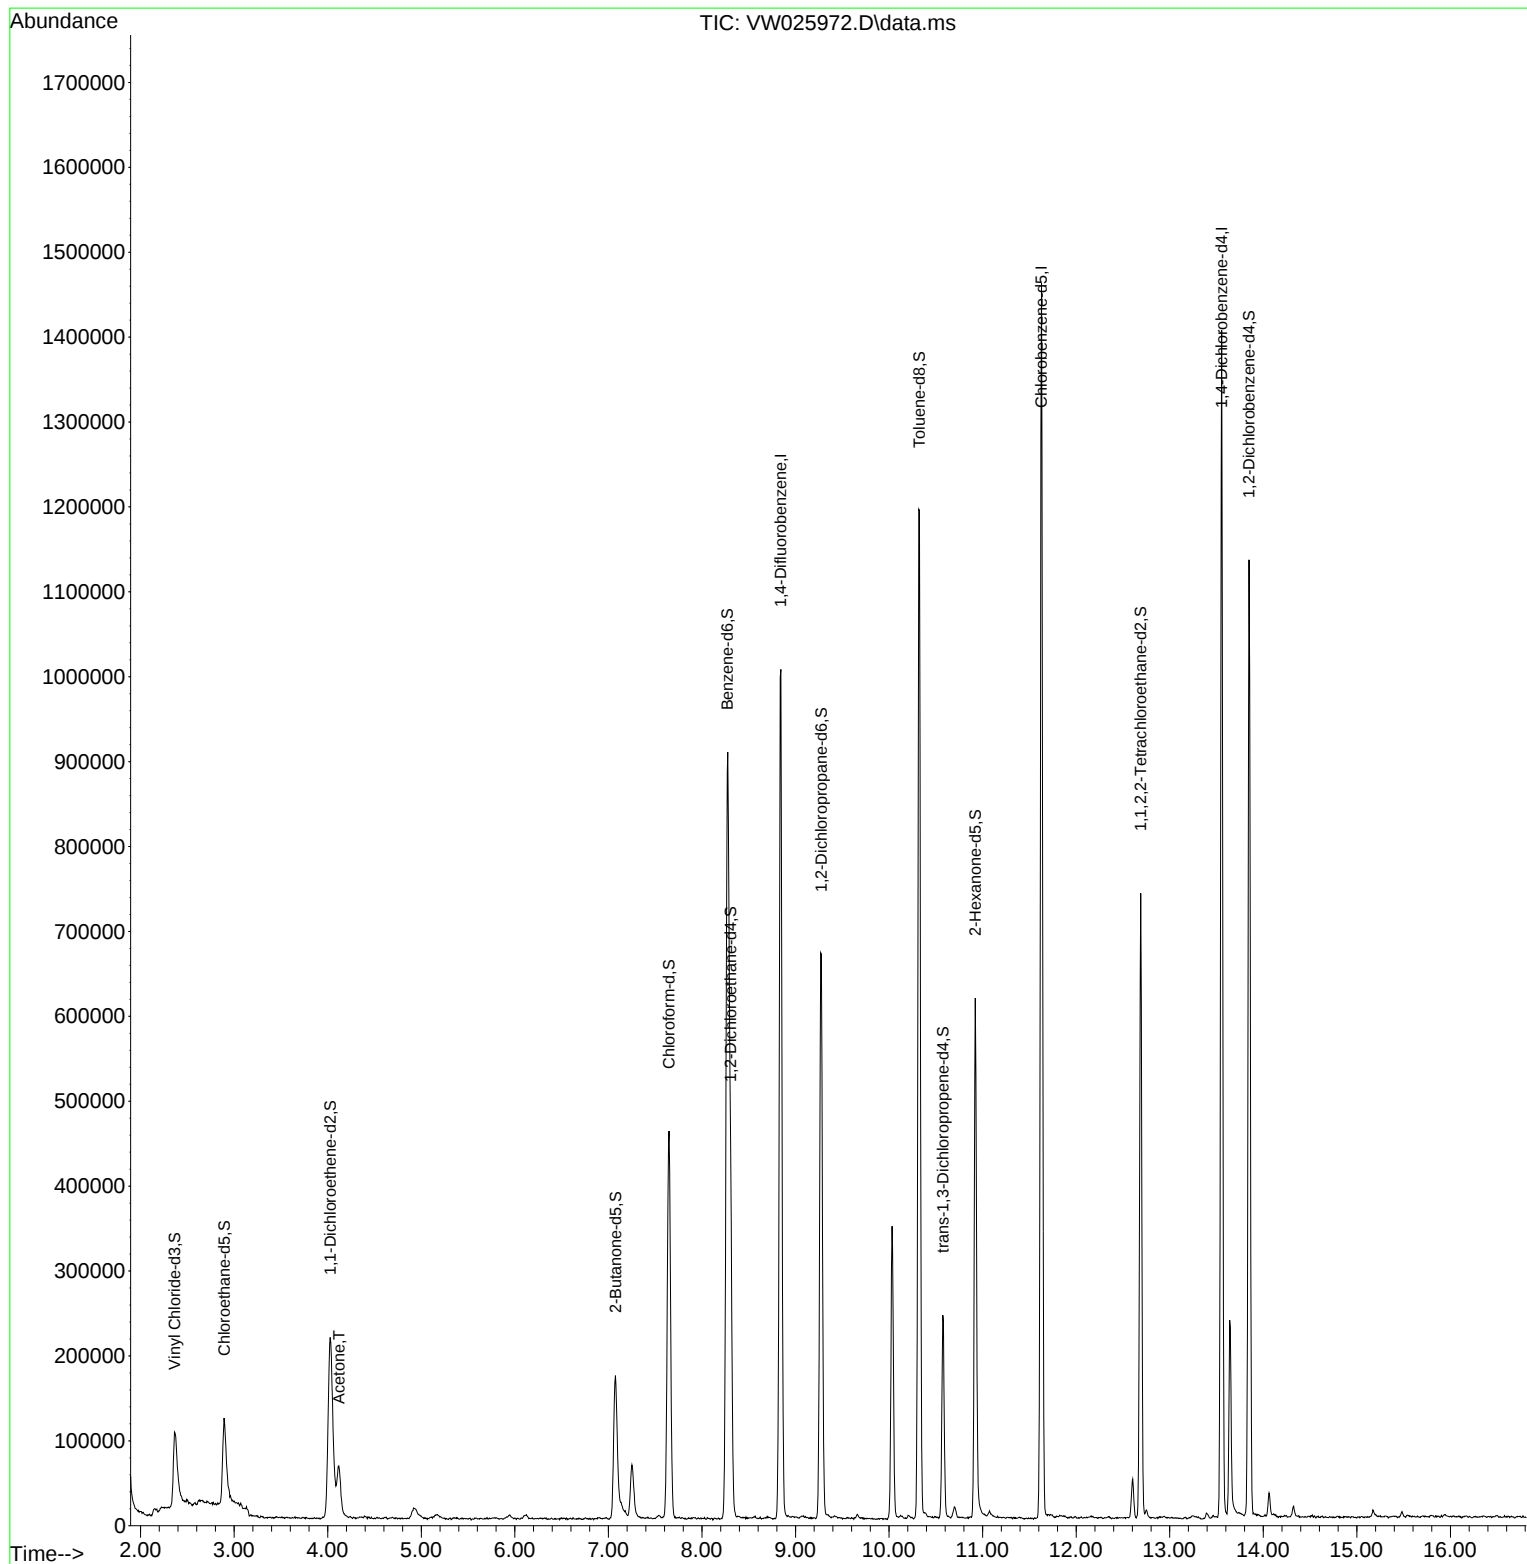

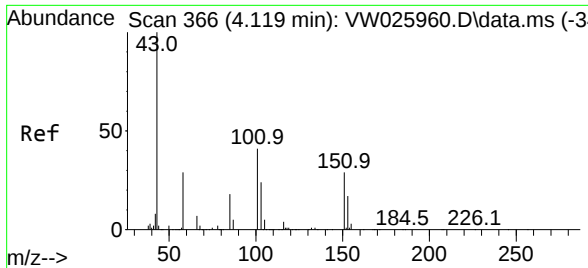

#13
 Acetone
 Concen: 29.526 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW025972.D
 Acq: 12 May 2023 18:37

Instrument :
 MSVOA_W
 ClientSampleId :
 GBW07

Tgt Ion: 43 Resp: 97030
 Ion Ratio Lower Upper
 43 100
 58 30.0 0.0 58.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2023
 Supervised By :Mahesh Dadoda 05/15/2023

