

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
 Data File : VW023016.D
 Acq On : 13 May 2022 10:44
 Operator : SY/VA
 Sample : N2746-07
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: May 13 23:58:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 23:57:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	334479	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	325564	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	164321	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	167988	24.480	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.920%
7) Chloroethane-d5	2.885	69	124556	27.899	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.600%
11) 1,1-Dichloroethene-d2	4.013	63	169039	19.064	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.240%
21) 2-Butanone-d5	7.080	46	58176	44.588	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.180%
24) Chloroform-d	7.647	84	246837	25.189	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.760%
26) 1,2-Dichloroethane-d4	8.305	65	141107	26.254	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.000%
32) Benzene-d6	8.275	84	508811	27.114	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.440%
36) 1,2-Dichloropropane-d6	9.274	67	140306	26.617	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.480%
41) Toluene-d8	10.323	98	488987	26.975	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	107.920%
43) trans-1,3-Dichloroprop...	10.579	79	59907	24.683	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.720%
47) 2-Hexanone-d5	10.920	63	48754	48.450	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.900%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	117936	24.004	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.000%
66) 1,2-Dichlorobenzene-d4	13.853	152	161435	28.104	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	112.400%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	5517	0.767	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
Data File : VW023016.D
Acq On : 13 May 2022 10:44
Operator : SY/VA
Sample : N2746-07
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: May 13 23:58:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 23:57:51 2022
Response via : Initial Calibration

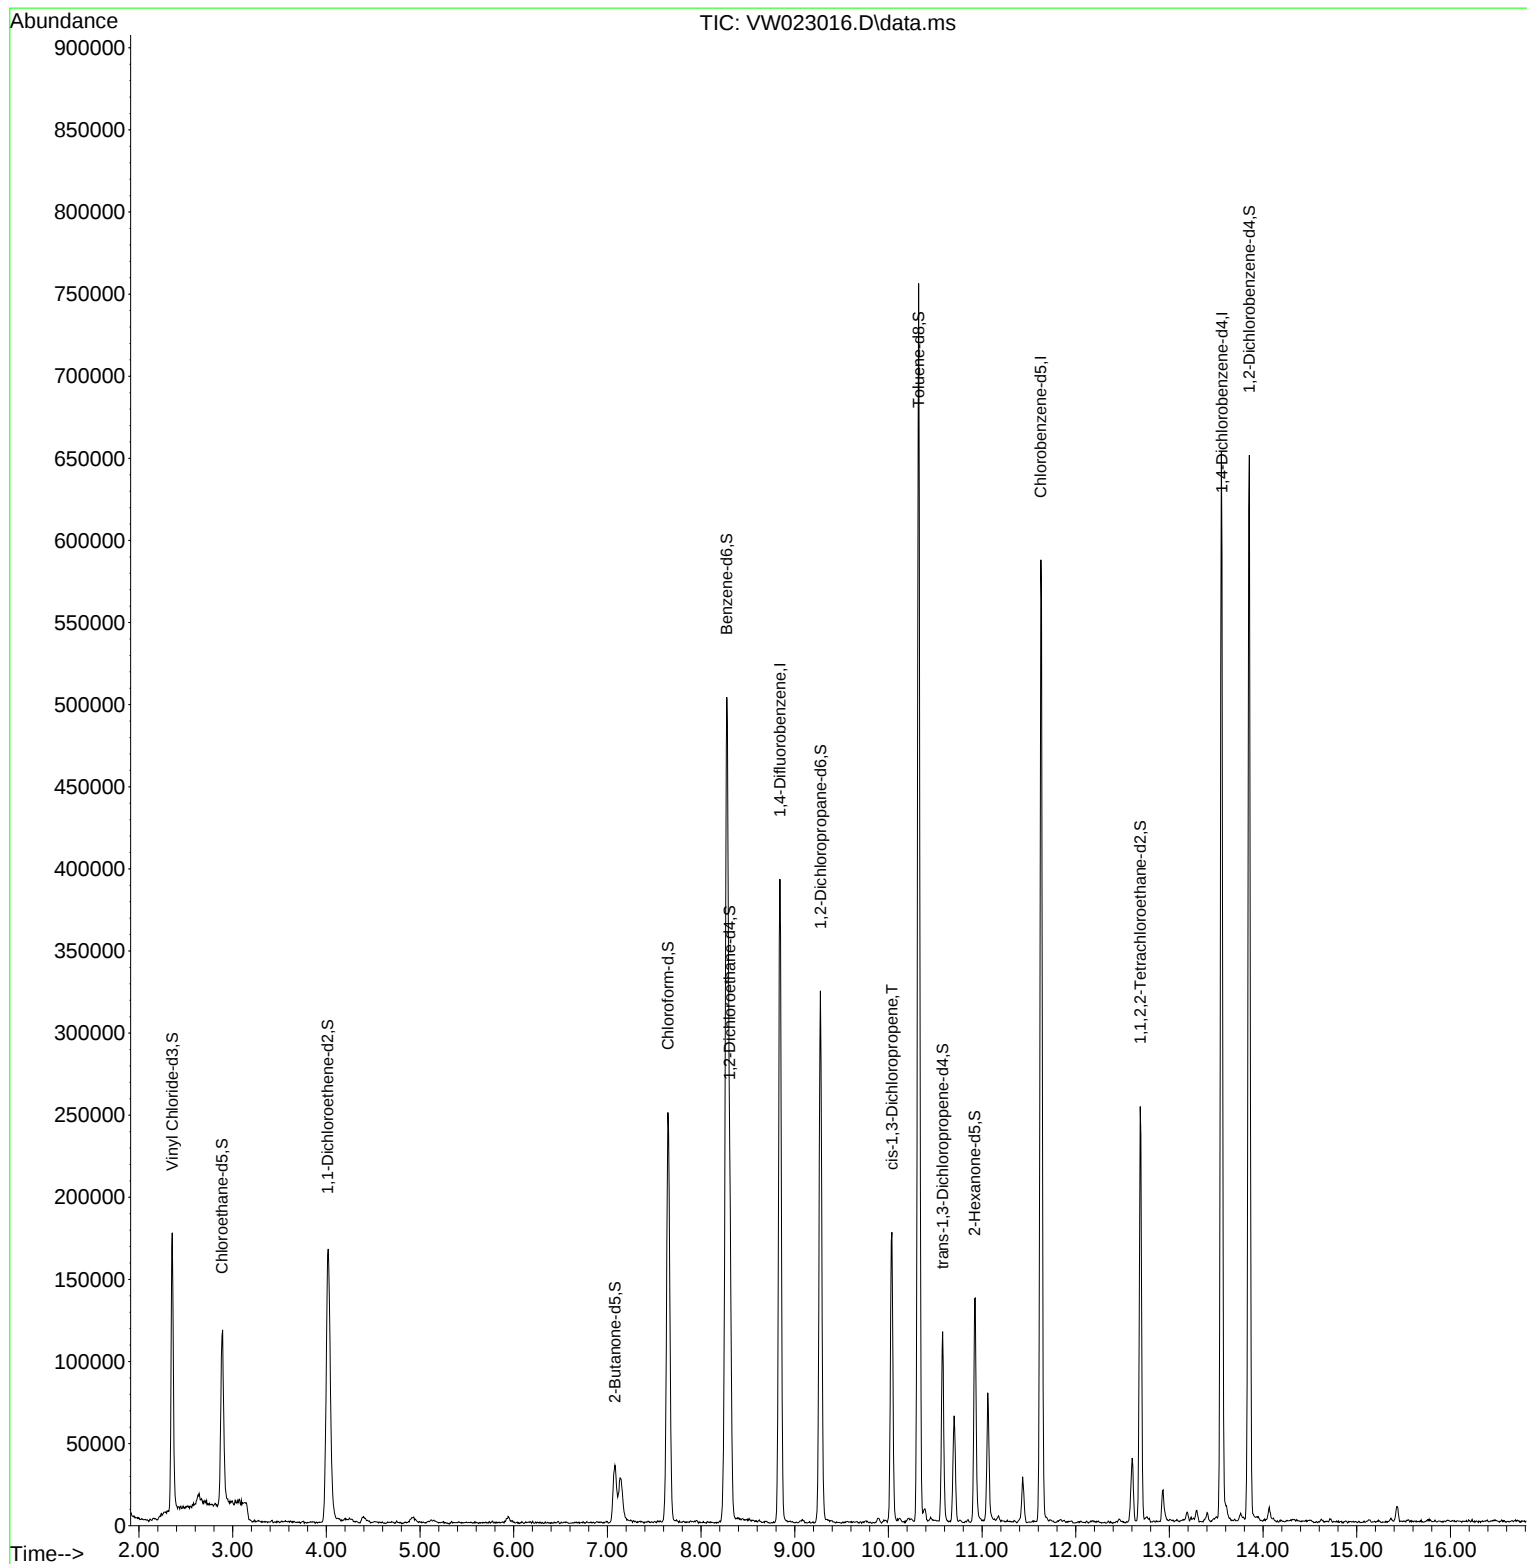

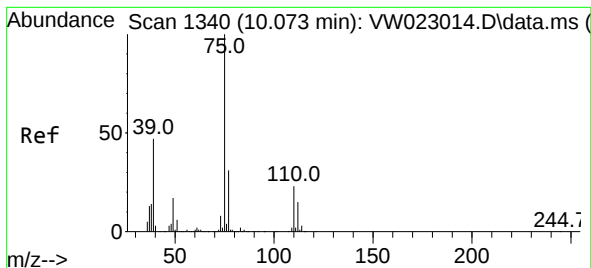

#39
 cis-1,3-Dichloropropene
 Concen: 0.767 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023016.D
 Acq: 13 May 2022 10:44

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 5517
 Ion Ratio Lower Upper
 75 100
 77 30.6 22.1 41.1

