

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
 Data File : VW023031.D
 Acq On : 13 May 2022 16:46
 Operator : SY/VA
 Sample : N2821-12
 Misc : 4.81g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLD2

Quant Time: May 14 00:01:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 23:57:51 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	350987	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	291531	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	102472	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	192762	26.769	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.080%	
7) Chloroethane-d5		2.885	69	143234	30.574	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	122.280%	
11) 1,1-Dichloroethene-d2		4.013	63	162948	17.513	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.040%	
21) 2-Butanone-d5		7.074	46	16323	11.922	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	23.840%	
24) Chloroform-d		7.647	84	280354	27.264	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	109.040%	
26) 1,2-Dichloroethane-d4		8.305	65	164666	29.197	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	116.800%	
32) Benzene-d6		8.275	84	520817	30.994	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	123.960%	
36) 1,2-Dichloropropane-d6		9.274	67	161125	34.135	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	136.560%#	
41) Toluene-d8		10.323	98	443684	27.333	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	109.320%	
43) trans-1,3-Dichloroprop...		10.579	79	46886	21.573	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.280%	
47) 2-Hexanone-d5		10.927	63	12722	14.119	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	28.240%	
56) 1,1,2,2-Tetrachloroeth...		12.689	84	129399	29.412	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	117.640%	
66) 1,2-Dichlorobenzene-d4		13.847	152	97690	27.272	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.080%	
Target Compounds							
39) cis-1,3-Dichloropropene		10.037	75	3908	0.606	ug/L	Qvalue # 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
Data File : VW023031.D
Acq On : 13 May 2022 16:46
Operator : SY/VA
Sample : N2821-12
Misc : 4.81g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXLD2

Quant Time: May 14 00:01:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 23:57:51 2022
Response via : Initial Calibration

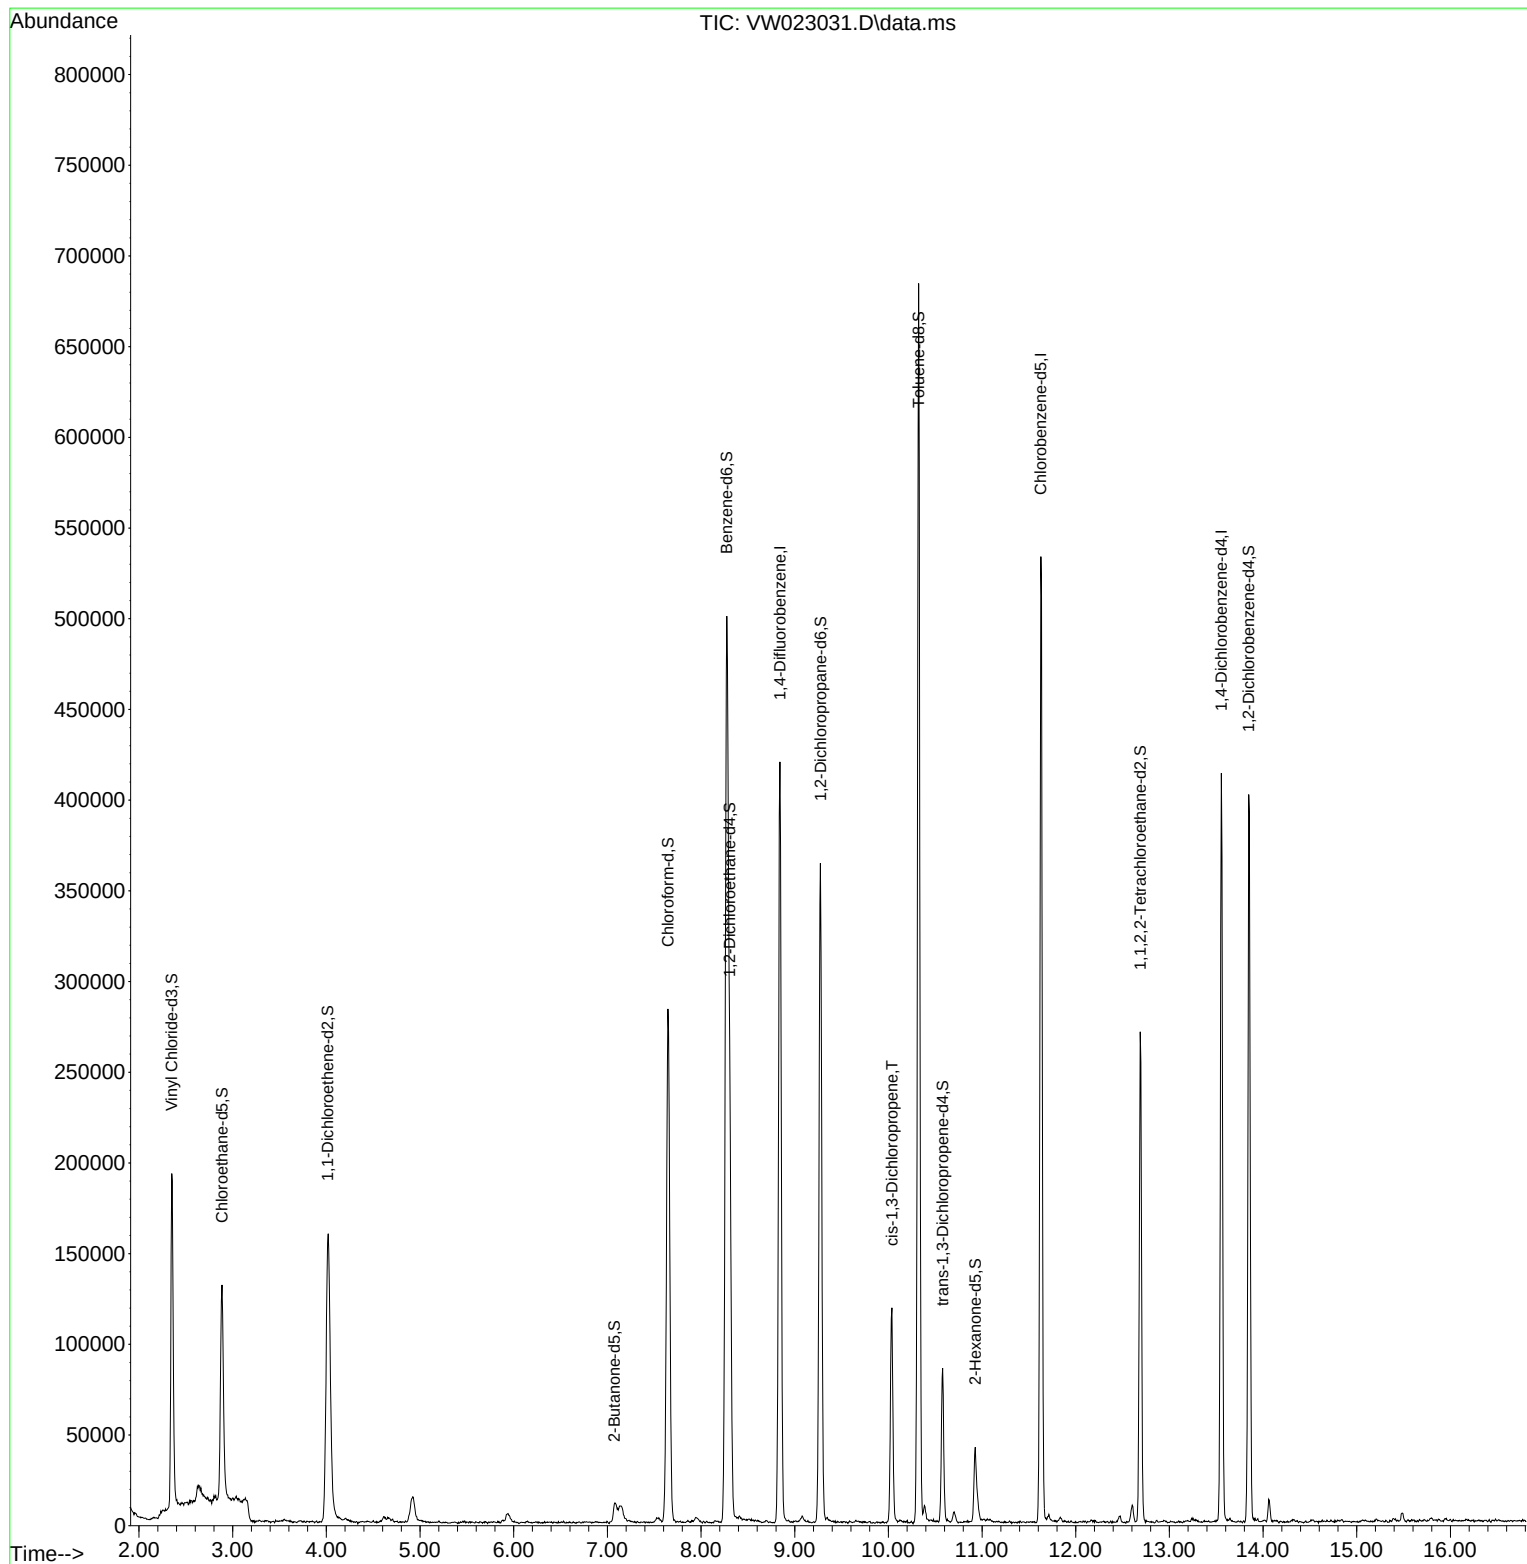

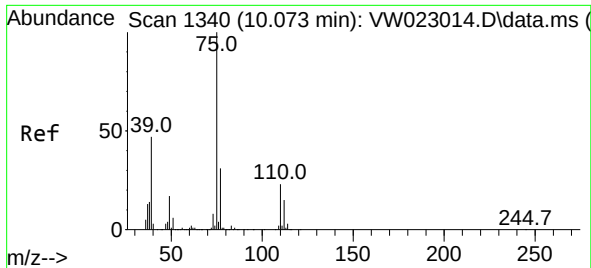

#39
 cis-1,3-Dichloropropene
 Concen: 0.606 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW023031.D
 Acq: 13 May 2022 16:46

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLD2

Tgt Ion: 75 Resp: 3908
 Ion Ratio Lower Upper
 75 100
 77 44.1 22.1 41.1#

