




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
 Data File : VW023022.D
 Acq On : 13 May 2022 13:08
 Operator : SY/VA
 Sample : N2821-03
 Misc : 4.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLC2

Manual IntegrationsAPPROVED

Quant Time: May 14 00:00:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 23:57:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

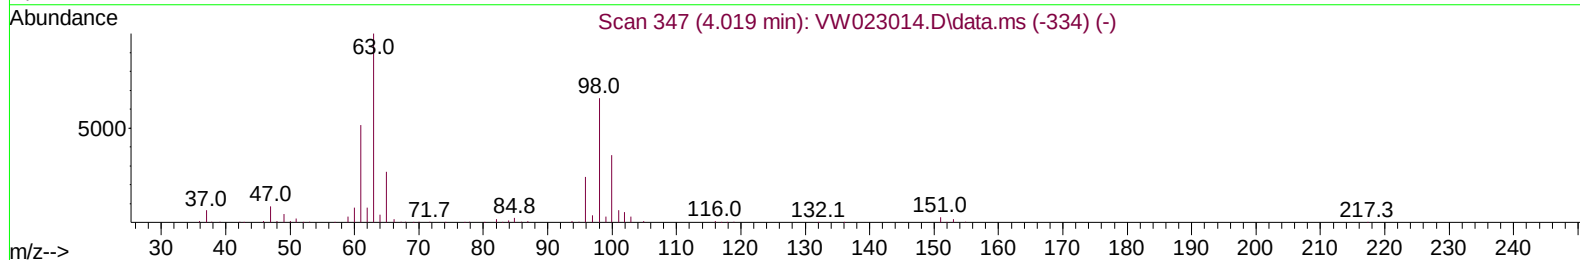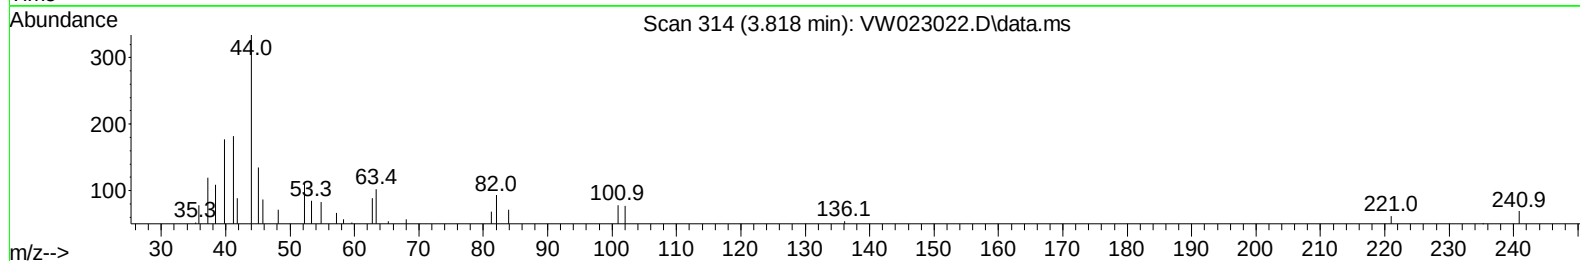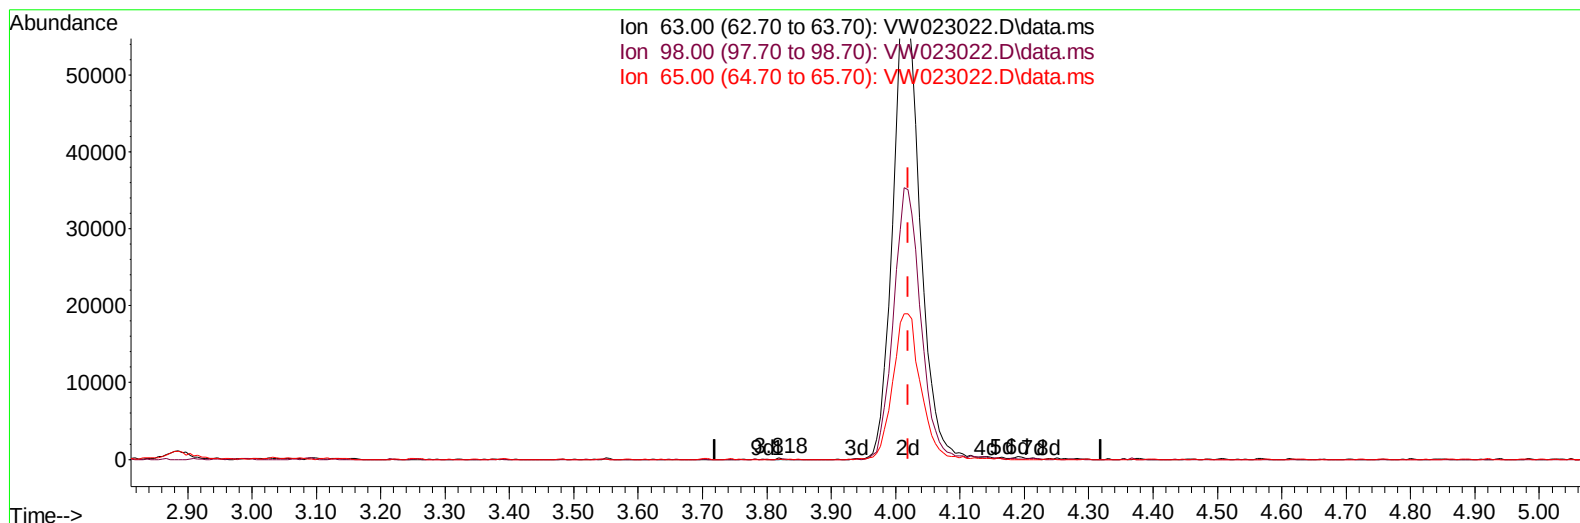

TIC: VW023022.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.818min (-0.201) 0.01 ug/L

response	94	
Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	55.32
65.00	23.30	20.21
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
Data File : VW023022.D
Acq On : 13 May 2022 13:08
Operator : SY/VA
Sample : N2821-03
Misc : 4.77g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXLC2

Manual IntegrationsAPPROVED

Quant Time: May 14 00:00:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 23:57:51 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

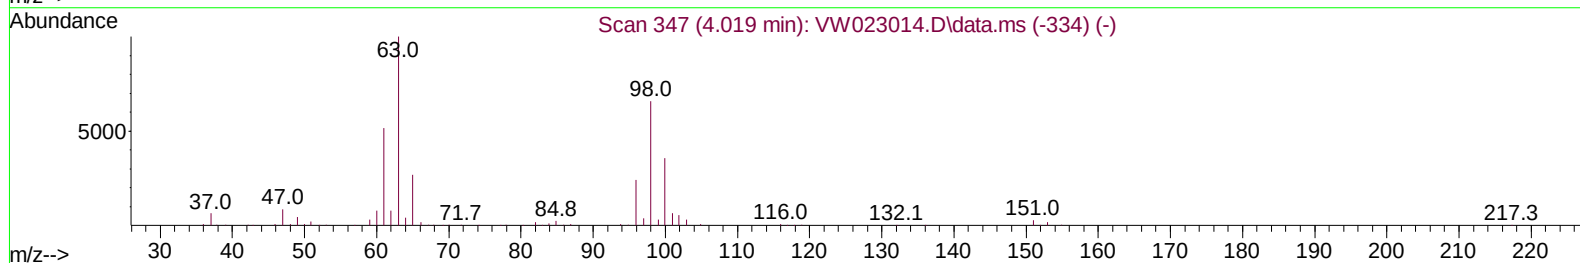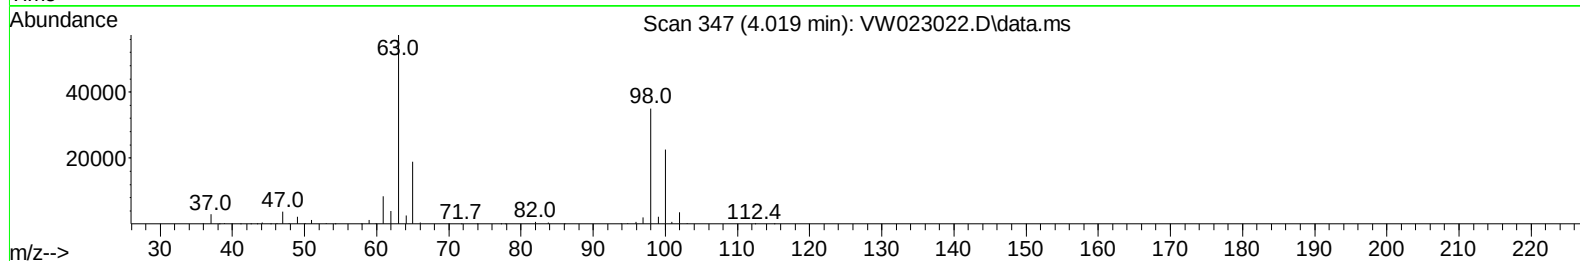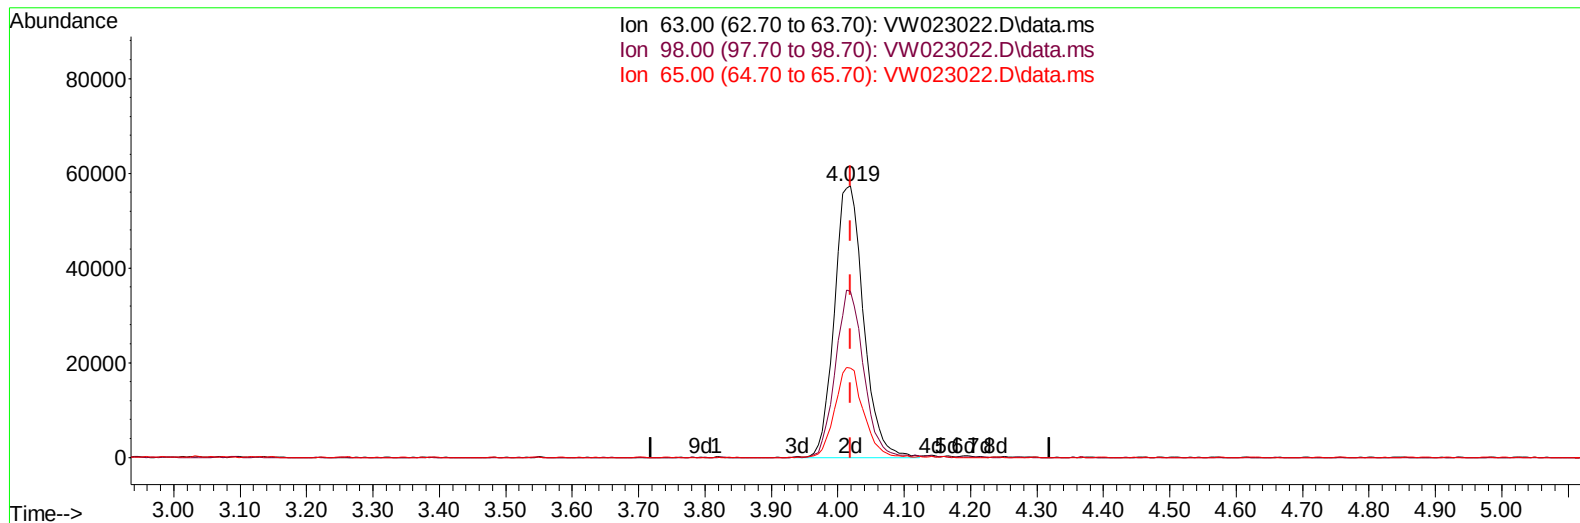

TIC: VW023022.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.000) 18.12 ug/L m

response 174866

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.03#
65.00	23.30	0.01#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
 Data File : VW023022.D
 Acq On : 13 May 2022 13:08
 Operator : SY/VA
 Sample : N2821-03
 Misc : 4.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLC2

Manual IntegrationsAPPROVED

Quant Time: May 14 00:00:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 23:57:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

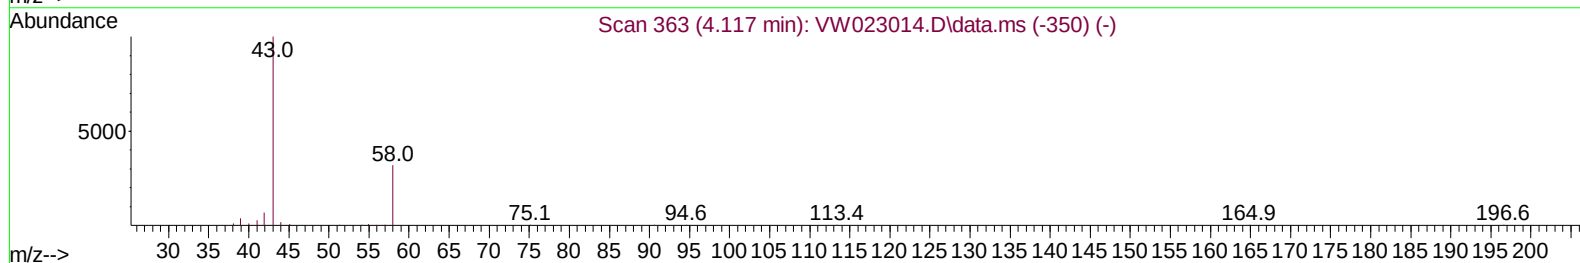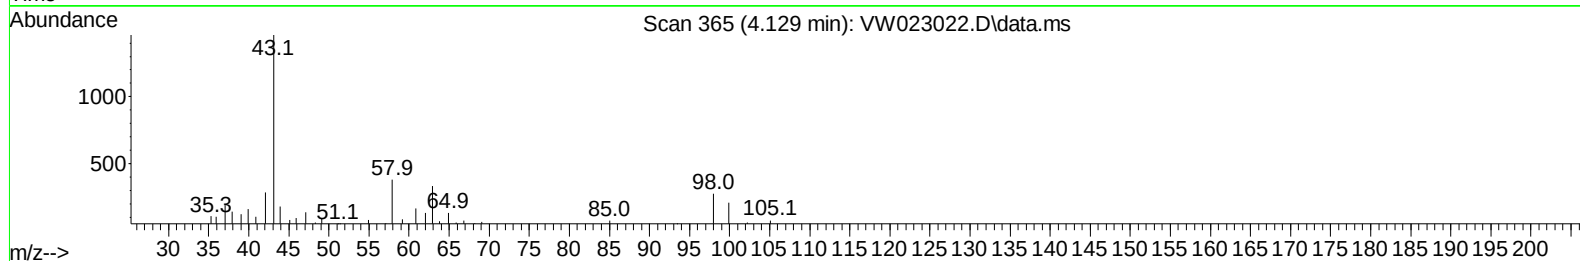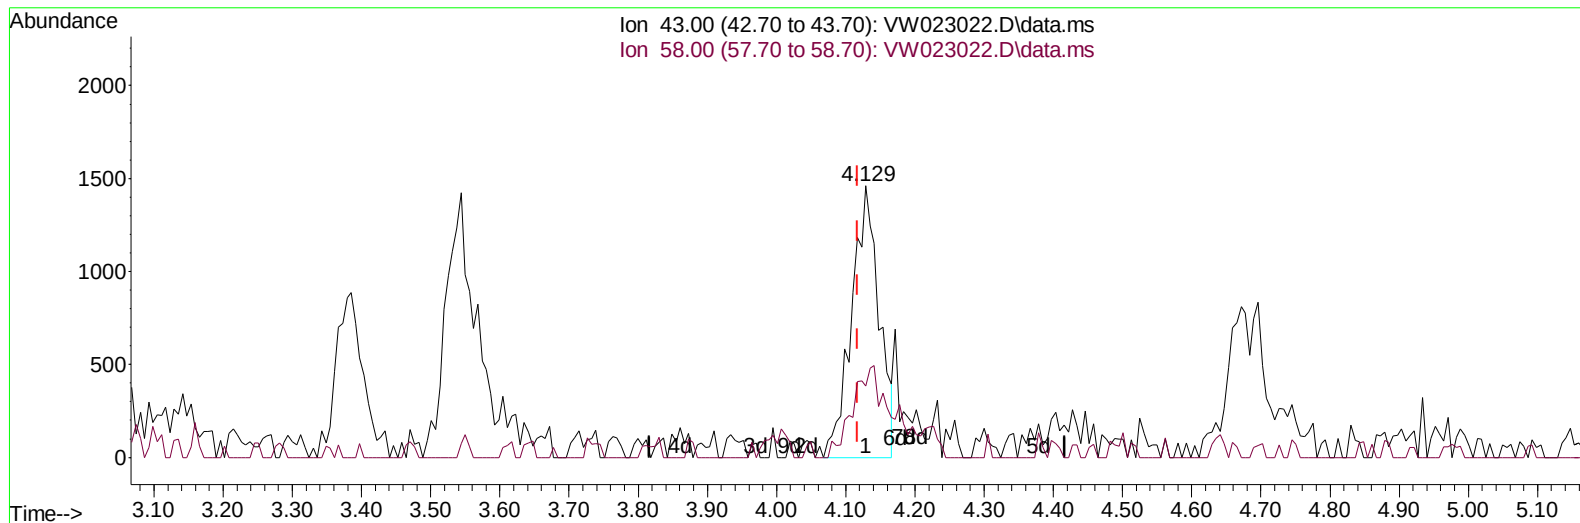

TIC: VW023022.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 3.79 ug/L

response 4027

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	10.93
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
 Data File : VW023022.D
 Acq On : 13 May 2022 13:08
 Operator : SY/VA
 Sample : N2821-03
 Misc : 4.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLC2

Manual IntegrationsAPPROVED

Quant Time: May 14 00:00:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 23:57:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	364016	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	288012	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93304	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	200913	26.902	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	107.600%	
7) Chloroethane-d5	2.885	69	145919	30.032	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	120.120%	
11) 1,1-Dichloroethene-d2	4.019	63	174866m	18.121	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	72.480%	
21) 2-Butanone-d5	7.080	46	38933	27.418	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	54.840%	
24) Chloroform-d	7.647	84	292623	27.438	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	109.760%	
26) 1,2-Dichloroethane-d4	8.305	65	169713	29.015	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	116.040%	
32) Benzene-d6	8.275	84	559462	33.701	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	134.800%	
36) 1,2-Dichloropropane-d6	9.274	67	169835	36.420	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	145.680%#	
41) Toluene-d8	10.323	98	471608	29.408	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	117.640%	
43) trans-1,3-Dichloroprop...	10.579	79	43029	20.040	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	80.160%	
47) 2-Hexanone-d5	10.927	63	27803	31.232	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	62.460%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	123432	28.398	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	113.600%	
66) 1,2-Dichlorobenzene-d4	13.847	152	90837	27.850	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	111.400%	
Target Compounds						
13) Acetone	4.129	43	4027	3.788	ug/L	Qvalue 62

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
Data File : VW023022.D
Acq On : 13 May 2022 13:08
Operator : SY/VA
Sample : N2821-03
Misc : 4.77g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXLC2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 14 00:00:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 23:57:51 2022
Response via : Initial Calibration

