

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
 Data File : VW023022.D
 Acq On : 13 May 2022 13:08
 Operator : SY/VA
 Sample : N2821-03
 Misc : 4.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLC2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 14 00:00:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 23:57:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	364016	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	288012	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93304	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	200913	26.902	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.600%
7) Chloroethane-d5	2.885	69	145919	30.032	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	120.120%
11) 1,1-Dichloroethene-d2	4.019	63	174866m	18.121	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.480%
21) 2-Butanone-d5	7.080	46	38933	27.418	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.840%
24) Chloroform-d	7.647	84	292623	27.438	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	109.760%
26) 1,2-Dichloroethane-d4	8.305	65	169713	29.015	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	116.040%
32) Benzene-d6	8.275	84	559462	33.701	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	134.800%
36) 1,2-Dichloropropane-d6	9.274	67	169835	36.420	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	145.680%#
41) Toluene-d8	10.323	98	471608	29.408	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	117.640%
43) trans-1,3-Dichloroprop...	10.579	79	43029	20.040	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.160%
47) 2-Hexanone-d5	10.927	63	27803	31.232	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.460%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	123432	28.398	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.600%
66) 1,2-Dichlorobenzene-d4	13.847	152	90837	27.850	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.400%
Target Compounds					Qvalue	
13) Acetone	4.129	43	4027	3.788	ug/L	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
Data File : VW023022.D
Acq On : 13 May 2022 13:08
Operator : SY/VA
Sample : N2821-03
Misc : 4.77g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EXLC2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 14 00:00:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 23:57:51 2022
Response via : Initial Calibration

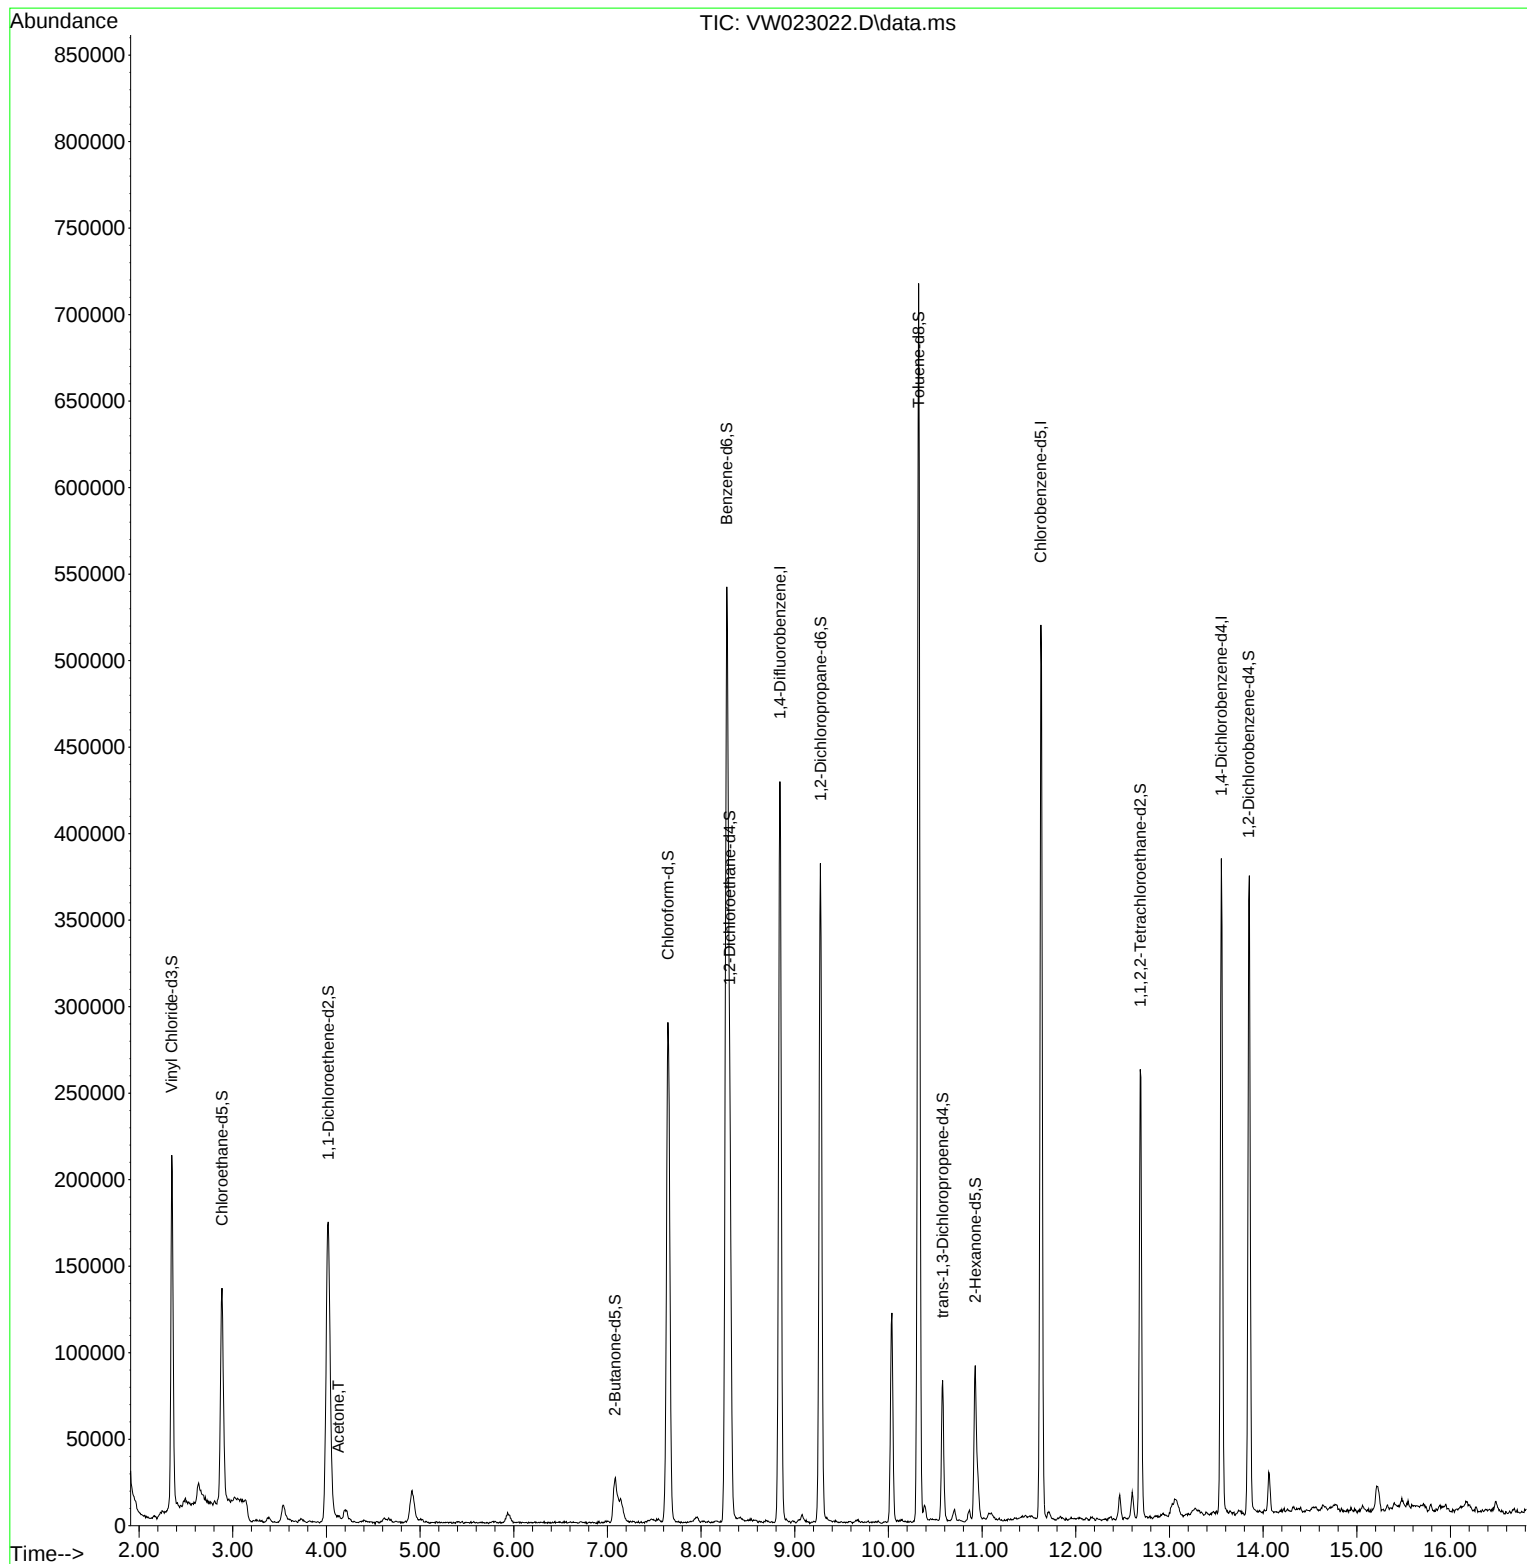

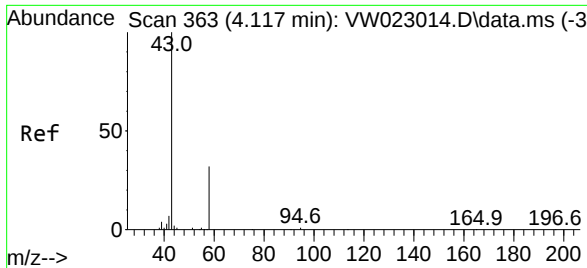

#13

Acetone

Concen: 3.788 ug/L

RT: 4.129 min Scan# 30

Delta R.T. 0.012 min

Lab File: VW023022.D


Acq: 13 May 2022 13:08

Instrument :

MSVOA_W

ClientSampleId :

EXLC2

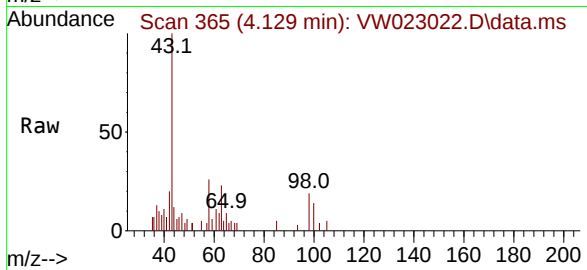

Tgt Ion: 43 Resp: 402

Ion Ratio Lower Upper

43 100

58 10.9 0.0 64.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022

Supervised By :Mahesh Dadoda 05/16/2022

