

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
 Data File : VW023026.D
 Acq On : 13 May 2022 14:45
 Operator : SY/VA
 Sample : N2821-07
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLC7

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2022
 Supervised By : Mahesh Dadoda 05/16/2022

Quant Time: May 14 00:00:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 23:57:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	417733	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	370023	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	142938	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	216151	25.221	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 100.880%			
7) Chloroethane-d5	2.885	69	166634	29.886	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 119.560%			
11) 1,1-Dichloroethene-d2	4.013	63	198470	17.922	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 71.680%			
21) 2-Butanone-d5	7.080	46	36783	22.573	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 45.140%			
24) Chloroform-d	7.647	84	313409	25.608	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 102.440%			
26) 1,2-Dichloroethane-d4	8.305	65	182734m	27.223	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 108.880%			
32) Benzene-d6	8.275	84	613048	28.744	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 114.960%			
36) 1,2-Dichloropropane-d6	9.274	67	180403	30.112	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 120.440%#			
41) Toluene-d8	10.323	98	555332	26.954	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 107.800%			
43) trans-1,3-Dichloroprop...	10.573	79	61116	22.155	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 88.640%			
47) 2-Hexanone-d5	10.921	63	32066	28.037	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 56.080%			
56) 1,1,2,2-Tetrachloroeth...	12.689	84	151674	27.162	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 108.640%			
66) 1,2-Dichlorobenzene-d4	13.853	152	136330	27.284	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 109.120%			
Target Compounds					Qvalue	
13) Acetone	4.123	43	4011	3.288	ug/L	59

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
Data File : VW023026.D
Acq On : 13 May 2022 14:45
Operator : SY/VA
Sample : N2821-07
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EXLC7

Quant Time: May 14 00:00:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 23:57:51 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 05/15/2022
Supervised By : Mahesh Dadoda 05/16/2022

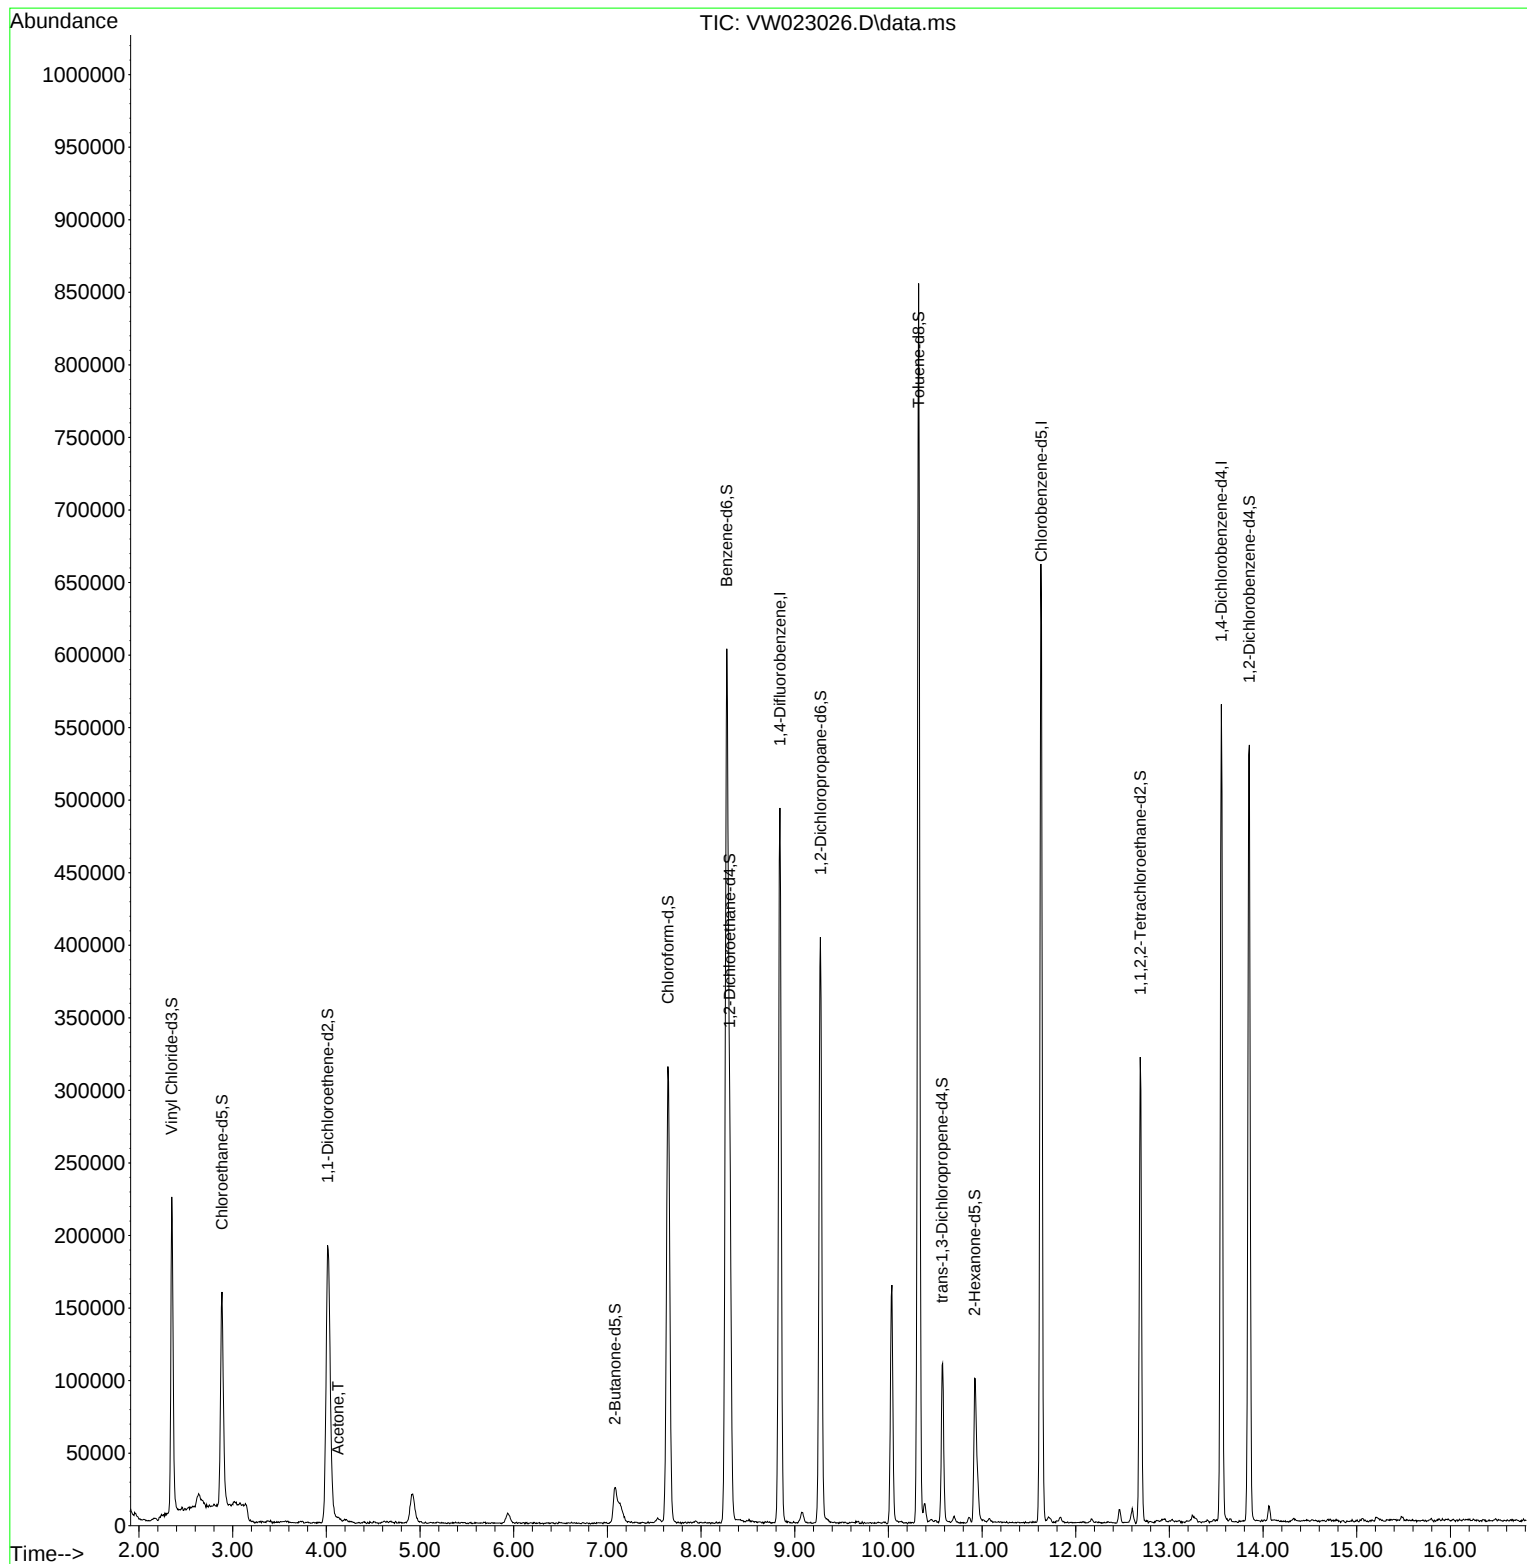

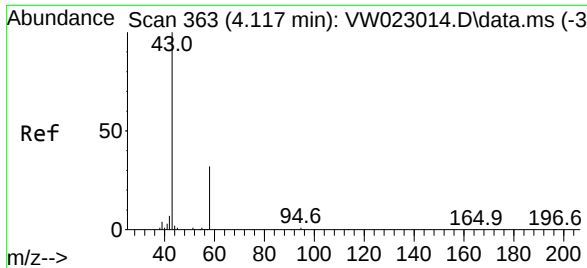

#13
 Acetone
 Concen: 3.288 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW023026.D
 Acq: 13 May 2022 14:45

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLC7

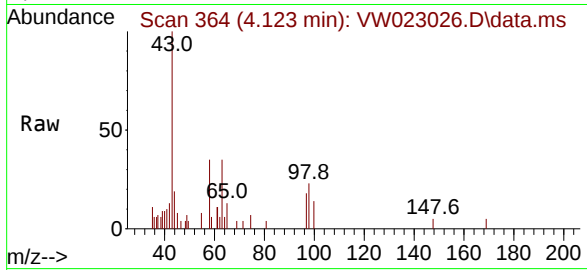

Tgt Ion: 43 Resp: 401
 Ion Ratio Lower Upper
 43 100
 58 9.3 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

