

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
 Data File : VW023028.D
 Acq On : 13 May 2022 15:33
 Operator : SY/VA
 Sample : N2821-09
 Misc : 4.46g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLC9

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 14 00:01:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 23:57:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	337894	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	266337	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	85529	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	198938	28.697	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 114.800%			
7) Chloroethane-d5	2.885	69	149801	33.215	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 132.840%			
11) 1,1-Dichloroethene-d2	4.013	63	168382m	18.798	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 75.200%			
21) 2-Butanone-d5	7.080	46	33558	25.460	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 50.920%			
24) Chloroform-d	7.653	84	285423	28.832	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 115.320%			
26) 1,2-Dichloroethane-d4	8.305	65	170538m	31.410	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 125.640%			
32) Benzene-d6	8.275	84	524624	34.174	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 136.680%#			
36) 1,2-Dichloropropane-d6	9.274	67	164747	38.204	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 152.800%#			
41) Toluene-d8	10.323	98	421319	28.411	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 113.640%			
43) trans-1,3-Dichloroprop...	10.579	79	40876	20.587	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 82.360%			
47) 2-Hexanone-d5	10.927	63	19037	23.125	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 46.260%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	131429	32.699	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 130.800%#			
66) 1,2-Dichlorobenzene-d4	13.853	152	86045	28.779	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 115.120%			
Target Compounds					Qvalue	
13) Acetone	4.129	43	5326m	5.397	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
Data File : VW023028.D
Acq On : 13 May 2022 15:33
Operator : SY/VA
Sample : N2821-09
Misc : 4.46g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EXLC9

Quant Time: May 14 00:01:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 23:57:51 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

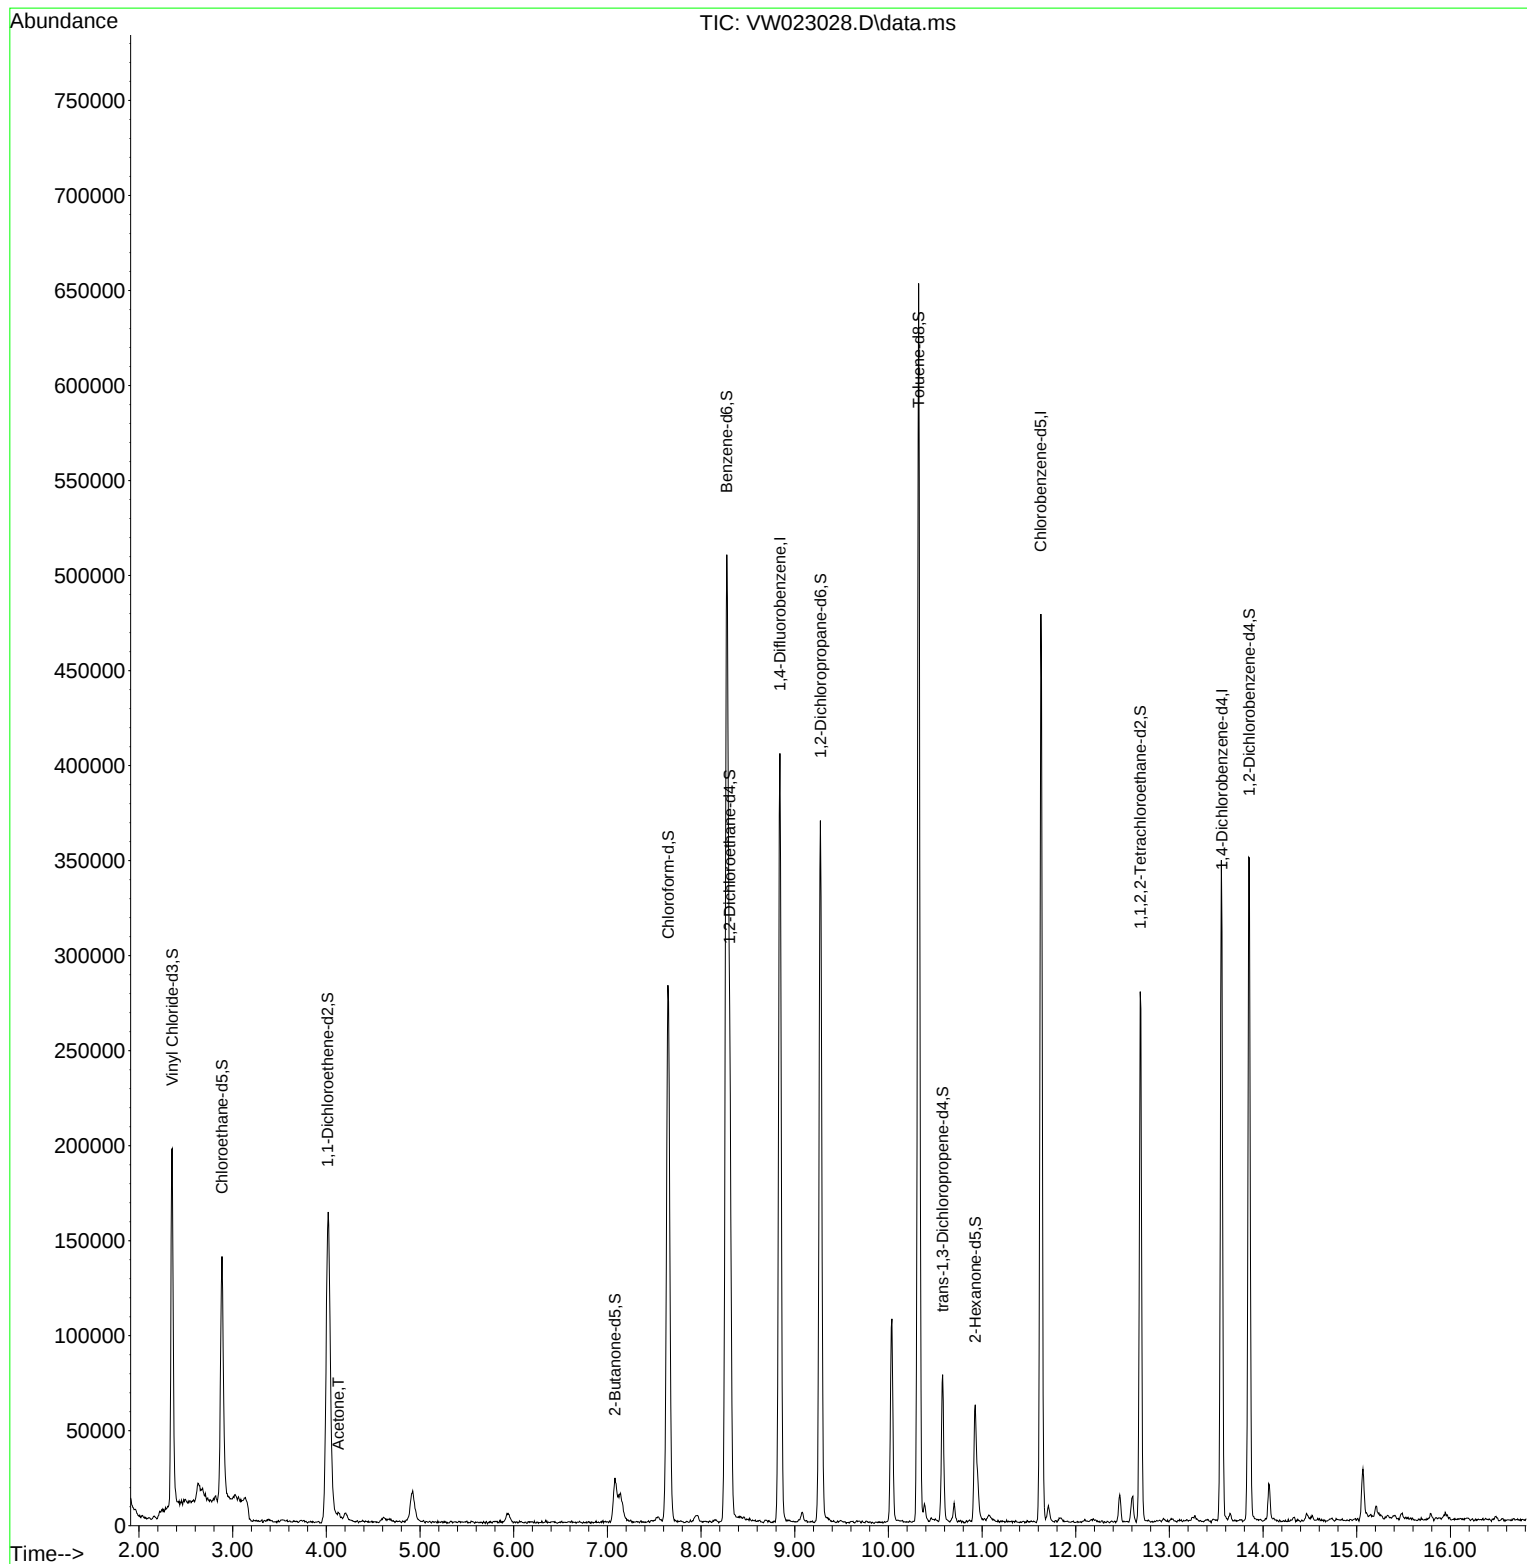

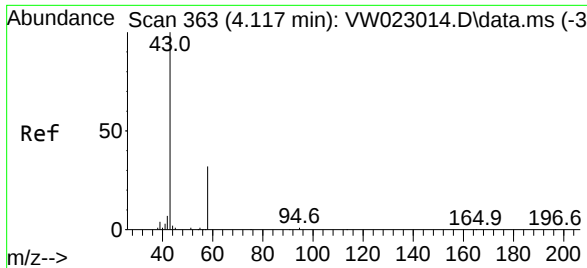

#13

Acetone

Concen: 5.397 ug/L m

RT: 4.129 min Scan# 30

Delta R.T. 0.012 min

Lab File: VW023028.D


Acq: 13 May 2022 15:33

Instrument :

MSVOA_W

ClientSampleId :

EXLC9

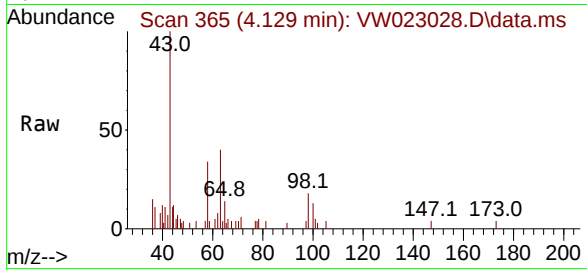

Tgt Ion: 43 Resp: 5320

Ion Ratio Lower Upper

43 100

58 26.1 0.0 64.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022

Supervised By :Mahesh Dadoda 05/16/2022

