

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
 Data File : VW023030.D
 Acq On : 13 May 2022 16:22
 Operator : SY/VA
 Sample : N2821-11
 Misc : 6.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLD1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 14 00:01:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 23:57:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	353075	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	287005	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	96428	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	196702	27.154	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 108.600%			
7) Chloroethane-d5	2.885	69	141160	29.953	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 119.800%			
11) 1,1-Dichloroethene-d2	4.013	63	165996m	17.735	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 70.920%			
21) 2-Butanone-d5	7.080	46	34151	24.796	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 49.600%			
24) Chloroform-d	7.653	84	283514	27.408	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 109.640%			
26) 1,2-Dichloroethane-d4	8.305	65	168275	29.660	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 118.640%			
32) Benzene-d6	8.275	84	521731	31.538	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 126.160%			
36) 1,2-Dichloropropane-d6	9.274	67	164083	35.310	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 141.240%#			
41) Toluene-d8	10.323	98	429569	26.881	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 107.520%			
43) trans-1,3-Dichloroprop...	10.579	79	48294	22.571	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 90.280%			
47) 2-Hexanone-d5	10.927	63	24756	27.907	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 55.820%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	137332	31.707	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 126.840%#			
66) 1,2-Dichlorobenzene-d4	13.853	152	99572	29.540	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 118.160%			
Target Compounds						Qvalue
46) Tetrachloroethene	10.866	164	6224	1.781	ug/L #	71

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051322\
Data File : VW023030.D
Acq On : 13 May 2022 16:22
Operator : SY/VA
Sample : N2821-11
Misc : 6.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EXLD1

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2022
Supervised By : Mahesh Dadoda 05/16/2022


Quant Time: May 14 00:01:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 23:57:51 2022
Response via : Initial Calibration

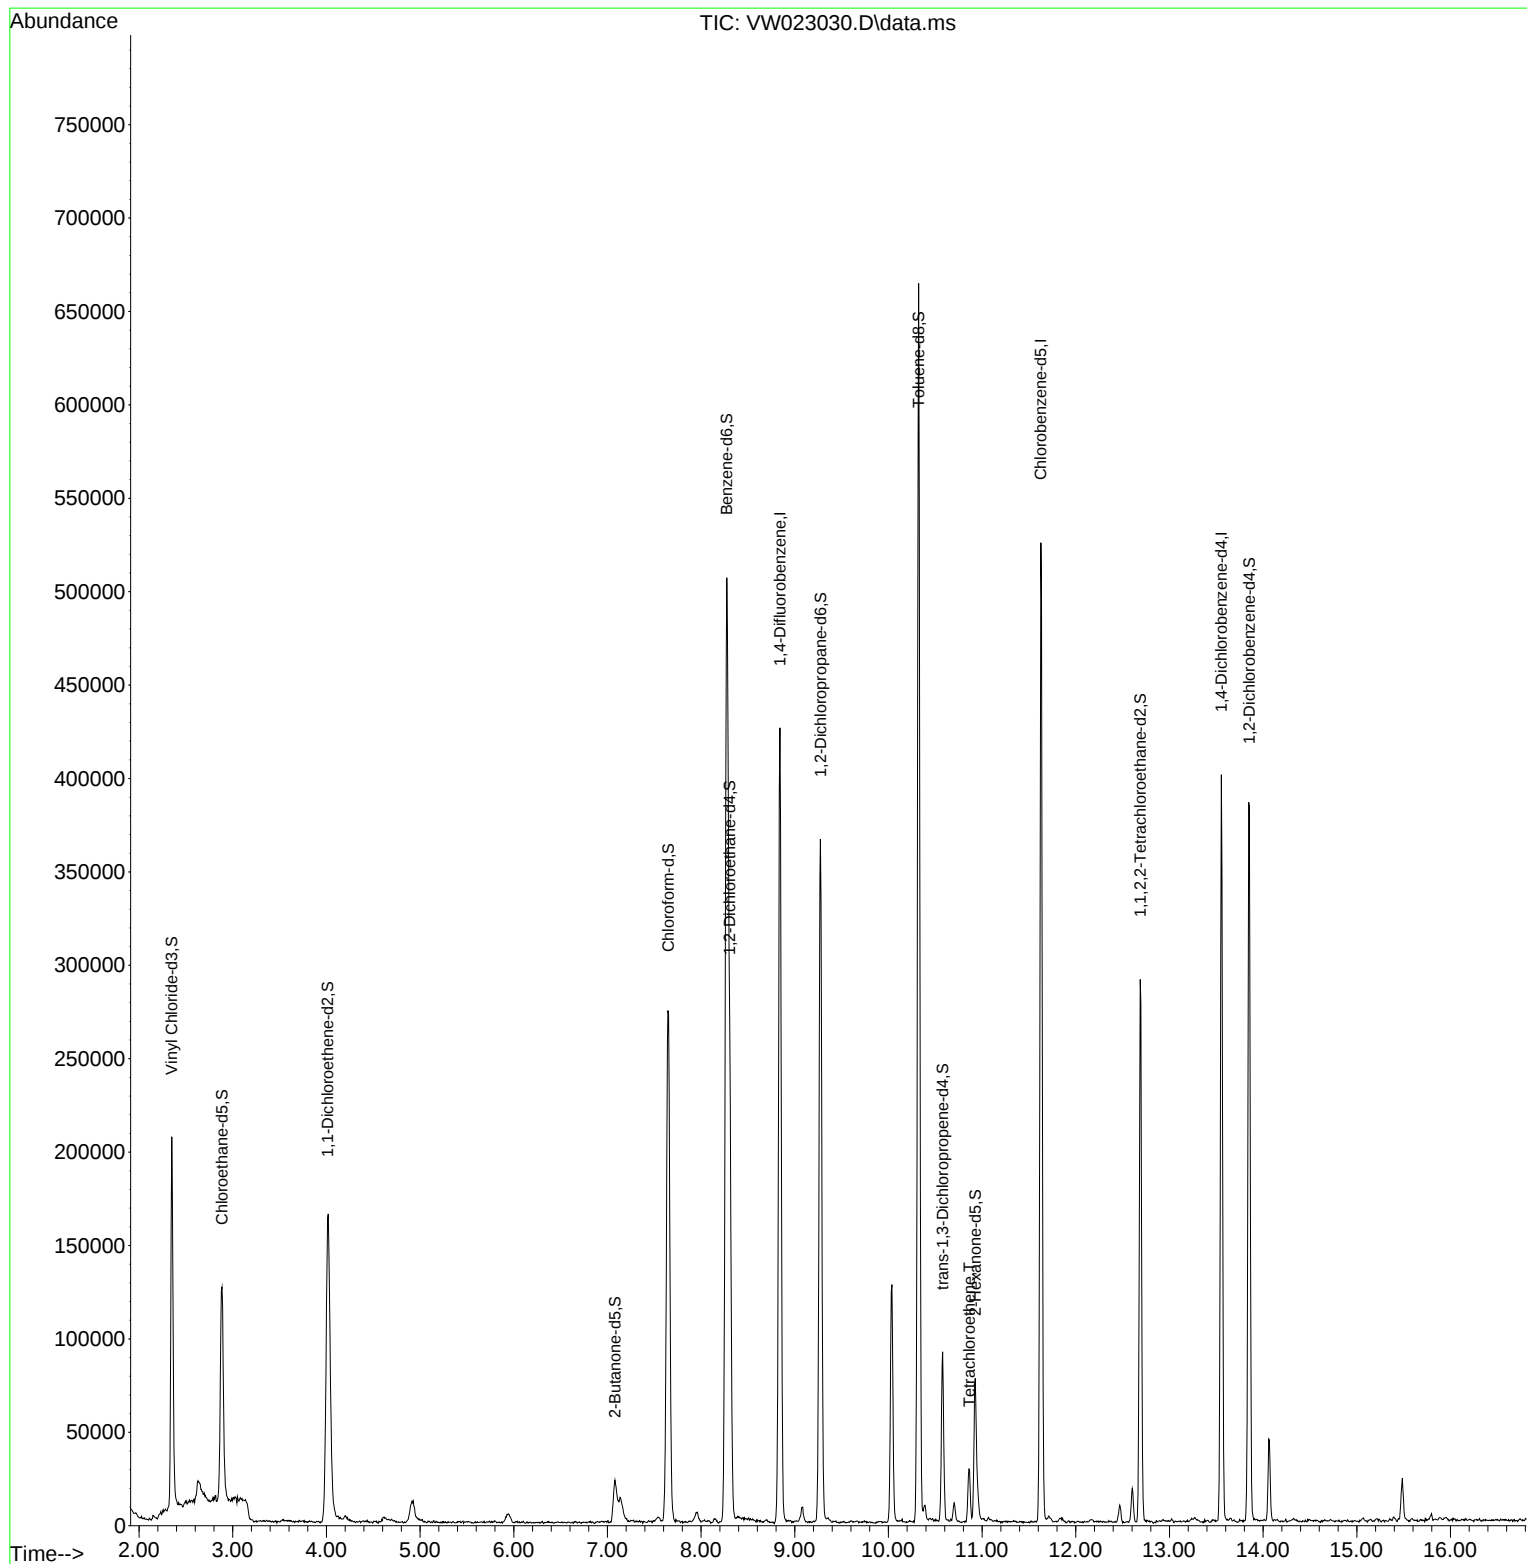

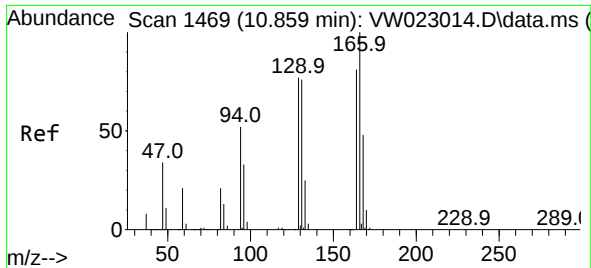

#46
Tetrachloroethene
Concen: 1.781 ug/L
RT: 10.866 min Scan# 14
Delta R.T. 0.006 min
Lab File: VW023030.D
Acq: 13 May 2022 16:22

Instrument :
MSVOA_W
ClientSampleId :
EXLD1

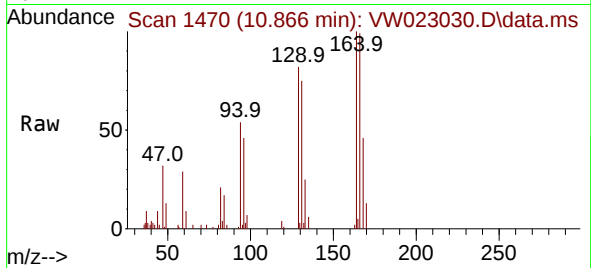

Tgt Ion	Ratio	Lower	Upper
164	100		
129	84.3	76.9	142.7
131	75.1	75.1	139.5
166	98.7	96.0	178.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

