




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051524\
 Data File : VW028600.D
 Acq On : 15 May 2024 12:20
 Operator : SY/MD
 Sample : P2484-01
 Misc : 5.46g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH9P8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/16/2024
 Supervised By :Mahesh Dadoda 05/20/2024

Quant Time: May 16 02:15:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 16 02:15:20 2024
 Response via : Initial Calibration

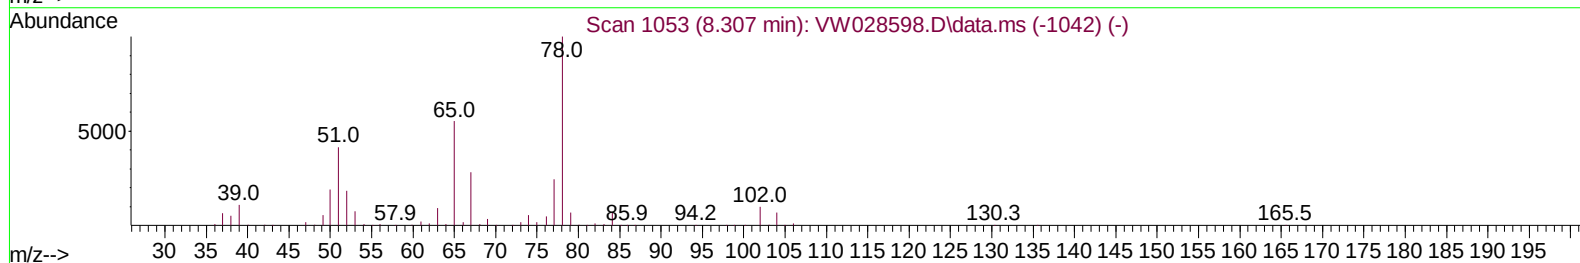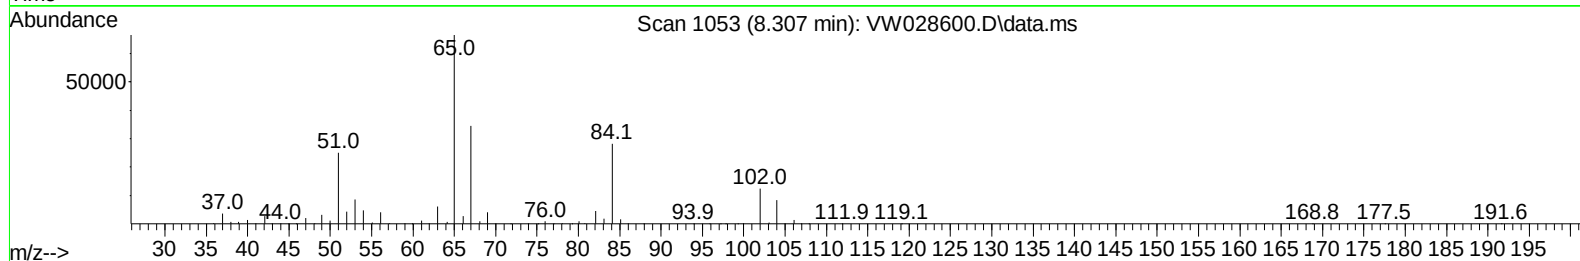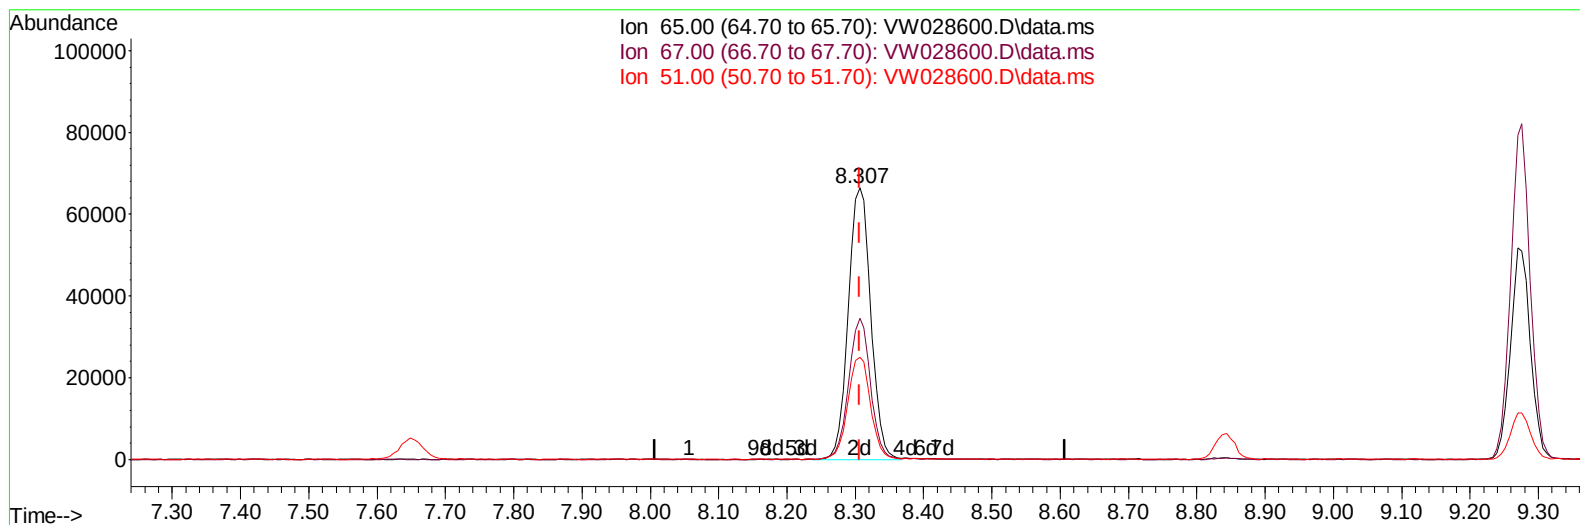

TIC: VW028600.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 16.23 ug/L m

response 151970

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.60	0.04#
51.00	101.70	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051524\
 Data File : VW028600.D
 Acq On : 15 May 2024 12:20
 Operator : SY/MD
 Sample : P2484-01
 Misc : 5.46g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH9P8

Manual IntegrationsAPPROVED

Quant Time: May 16 02:15:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 16 02:15:20 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/16/2024
 Supervised By :Mahesh Dadoda 05/20/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		523488	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		454874	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		216401	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		165231	16.622	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	66.480%		
7) Chloroethane-d5	2.905	69		130582	17.156	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	68.640%		
11) 1,1-Dichloroethene-d2	4.021	65		71273	17.161	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	68.640%		
21) 2-Butanone-d5	7.081	46		61535	23.727	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	47.460%		
24) Chloroform-d	7.648	84		275171	16.823	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	67.280%		
26) 1,2-Dichloroethane-d4	8.307	65		151970m	16.228	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	64.920%#		
32) Benzene-d6	8.276	84		552388	18.201	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	72.800%		
36) 1,2-Dichloropropane-d6	9.276	67		162552	17.800	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	71.200%		
41) Toluene-d8	10.325	98		502720	18.705	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	74.800%		
43) trans-1,3-Dichloroprop...	10.575	79		62088	16.900	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	67.600%		
47) 2-Hexanone-d5	10.922	63		41608	26.416	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	52.840%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		111386	14.545	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	58.200%		
66) 1,2-Dichlorobenzene-d4	13.848	152		147805	17.920	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	71.680%#		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051524\
Data File : VW028600.D
Acq On : 15 May 2024 12:20
Operator : SY/MD
Sample : P2484-01
Misc : 5.46g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH9P8

Manual IntegrationsAPPROVED

Quant Time: May 16 02:15:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 16 02:15:20 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/16/2024
Supervised By :Mahesh Dadoda 05/20/2024

