

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051624\
 Data File : VW028623.D
 Acq On : 16 May 2024 15:16
 Operator : SY/MD
 Sample : P2484-19
 Misc : 5.67g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH9T1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2024
 Supervised By :Mahesh Dadoda 05/17/2024

Quant Time: May 17 01:03:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 17 01:01:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	371356	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	352090	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	165921	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	133592	18.944	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.760%		
7) Chloroethane-d5	2.899	69	111658	20.679	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.720%		
11) 1,1-Dichloroethene-d2	4.027	65	58997	20.024	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	80.080%		
21) 2-Butanone-d5	7.075	46	70861	38.516	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.040%		
24) Chloroform-d	7.648	84	252012	21.718	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	86.880%		
26) 1,2-Dichloroethane-d4	8.307	65	152867m	23.011	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.040%		
32) Benzene-d6	8.276	84	504859	21.492	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.960%		
36) 1,2-Dichloropropane-d6	9.276	67	156209	22.098	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.400%		
41) Toluene-d8	10.325	98	448366	21.553	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.200%		
43) trans-1,3-Dichloroprop...	10.575	79	60718	21.352	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.400%		
47) 2-Hexanone-d5	10.922	63	47885	39.277	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	78.560%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	120489	20.327	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	81.320%		
66) 1,2-Dichlorobenzene-d4	13.849	152	144465	22.844	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.360%		
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	14544	2.532	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051624\
Data File : VW028623.D
Acq On : 16 May 2024 15:16
Operator : SY/MD
Sample : P2484-19
Misc : 5.67g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BH9T1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2024
Supervised By :Mahesh Dadoda 05/17/2024


Quant Time: May 17 01:03:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 17 01:01:12 2024
Response via : Initial Calibration

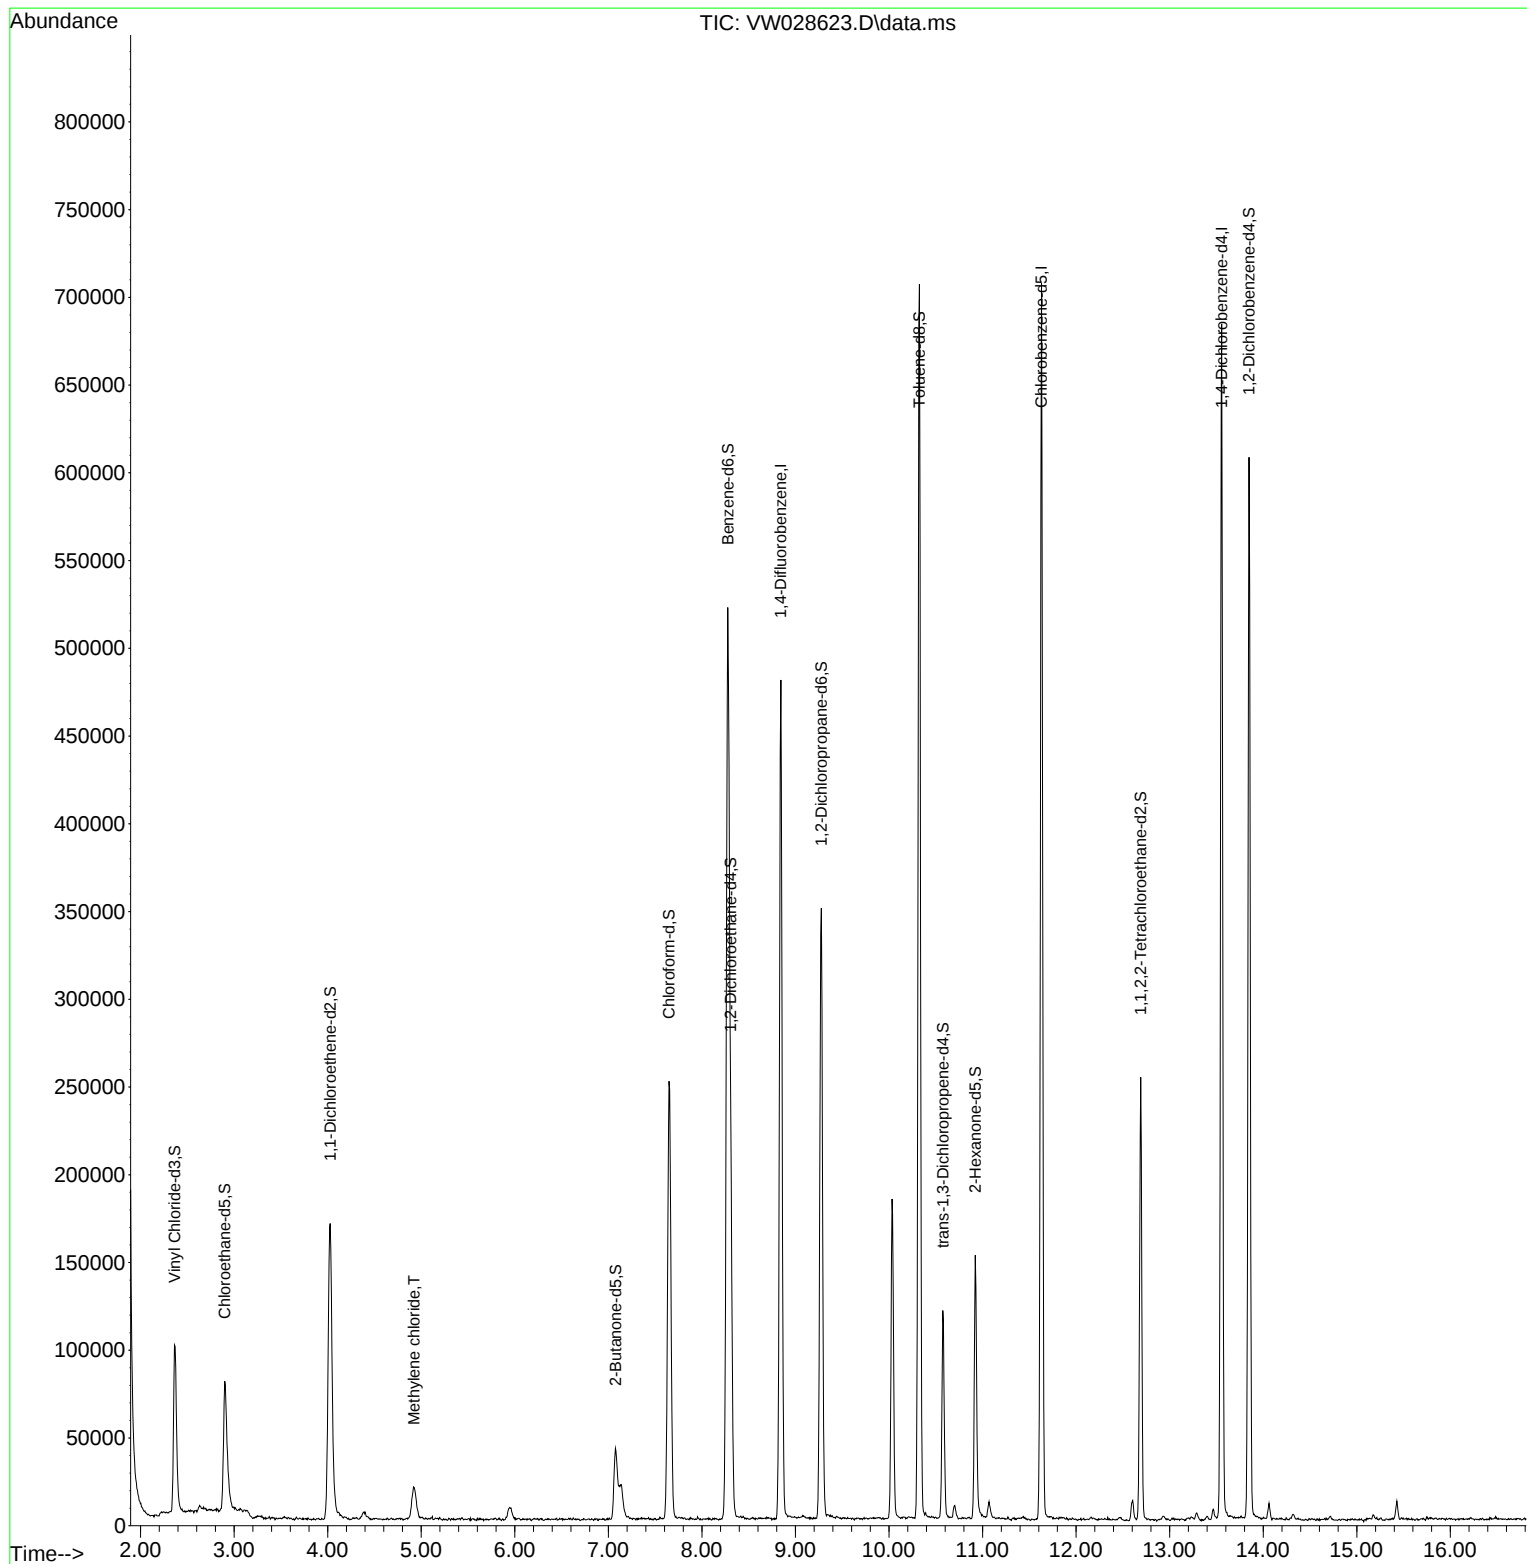

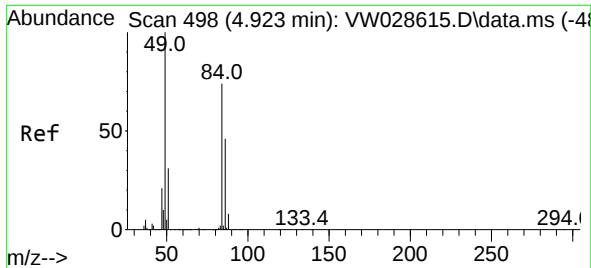

#16
Methylene chloride
Concen: 2.532 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW028623.D
Acq: 16 May 2024 15:16

Instrument :
MSVOA_W
ClientSampleId :
BH9T1

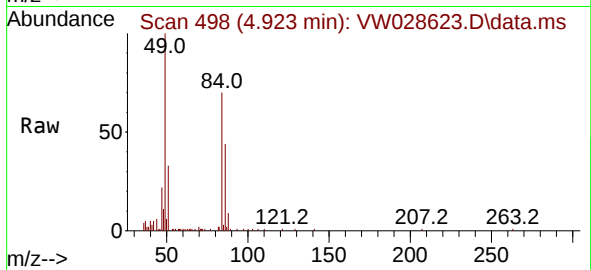

Tgt Ion: 84 Resp: 14544
Ion Ratio Lower Upper
84 100
86 62.9 44.4 82.4
49 142.7 100.2 186.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2024
Supervised By :Mahesh Dadoda 05/17/2024

