

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
 Data File : VW023098.D
 Acq On : 17 May 2022 14:12
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK463

Quant Time: May 18 01:29:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 18 01:26:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	327162	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	322520	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	176720	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	155845	23.218	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.880%
7) Chloroethane-d5	2.885	69	109929	25.174	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.680%
11) 1,1-Dichloroethene-d2	4.019	63	150802	17.388	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.560%
21) 2-Butanone-d5	7.080	46	71025	55.653	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.300%
24) Chloroform-d	7.653	84	239056	24.940	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.760%
26) 1,2-Dichloroethane-d4	8.305	65	142538	27.114	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.440%
32) Benzene-d6	8.274	84	479161	25.775	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.120%
36) 1,2-Dichloropropane-d6	9.274	67	136860	26.209	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.840%
41) Toluene-d8	10.323	98	469923	26.168	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.680%
43) trans-1,3-Dichloroprop...	10.579	79	60310	25.083	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.320%
47) 2-Hexanone-d5	10.926	63	57209	57.389	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.780%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	132934	27.312	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	163368	26.445	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.800%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	5467	0.767	ug/L	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
Data File : VW023098.D
Acq On : 17 May 2022 14:12
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK463

Quant Time: May 18 01:29:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 18 01:26:16 2022
Response via : Initial Calibration

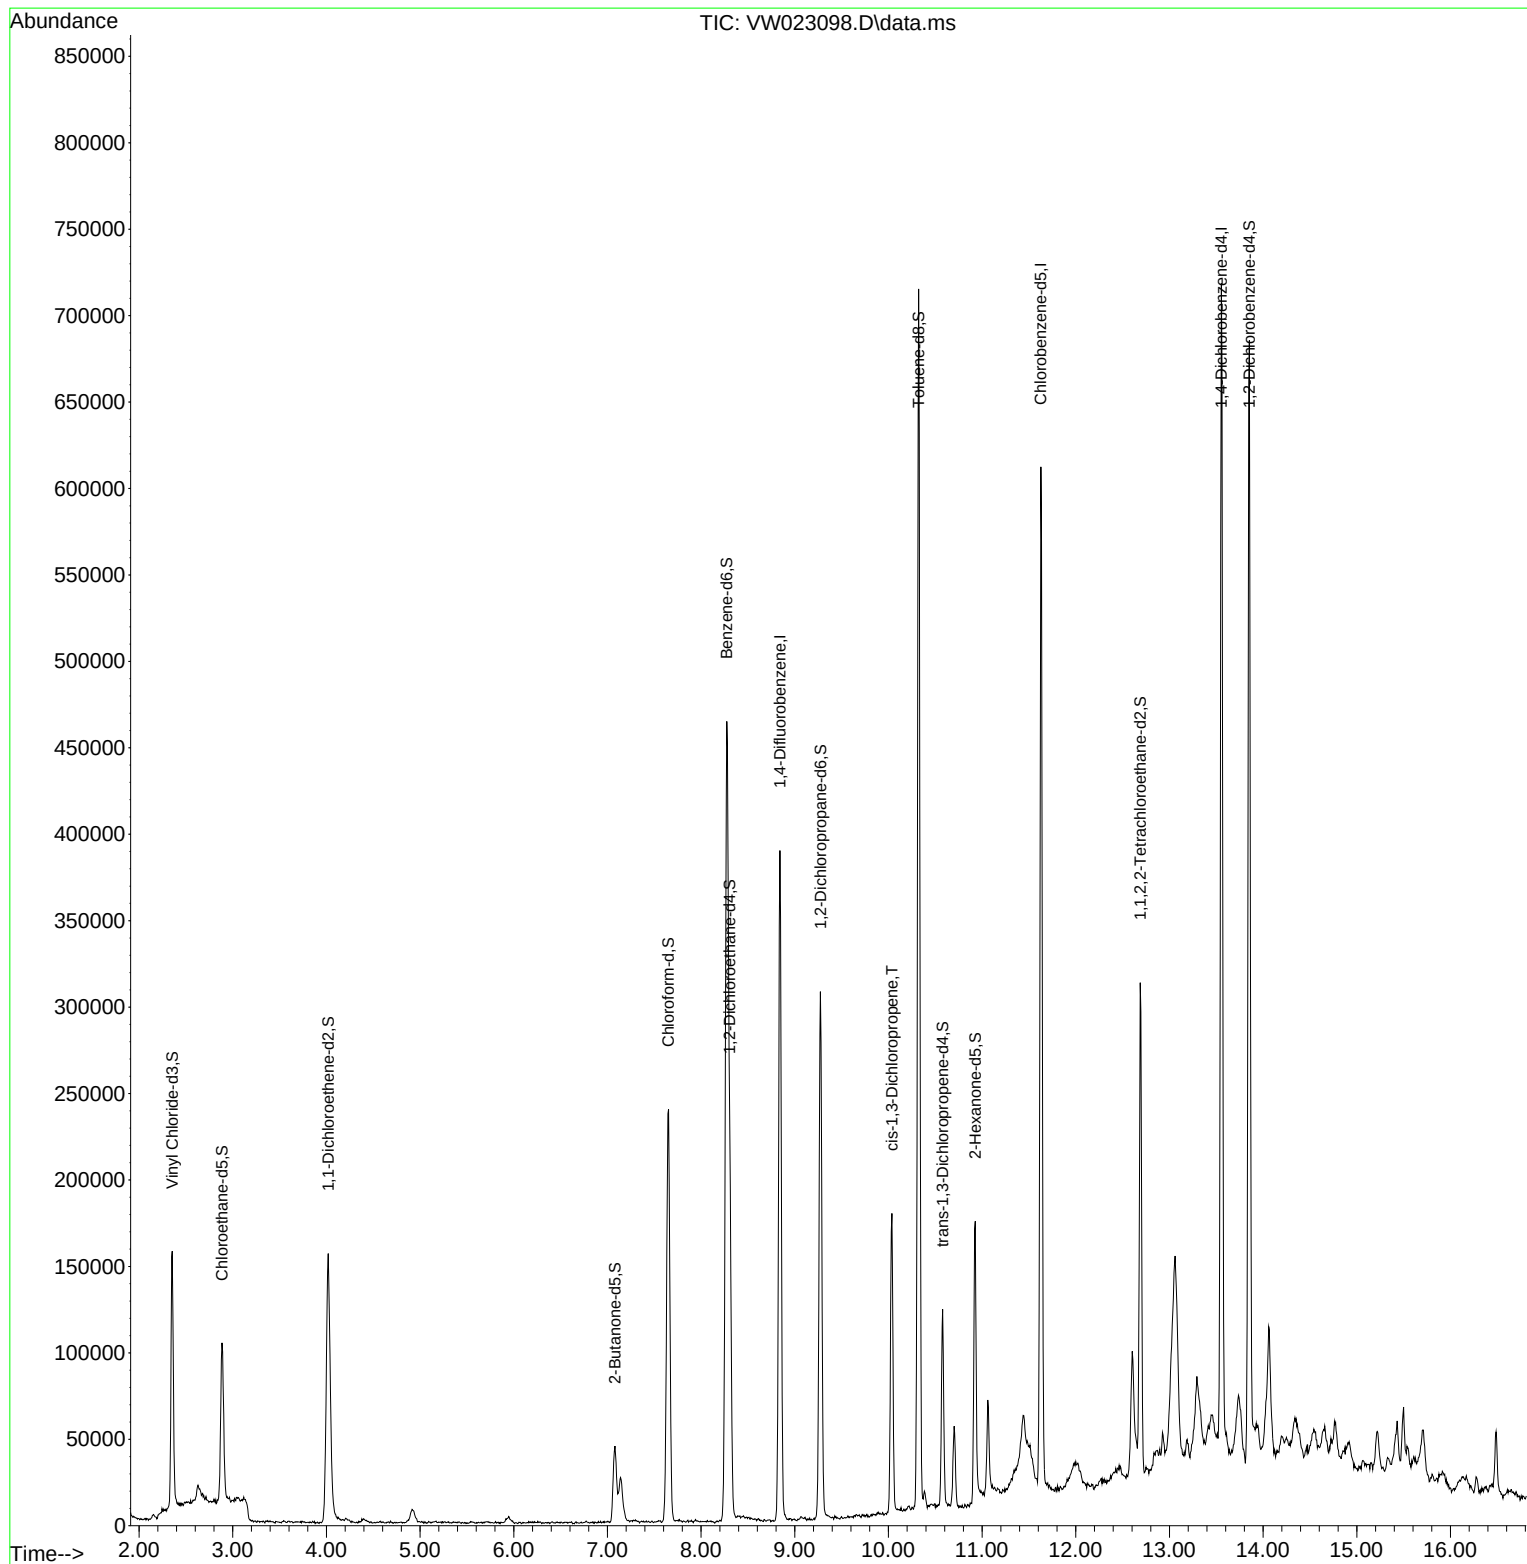

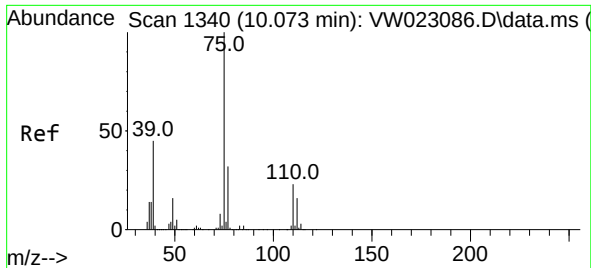

#39
 cis-1,3-Dichloropropene
 Concen: 0.767 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023098.D
 Acq: 17 May 2022 14:12

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK463

Tgt Ion: 75 Resp: 5467
 Ion Ratio Lower Upper
 75 100
 77 42.7 22.1 41.1#

