

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
 Data File : VW023104.D
 Acq On : 17 May 2022 16:37
 Operator : SY/VA
 Sample : N2843-06RE
 Misc : 6.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4H6

Quant Time: May 18 01:30:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 18 01:26:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	358282	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	311703	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	128908	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	104589	14.228	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.920%
7) Chloroethane-d5	2.885	69	79500	16.624	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.480%
11) 1,1-Dichloroethene-d2	4.013	63	103694	10.918	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.680%#
21) 2-Butanone-d5	7.080	46	49321	35.290	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.580%
24) Chloroform-d	7.647	84	212850	20.278	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.120%
26) 1,2-Dichloroethane-d4	8.305	65	121244	21.060	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.240%
32) Benzene-d6	8.275	84	376195	20.939	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.760%
36) 1,2-Dichloropropane-d6	9.274	67	118489	23.478	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.920%
41) Toluene-d8	10.323	98	324488	18.696	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.800%
43) trans-1,3-Dichloroprop...	10.579	79	41885	18.025	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.080%
47) 2-Hexanone-d5	10.920	63	37276	38.691	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.380%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	108785	23.126	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	91339	20.270	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.080%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.043	75	3611	0.524	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
Data File : VW023104.D
Acq On : 17 May 2022 16:37
Operator : SY/VA
Sample : N2843-06RE
Misc : 6.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4H6

Quant Time: May 18 01:30:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 18 01:26:16 2022
Response via : Initial Calibration

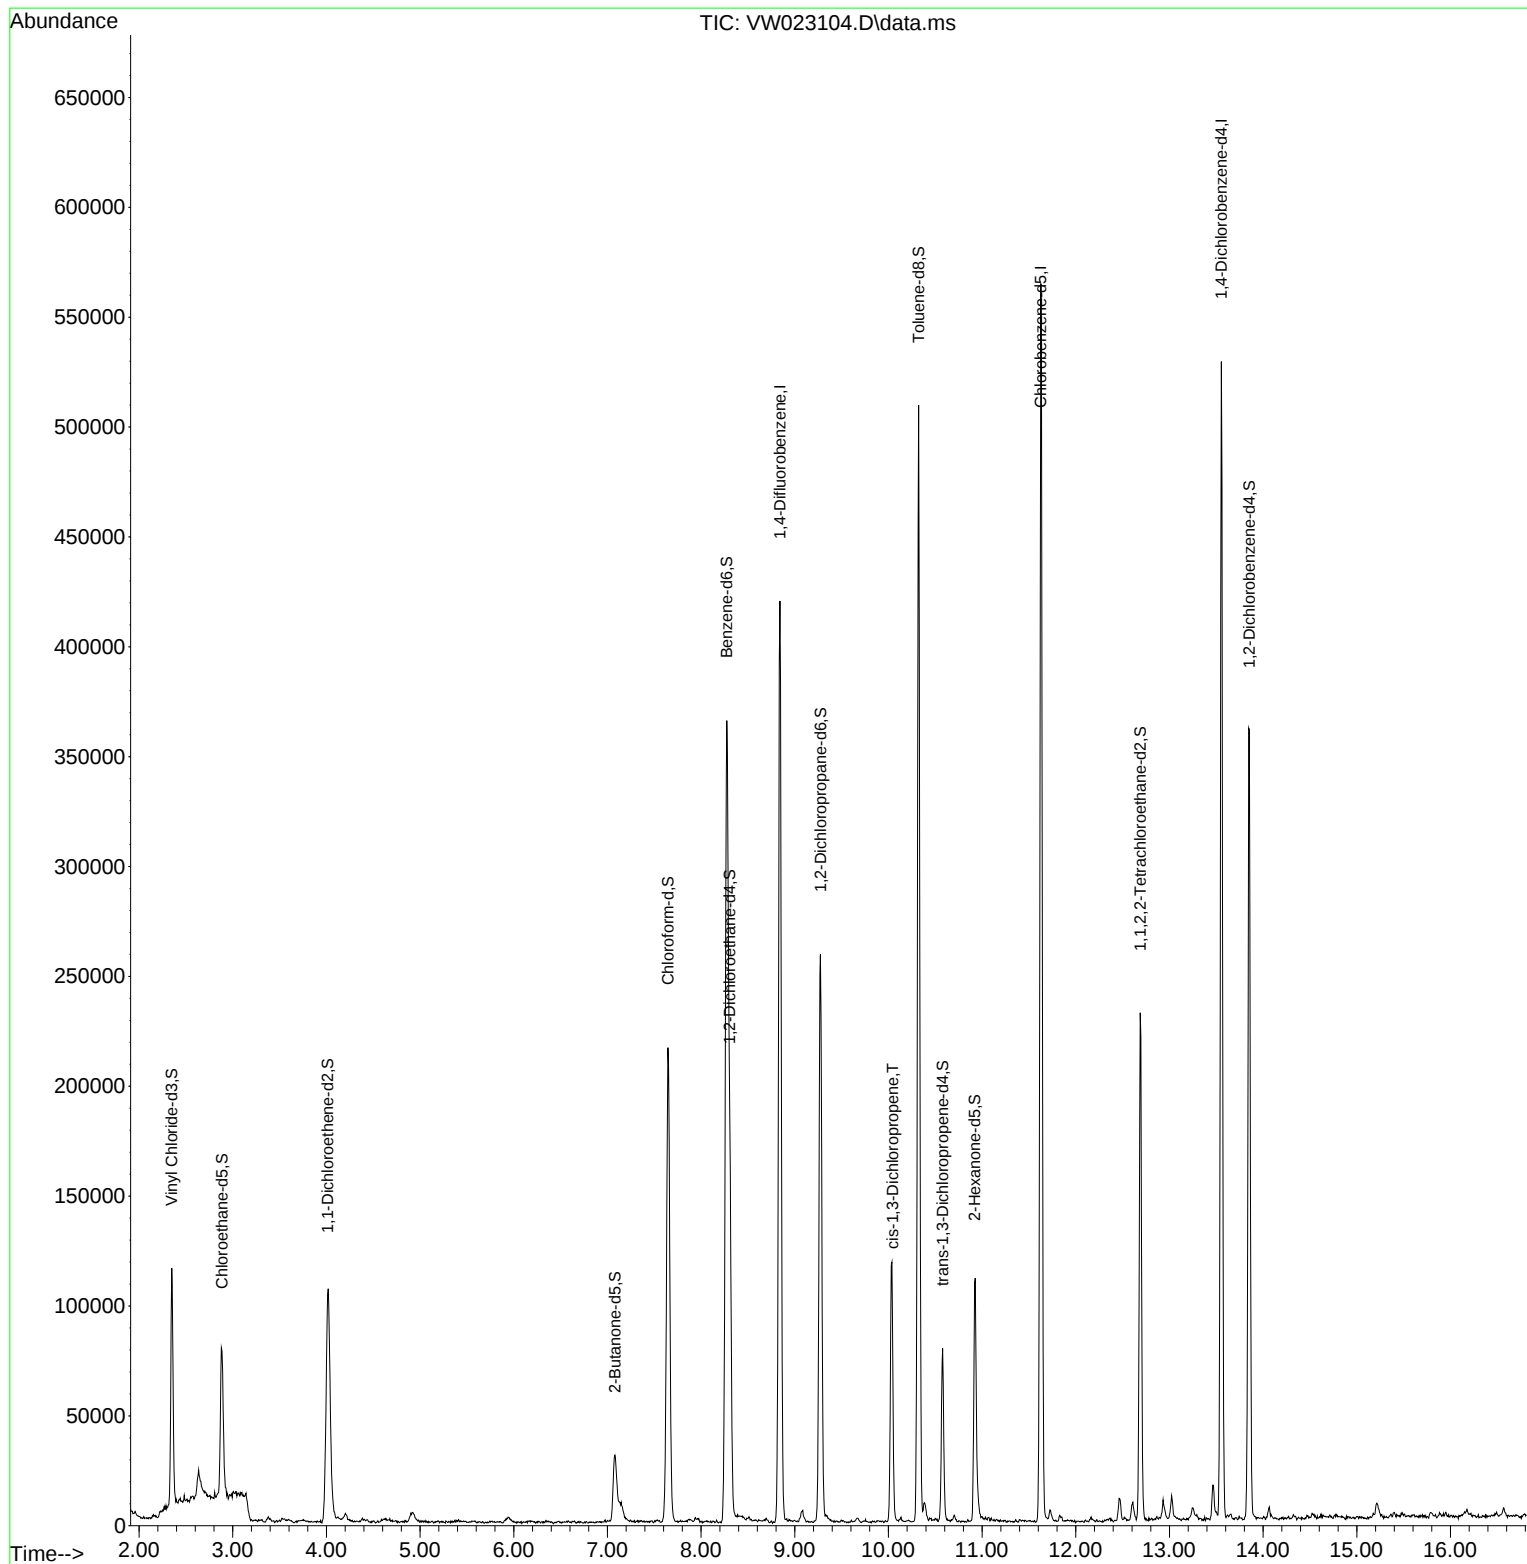

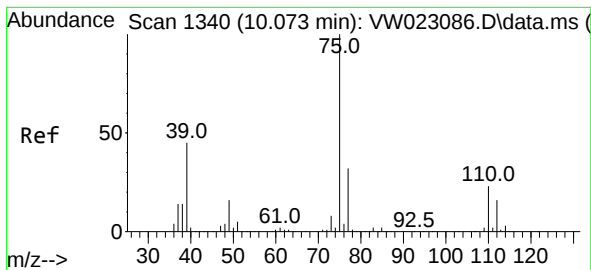

#39
 cis-1,3-Dichloropropene
 Concen: 0.524 ug/L
 RT: 10.043 min Scan# 11
 Delta R.T. -0.031 min
 Lab File: VW023104.D
 Acq: 17 May 2022 16:37

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4H6

Tgt Ion: 75 Resp: 3611
 Ion Ratio Lower Upper
 75 100
 77 40.5 22.1 41.1

