

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
 Data File : VW023111.D
 Acq On : 17 May 2022 20:33
 Operator : SY/VA
 Sample : N2883-02
 Misc : 6.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4K4

Quant Time: May 18 04:22:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 18 03:02:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	299989	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	268612	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	117457	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	91506	14.868	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.480%
7) Chloroethane-d5	2.879	69	68470	17.100	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.400%
11) 1,1-Dichloroethene-d2	4.233	63	151	0.019	ug/L	0.21
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.080%#
21) 2-Butanone-d5	7.080	46	77079	65.868	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	131.740%
24) Chloroform-d	7.647	84	181487	20.649	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.600%
26) 1,2-Dichloroethane-d4	8.305	65	111891	23.212	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.840%
32) Benzene-d6	8.275	84	328341	21.207	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.840%
36) 1,2-Dichloropropane-d6	9.274	67	101967	23.445	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.800%
41) Toluene-d8	10.323	98	290967	19.455	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.800%
43) trans-1,3-Dichloroprop...	10.579	79	41559	20.753	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.000%
47) 2-Hexanone-d5	10.927	63	60302	72.632	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	145.260%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	115639	28.527	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	92626	22.559	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.240%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	3847	0.648	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
Data File : VW023111.D
Acq On : 17 May 2022 20:33
Operator : SY/VA
Sample : N2883-02
Misc : 6.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4K4

Quant Time: May 18 04:22:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 18 03:02:16 2022
Response via : Initial Calibration

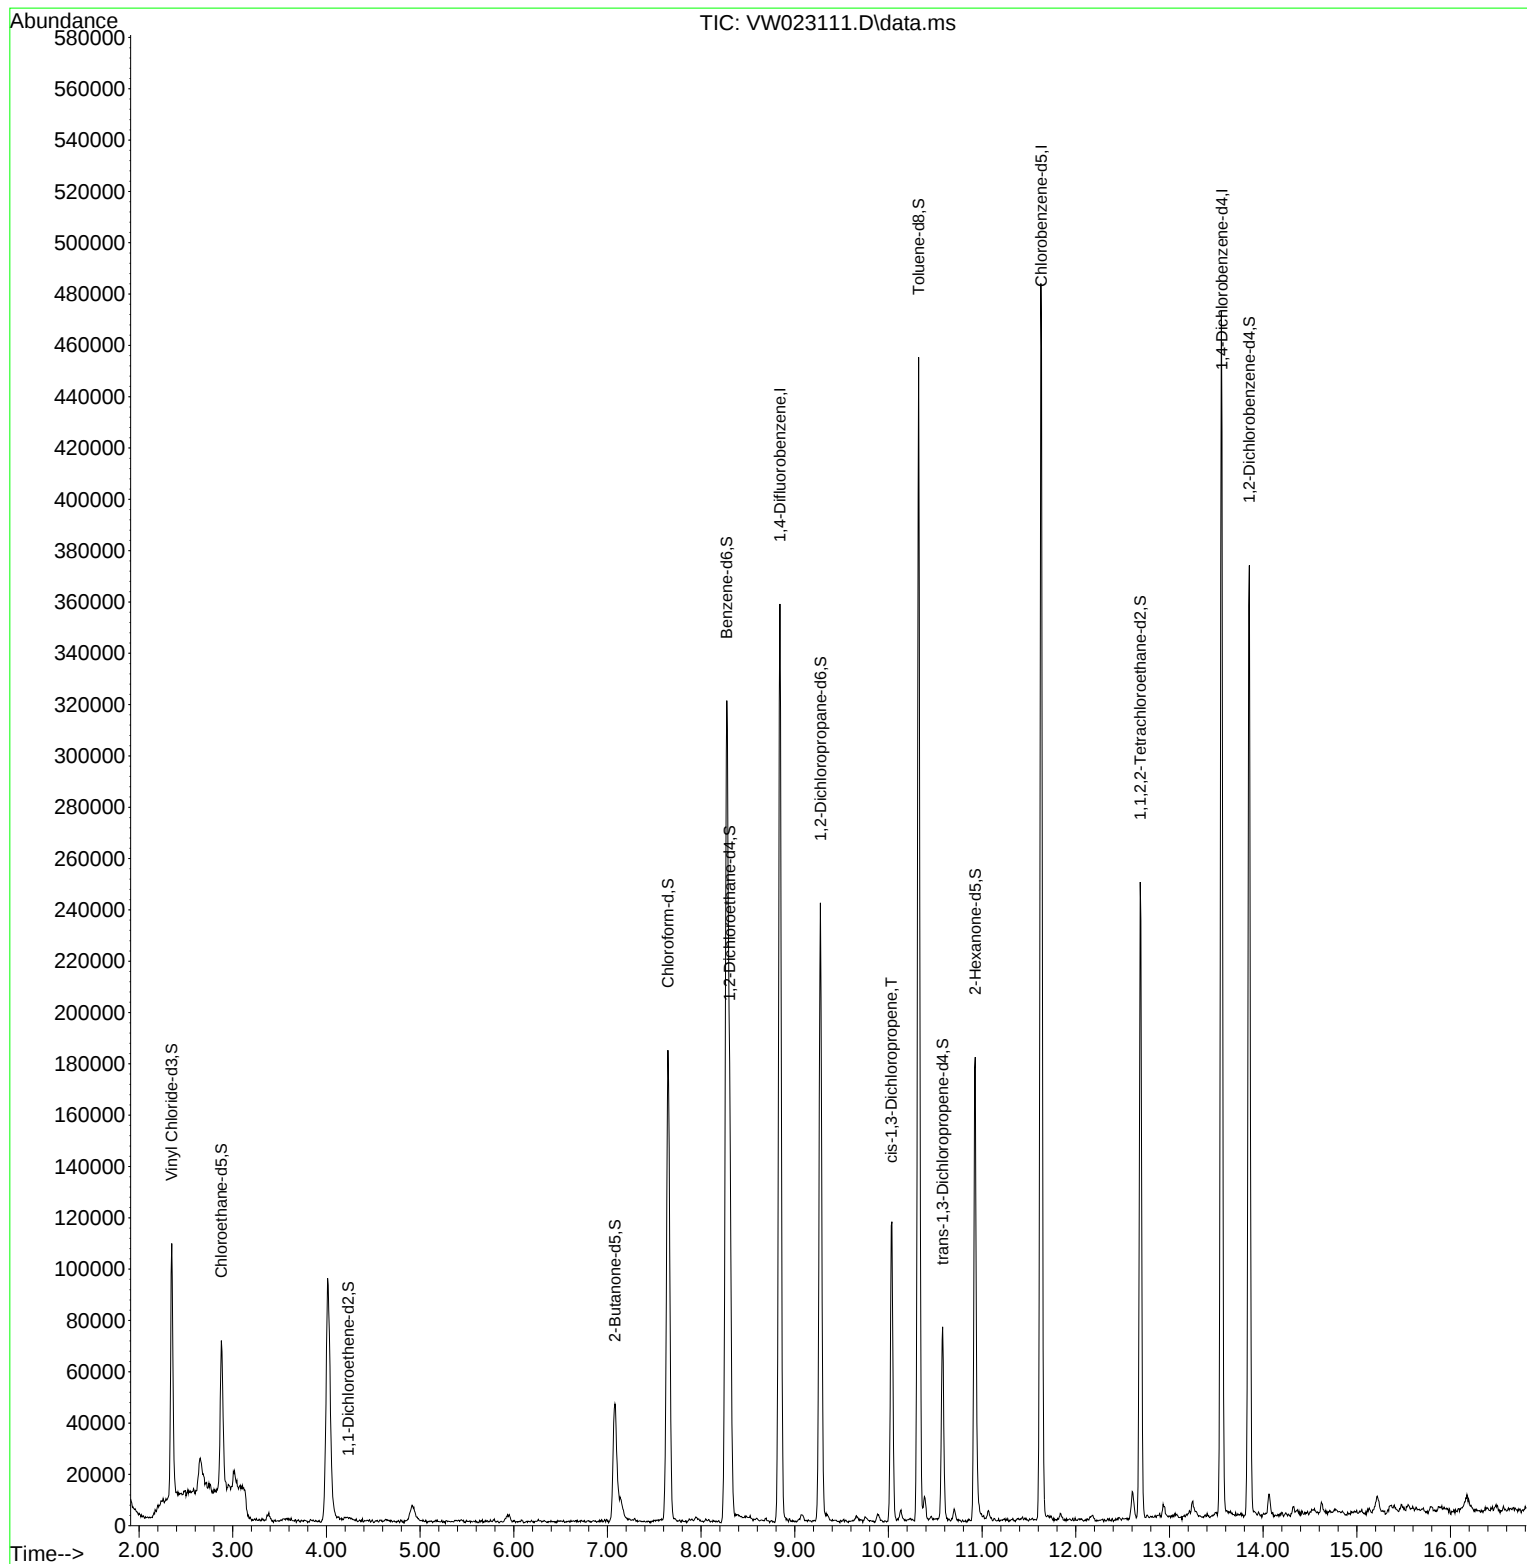

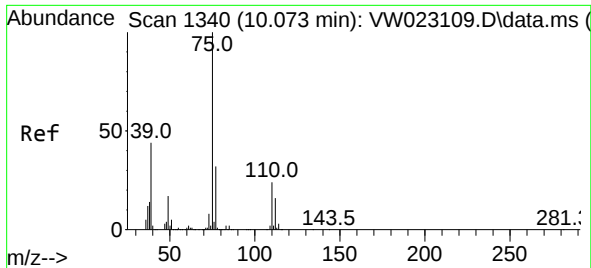

#39
 cis-1,3-Dichloropropene
 Concen: 0.648 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW023111.D
 Acq: 17 May 2022 20:33

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4K4

Tgt Ion: 75 Resp: 3847
 Ion Ratio Lower Upper
 75 100
 77 30.4 22.1 41.1

