

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
 Data File : VW023112.D
 Acq On : 17 May 2022 20:57
 Operator : SY/VA
 Sample : N2883-07
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4K7

Quant Time: May 18 04:23:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 18 03:02:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	304653	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	247231	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	83355	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	101306	16.208	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.840%
7) Chloroethane-d5	2.879	69	73664	18.115	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.480%
11) 1,1-Dichloroethene-d2	4.013	63	96695	11.973	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	47.880%
21) 2-Butanone-d5	7.080	46	32117	27.025	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.060%
24) Chloroform-d	7.647	84	196623	22.029	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.120%
26) 1,2-Dichloroethane-d4	8.305	65	109473	22.363	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.440%
32) Benzene-d6	8.275	84	333758	23.421	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.680%
36) 1,2-Dichloropropane-d6	9.274	67	110056	27.494	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.960%
41) Toluene-d8	10.323	98	284097	20.638	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.560%
43) trans-1,3-Dichloroprop...	10.579	79	27251	14.785	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	59.160%
47) 2-Hexanone-d5	10.920	63	24518	32.085	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.180%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	89672	24.034	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	59595	20.453	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.800%
Target Compounds						
39) cis-1,3-Dichloropropene	10.030	75	2665	0.488	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
Data File : VW023112.D
Acq On : 17 May 2022 20:57
Operator : SY/VA
Sample : N2883-07
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4K7

Quant Time: May 18 04:23:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 18 03:02:16 2022
Response via : Initial Calibration

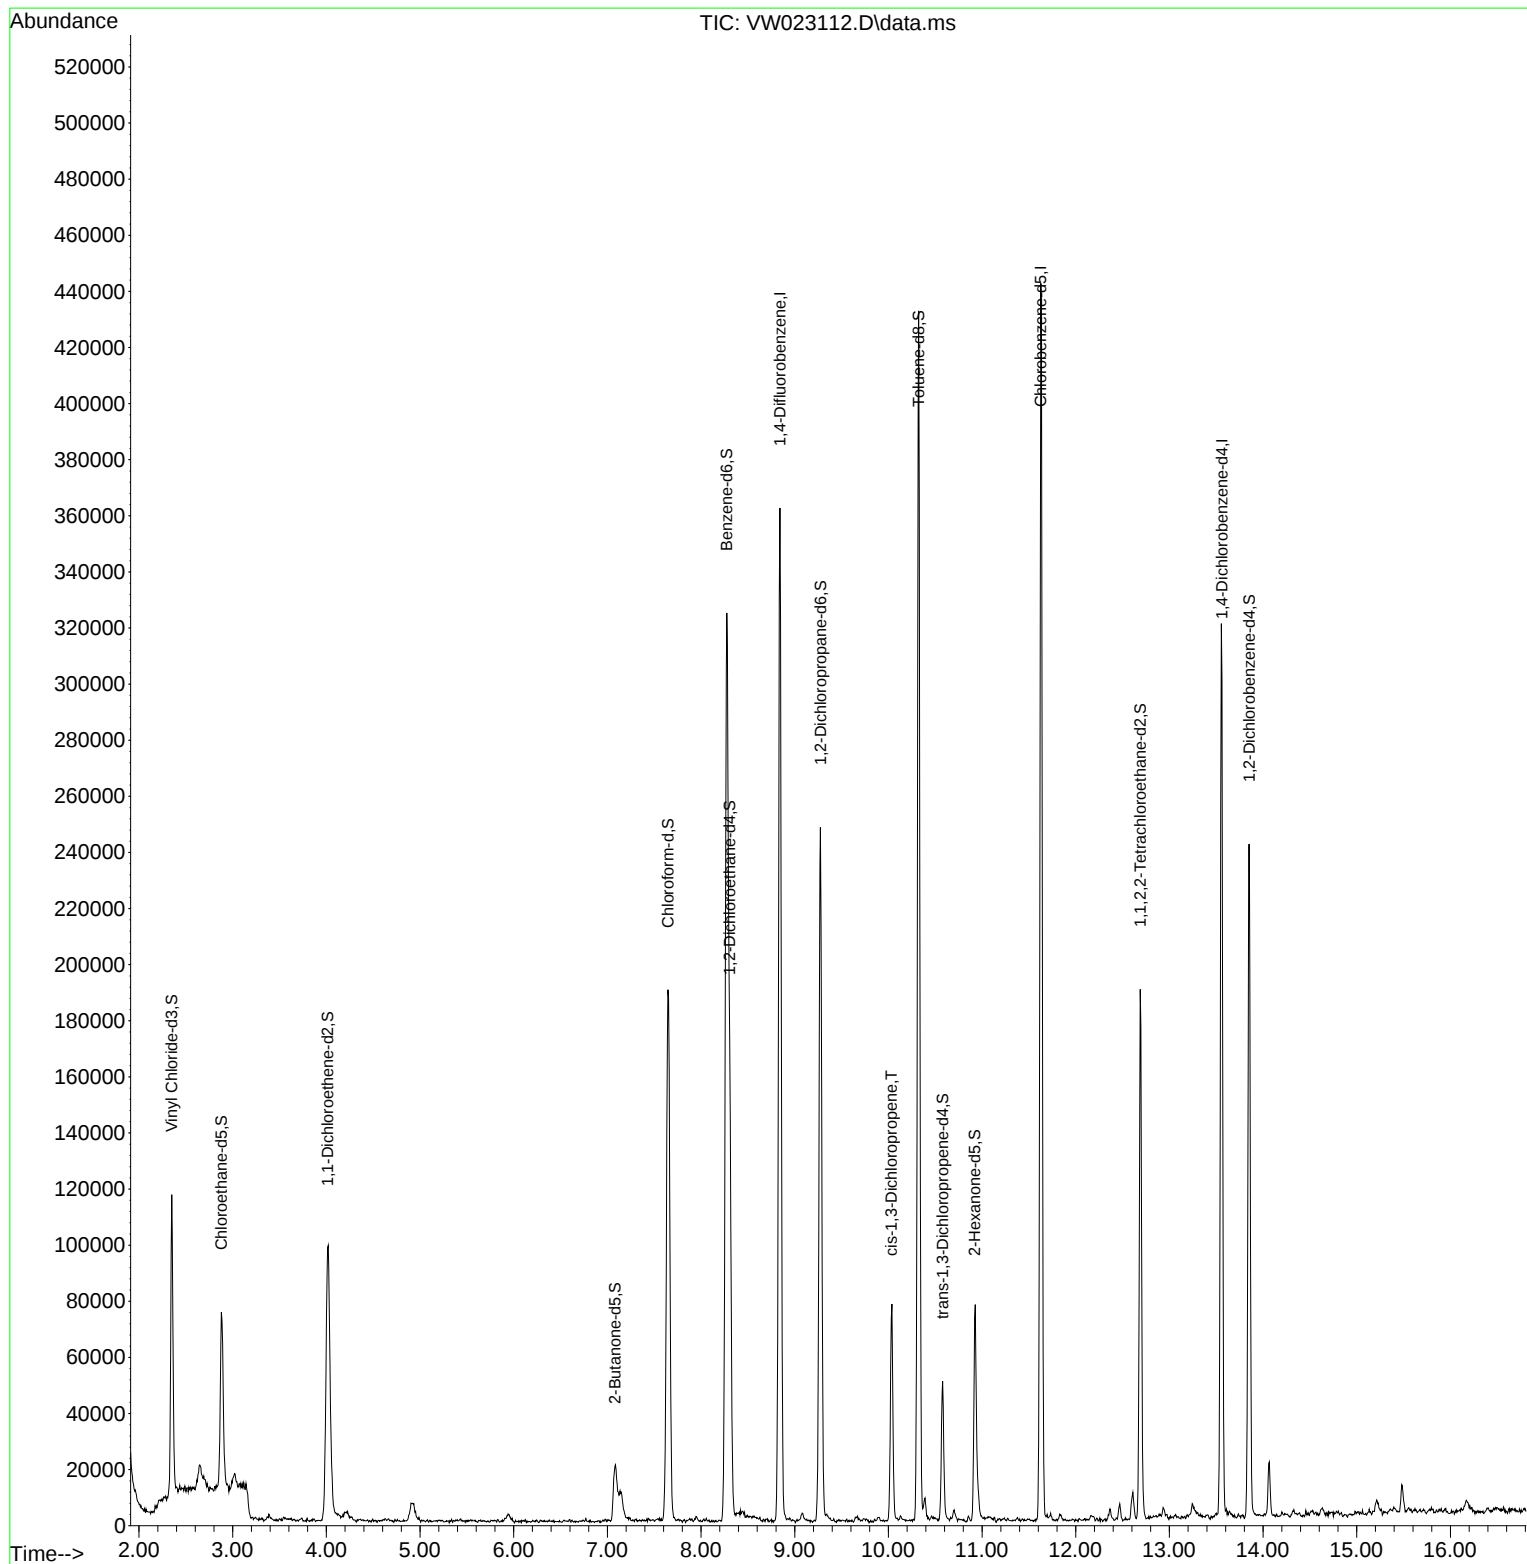

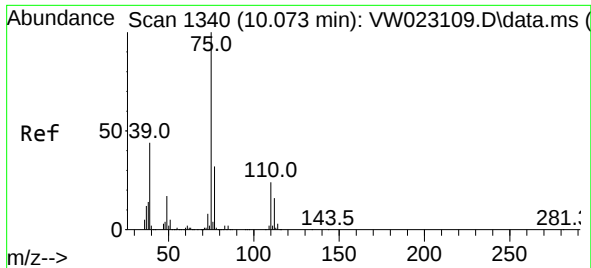

#39
 cis-1,3-Dichloropropene
 Concen: 0.488 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW023112.D
 Acq: 17 May 2022 20:57

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4K7

Tgt Ion: 75 Resp: 2665
 Ion Ratio Lower Upper
 75 100
 77 33.3 22.1 41.1

