




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
 Data File : VW023101.D
 Acq On : 17 May 2022 15:25
 Operator : SY/VA
 Sample : N2843-11
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4J1

Manual IntegrationsAPPROVED

Quant Time: May 18 01:29:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 18 01:26:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/18/2022
 Supervised By :Mahesh Dadoda 05/26/2022

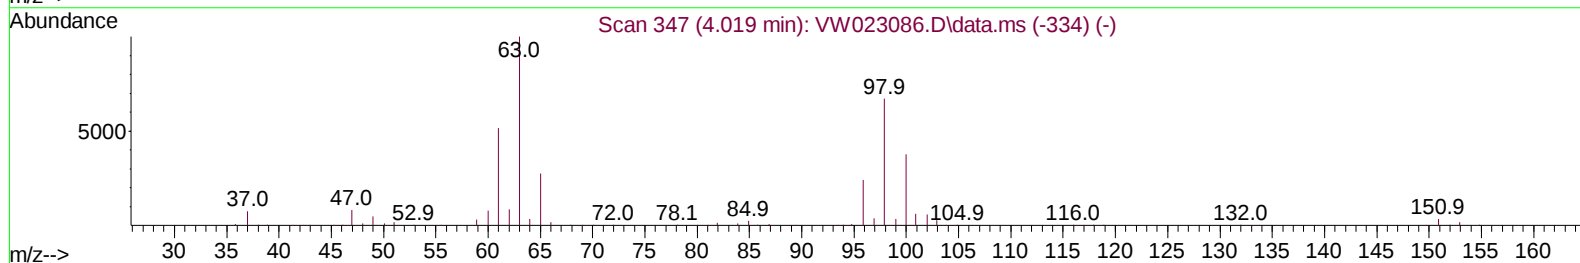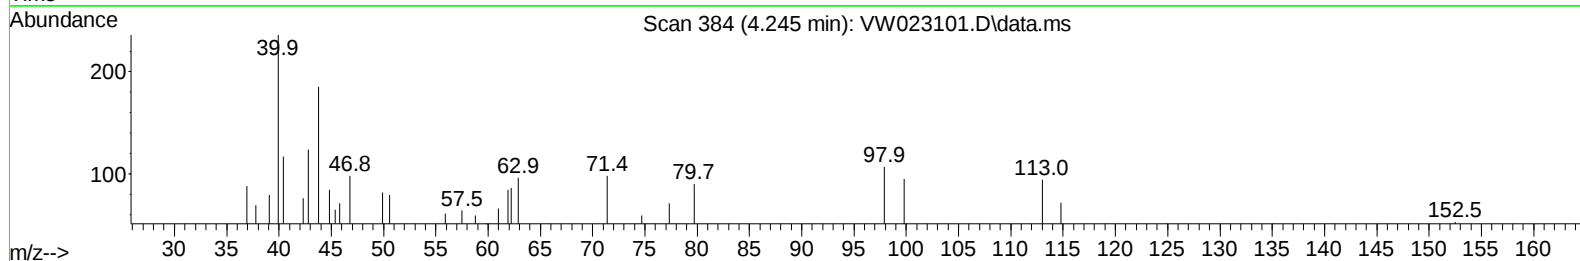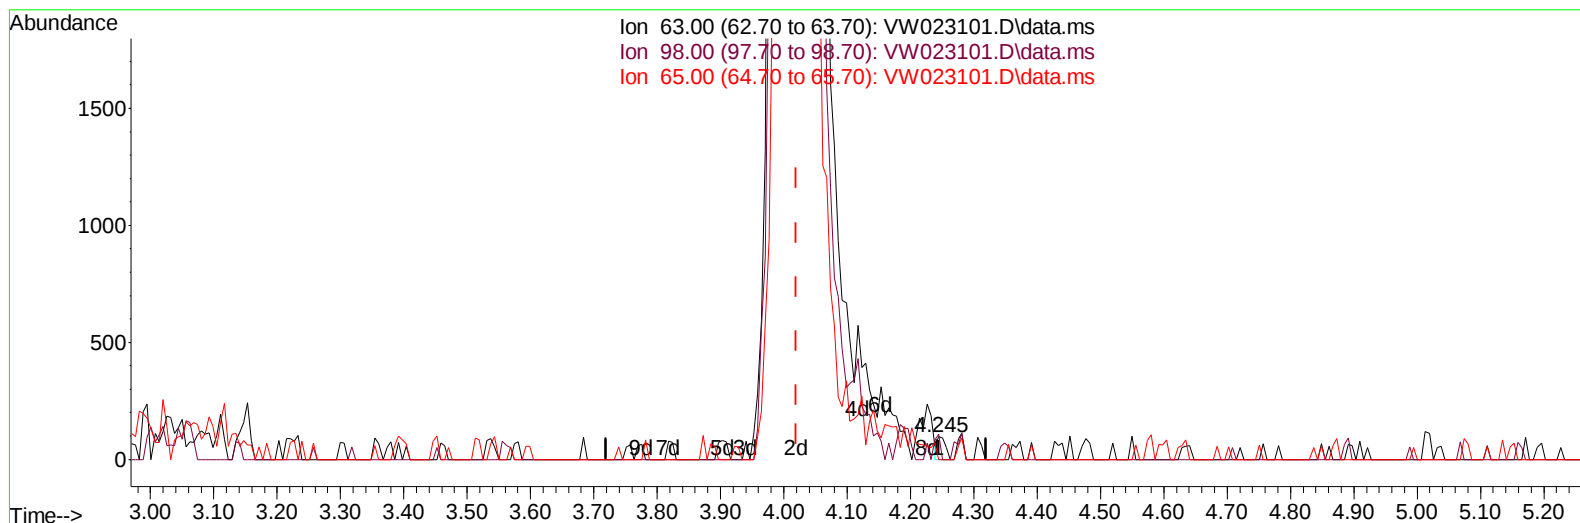

TIC: VW023101.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.245min (+ 0.226) 0.01 ug/L

response 87

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	80.46
65.00	23.30	29.89
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
Data File : VW023101.D
Acq On : 17 May 2022 15:25
Operator : SY/VA
Sample : N2843-11
Misc : 6.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4J1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/18/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 18 01:29:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 18 01:26:16 2022
Response via : Initial Calibration

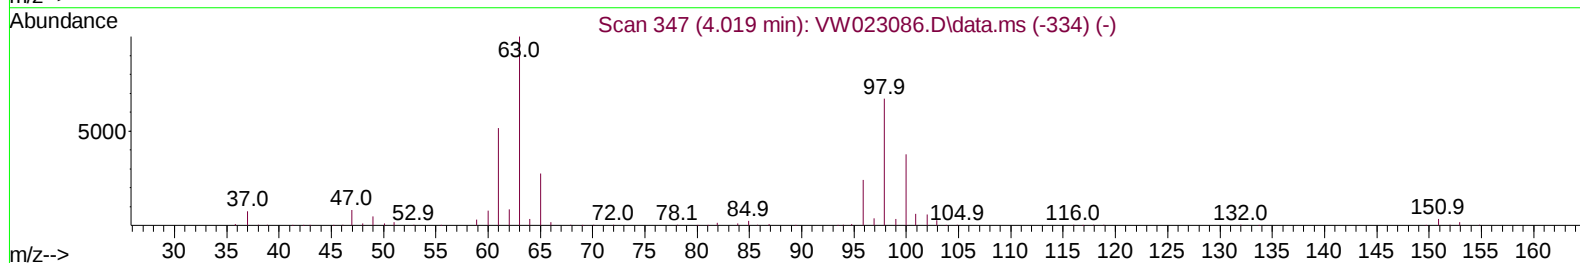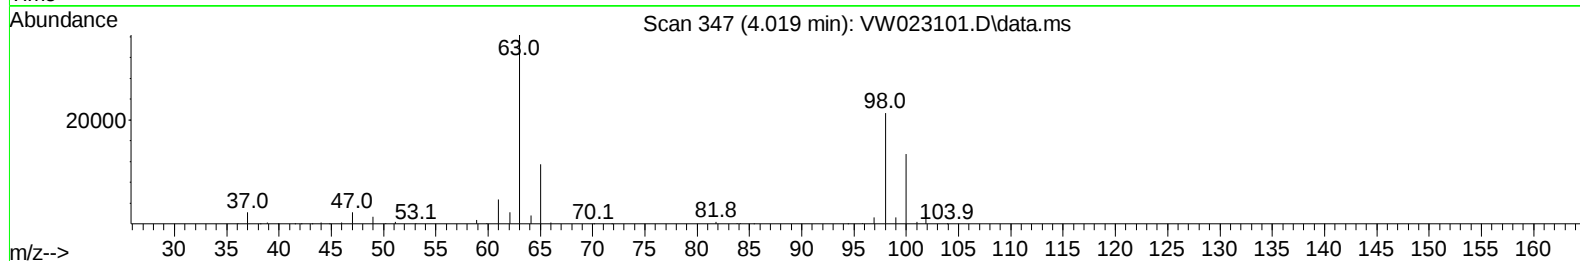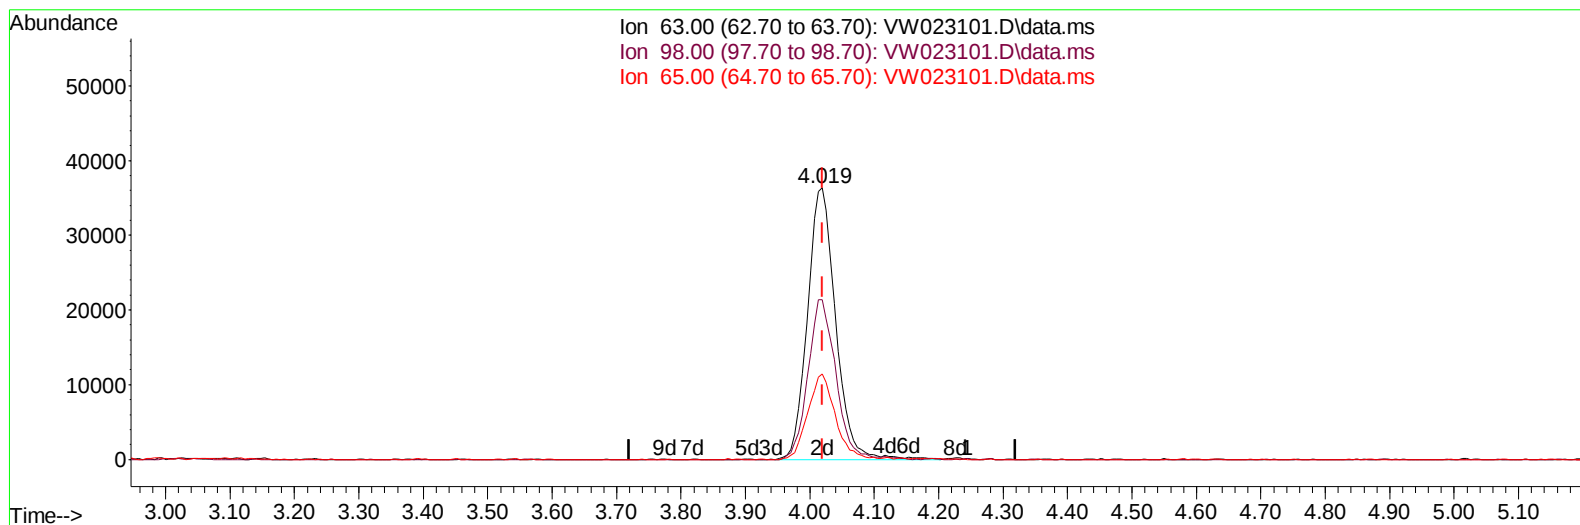

TIC: VW023101.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.000) 12.32 ug/L m

response 110266

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.06#
65.00	23.30	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
 Data File : VW023101.D
 Acq On : 17 May 2022 15:25
 Operator : SY/VA
 Sample : N2843-11
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4J1

Manual IntegrationsAPPROVED

Quant Time: May 18 01:29:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 18 01:26:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/18/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	337535	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	293024	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	121501	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	101614	14.673	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	58.680%		
7) Chloroethane-d5	2.885	69	91668	20.347	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.400%		
11) 1,1-Dichloroethene-d2	4.019	63	110266m	12.323	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	49.280%		
21) 2-Butanone-d5	7.080	46	59915	45.505	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	91.020%		
24) Chloroform-d	7.647	84	209880	21.224	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.880%		
26) 1,2-Dichloroethane-d4	8.305	65	121576	22.416	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	89.680%		
32) Benzene-d6	8.275	84	377407	22.345	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.400%		
36) 1,2-Dichloropropane-d6	9.274	67	119077	25.099	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	100.400%		
41) Toluene-d8	10.323	98	331339	20.308	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.240%		
43) trans-1,3-Dichloroprop...	10.579	79	43353	19.846	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.400%		
47) 2-Hexanone-d5	10.920	63	47844	52.826	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	105.660%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	111023	25.107	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	100.440%		
66) 1,2-Dichlorobenzene-d4	13.853	152	92833	21.857	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	87.440%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051722\
Data File : VW023101.D
Acq On : 17 May 2022 15:25
Operator : SY/VA
Sample : N2843-11
Misc : 6.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4J1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/18/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 18 01:29:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 18 01:26:16 2022
Response via : Initial Calibration

