

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023124.D
 Acq On : 18 May 2022 12:09
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 19 01:22:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	331441	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	318109	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	162773	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	142020	20.885	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.560%
7) Chloroethane-d5	2.885	69	97023	21.931	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.720%
11) 1,1-Dichloroethene-d2	4.019	63	147397	16.776	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.120%
21) 2-Butanone-d5	7.080	46	58058	44.905	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.820%
24) Chloroform-d	7.647	84	226641	23.340	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.360%
26) 1,2-Dichloroethane-d4	8.305	65	126992	23.845	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.360%
32) Benzene-d6	8.275	84	455123	24.822	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.280%
36) 1,2-Dichloropropane-d6	9.274	67	130253	25.289	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.160%
41) Toluene-d8	10.323	98	438444	24.754	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.000%
43) trans-1,3-Dichloroprop...	10.579	79	55101	23.235	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.920%
47) 2-Hexanone-d5	10.927	63	44415	45.173	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.340%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	117491	24.474	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	145571	25.584	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.320%
Target Compounds						
39) cis-1,3-Dichloropropene	10.036	75	4888	0.695	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023124.D
Acq On : 18 May 2022 12:09
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 19 01:22:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

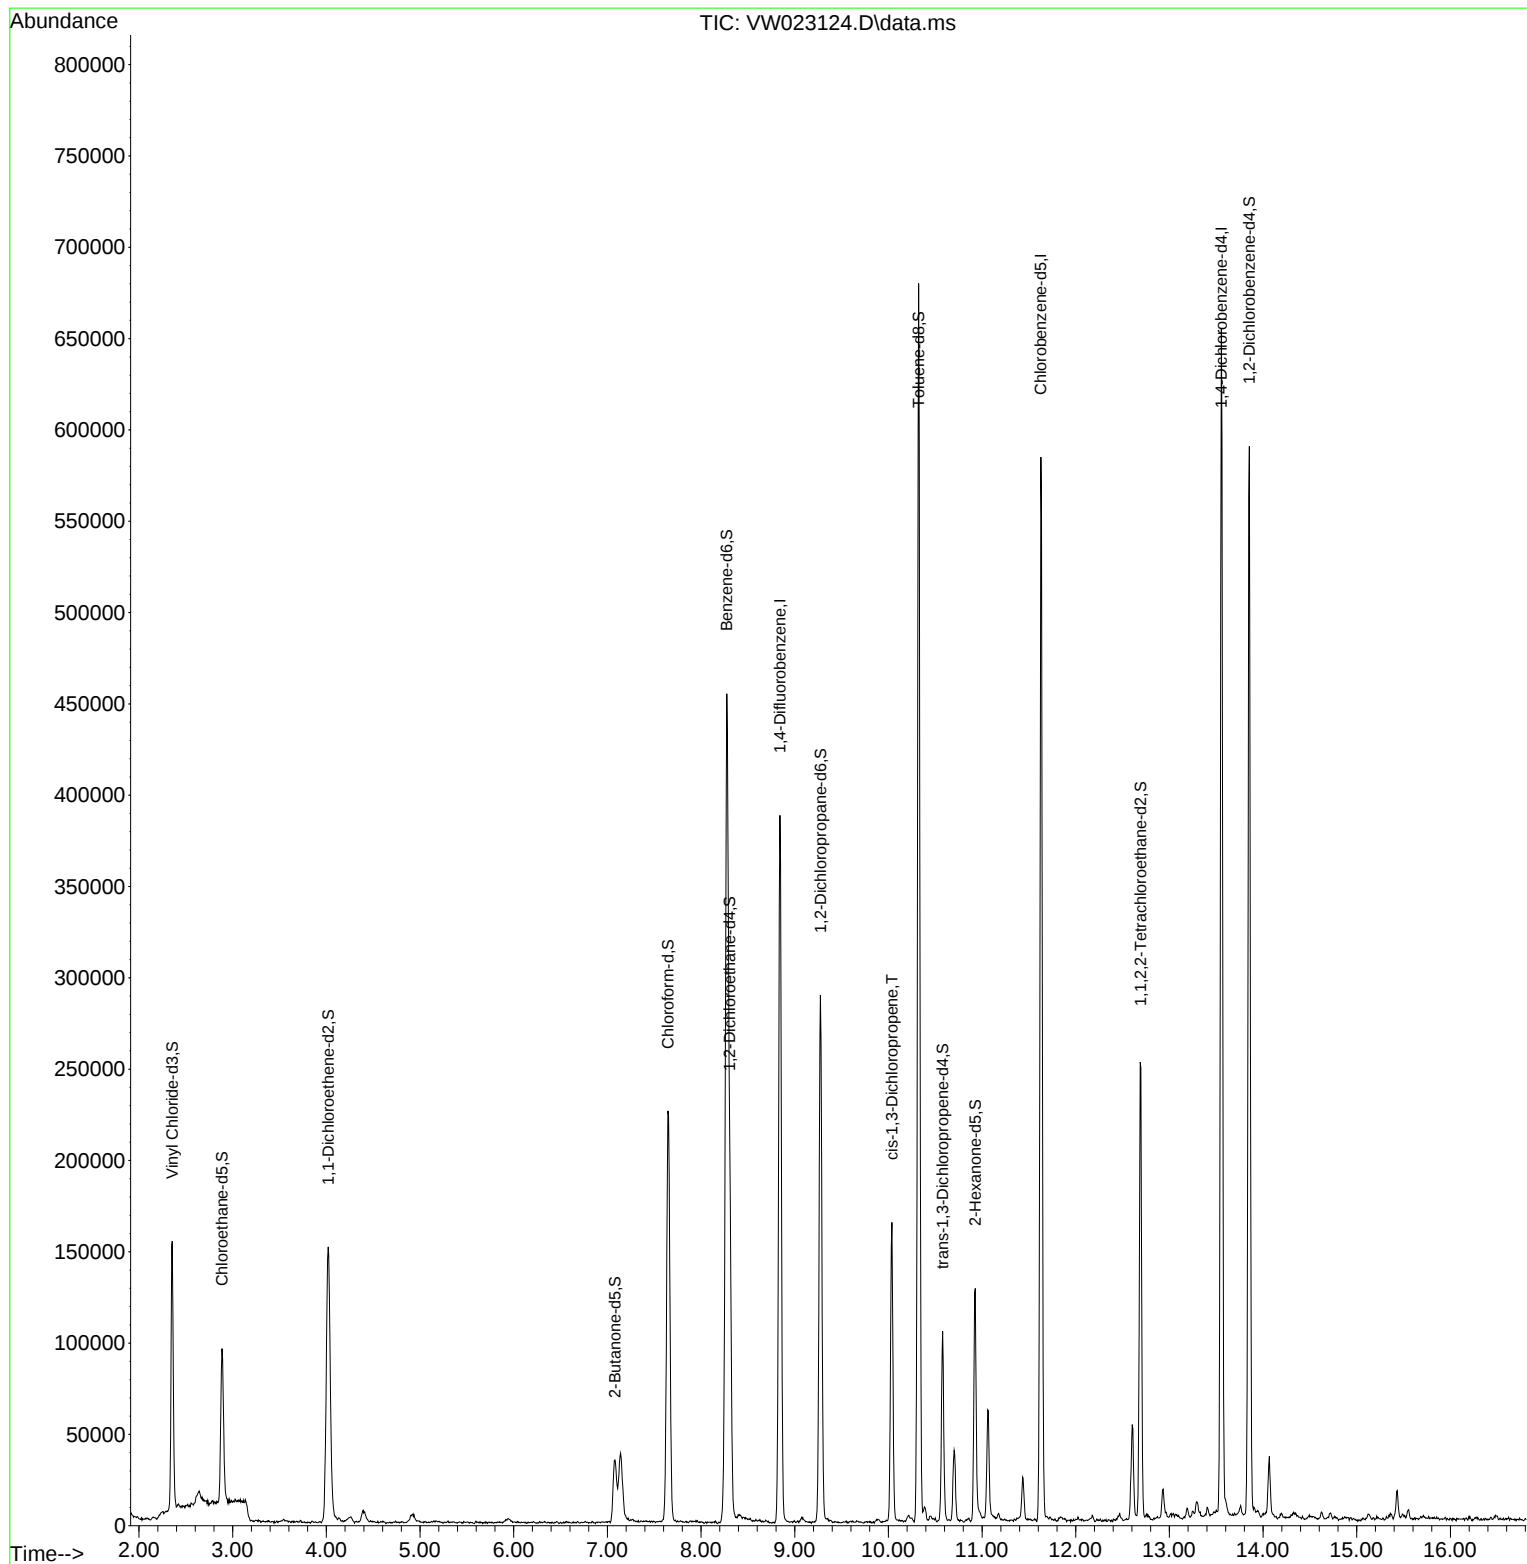

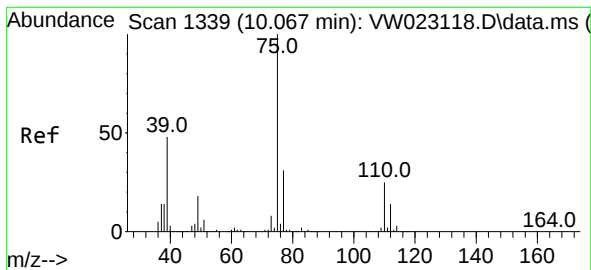

#39

cis-1,3-Dichloropropene

Concen: 0.695 ug/L

RT: 10.036 min Scan# 11

Delta R.T. -0.031 min


Lab File: VW023124.D

Acq: 18 May 2022 12:09

Instrument :

MSVOA_W

ClientSampleId :

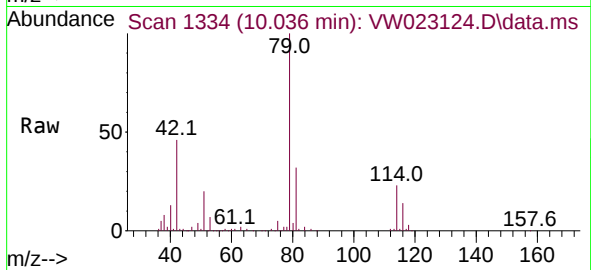

Tgt Ion: 75 Resp: 4888

Ion Ratio Lower Upper

75 100

77 35.6 22.1 41.1

