

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023125.D
 Acq On : 18 May 2022 12:33
 Operator : SY/VA
 Sample : N2883-03RE
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 19 01:23:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	219524	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	125304	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	23935	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	77313	17.166	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.680%
7) Chloroethane-d5	2.885	69	63682	21.734	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.920%
11) 1,1-Dichloroethene-d2	4.013	63	72968	12.539	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.160%
21) 2-Butanone-d5	7.214	46	156	0.182	ug/L	0.14
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.360%#
24) Chloroform-d	7.653	84	156675	24.360	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.440%
26) 1,2-Dichloroethane-d4	8.305	65	90994	25.796	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	8.275	84	263975	36.549	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	146.200%#
36) 1,2-Dichloropropane-d6	9.274	67	88016	43.383	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	173.520%#
41) Toluene-d8	10.323	98	175806	25.198	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.800%
43) trans-1,3-Dichloroprop...	10.579	79	22688	24.288	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.160%
47) 2-Hexanone-d5	10.927	63	39750	102.635	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	205.260%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	79342	41.958	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	167.840%#
66) 1,2-Dichlorobenzene-d4	13.853	152	24653	29.465	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	117.880%
Target Compounds						Qvalue
13) Acetone	4.129	43	7742	12.076	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023125.D
Acq On : 18 May 2022 12:33
Operator : SY/VA
Sample : N2883-03RE
Misc : 6.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 19 01:23:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

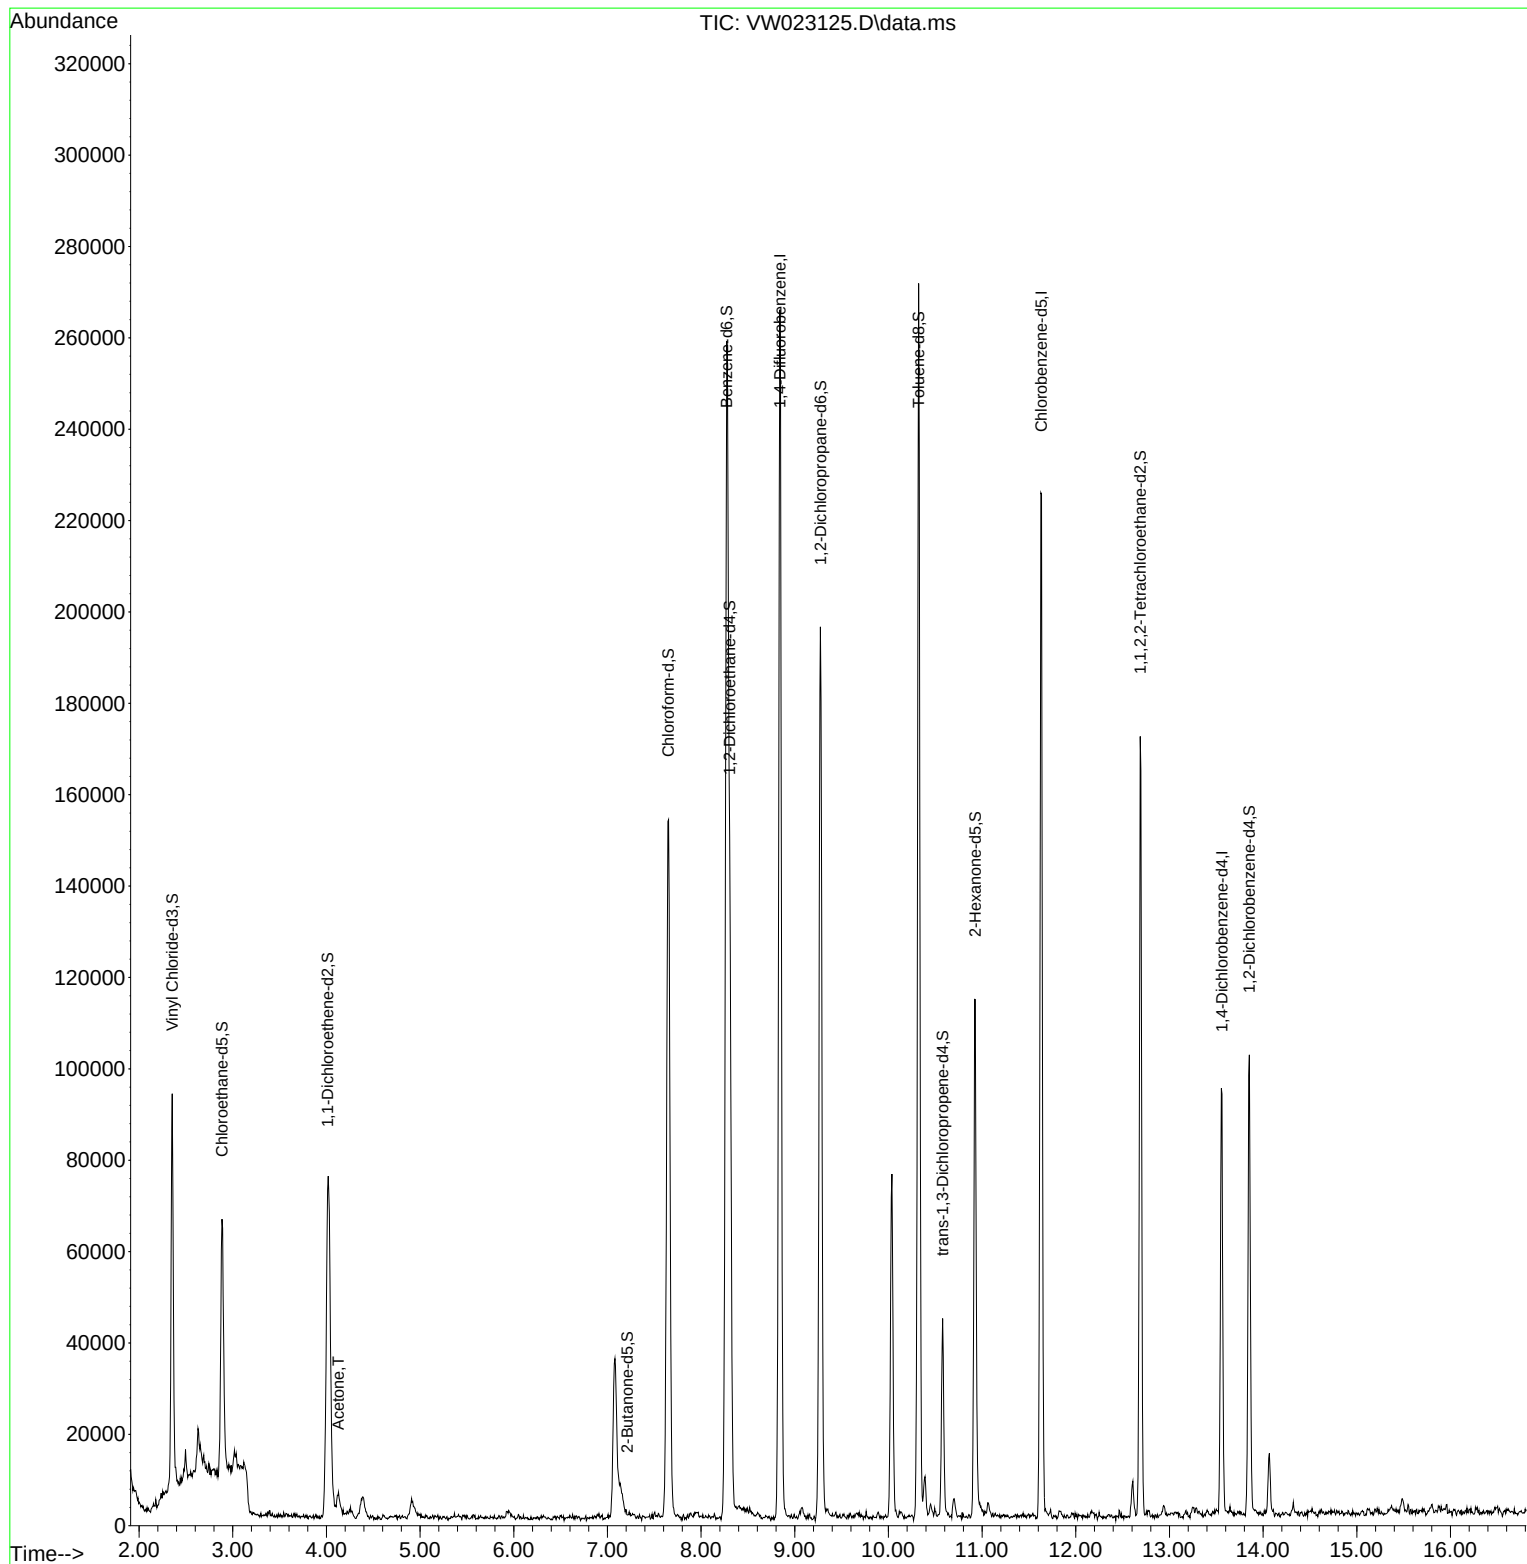

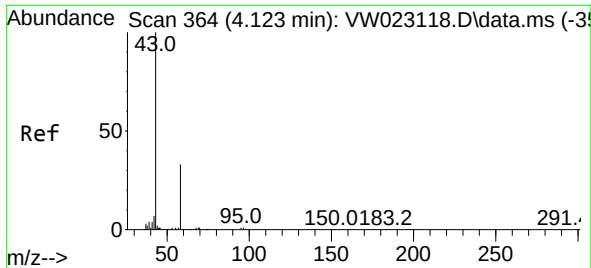

#13

Acetone

Concen: 12.076 ug/L

RT: 4.129 min Scan# 30

Delta R.T. 0.006 min


Lab File: VW023125.D

Acq: 18 May 2022 12:33

Instrument :

MSVOA_W

ClientSampleId :

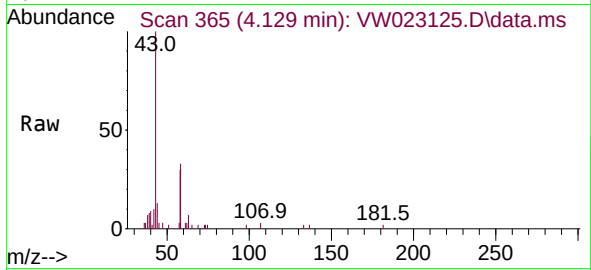

Tgt Ion: 43 Resp: 7742

Ion Ratio Lower Upper

43 100

58 23.7 0.0 64.0

