

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023132.D
 Acq On : 18 May 2022 15:22
 Operator : SY/VA
 Sample : N2860-02
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 19 01:24:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	237675	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	234928	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	118567	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	67164	13.774	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.080%
7) Chloroethane-d5	2.885	69	50938	16.057	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.240%
11) 1,1-Dichloroethene-d2	4.013	63	71099	11.284	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	45.120%
21) 2-Butanone-d5	7.080	46	68832	74.242	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	148.480%#
24) Chloroform-d	7.647	84	142997	20.536	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.160%
26) 1,2-Dichloroethane-d4	8.305	65	91502	23.959	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.840%
32) Benzene-d6	8.275	84	257037	18.982	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.920%
36) 1,2-Dichloropropane-d6	9.274	67	82454	21.677	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.720%
41) Toluene-d8	10.323	98	233119	17.822	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.280%
43) trans-1,3-Dichloroprop...	10.579	79	33661	19.220	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.880%
47) 2-Hexanone-d5	10.920	63	54374	74.882	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	149.760%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	107448	30.307	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.240%#
66) 1,2-Dichlorobenzene-d4	13.853	152	94775	22.867	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.480%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	3144	0.605	ug/L #	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023132.D
Acq On : 18 May 2022 15:22
Operator : SY/VA
Sample : N2860-02
Misc : 7.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 19 01:24:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

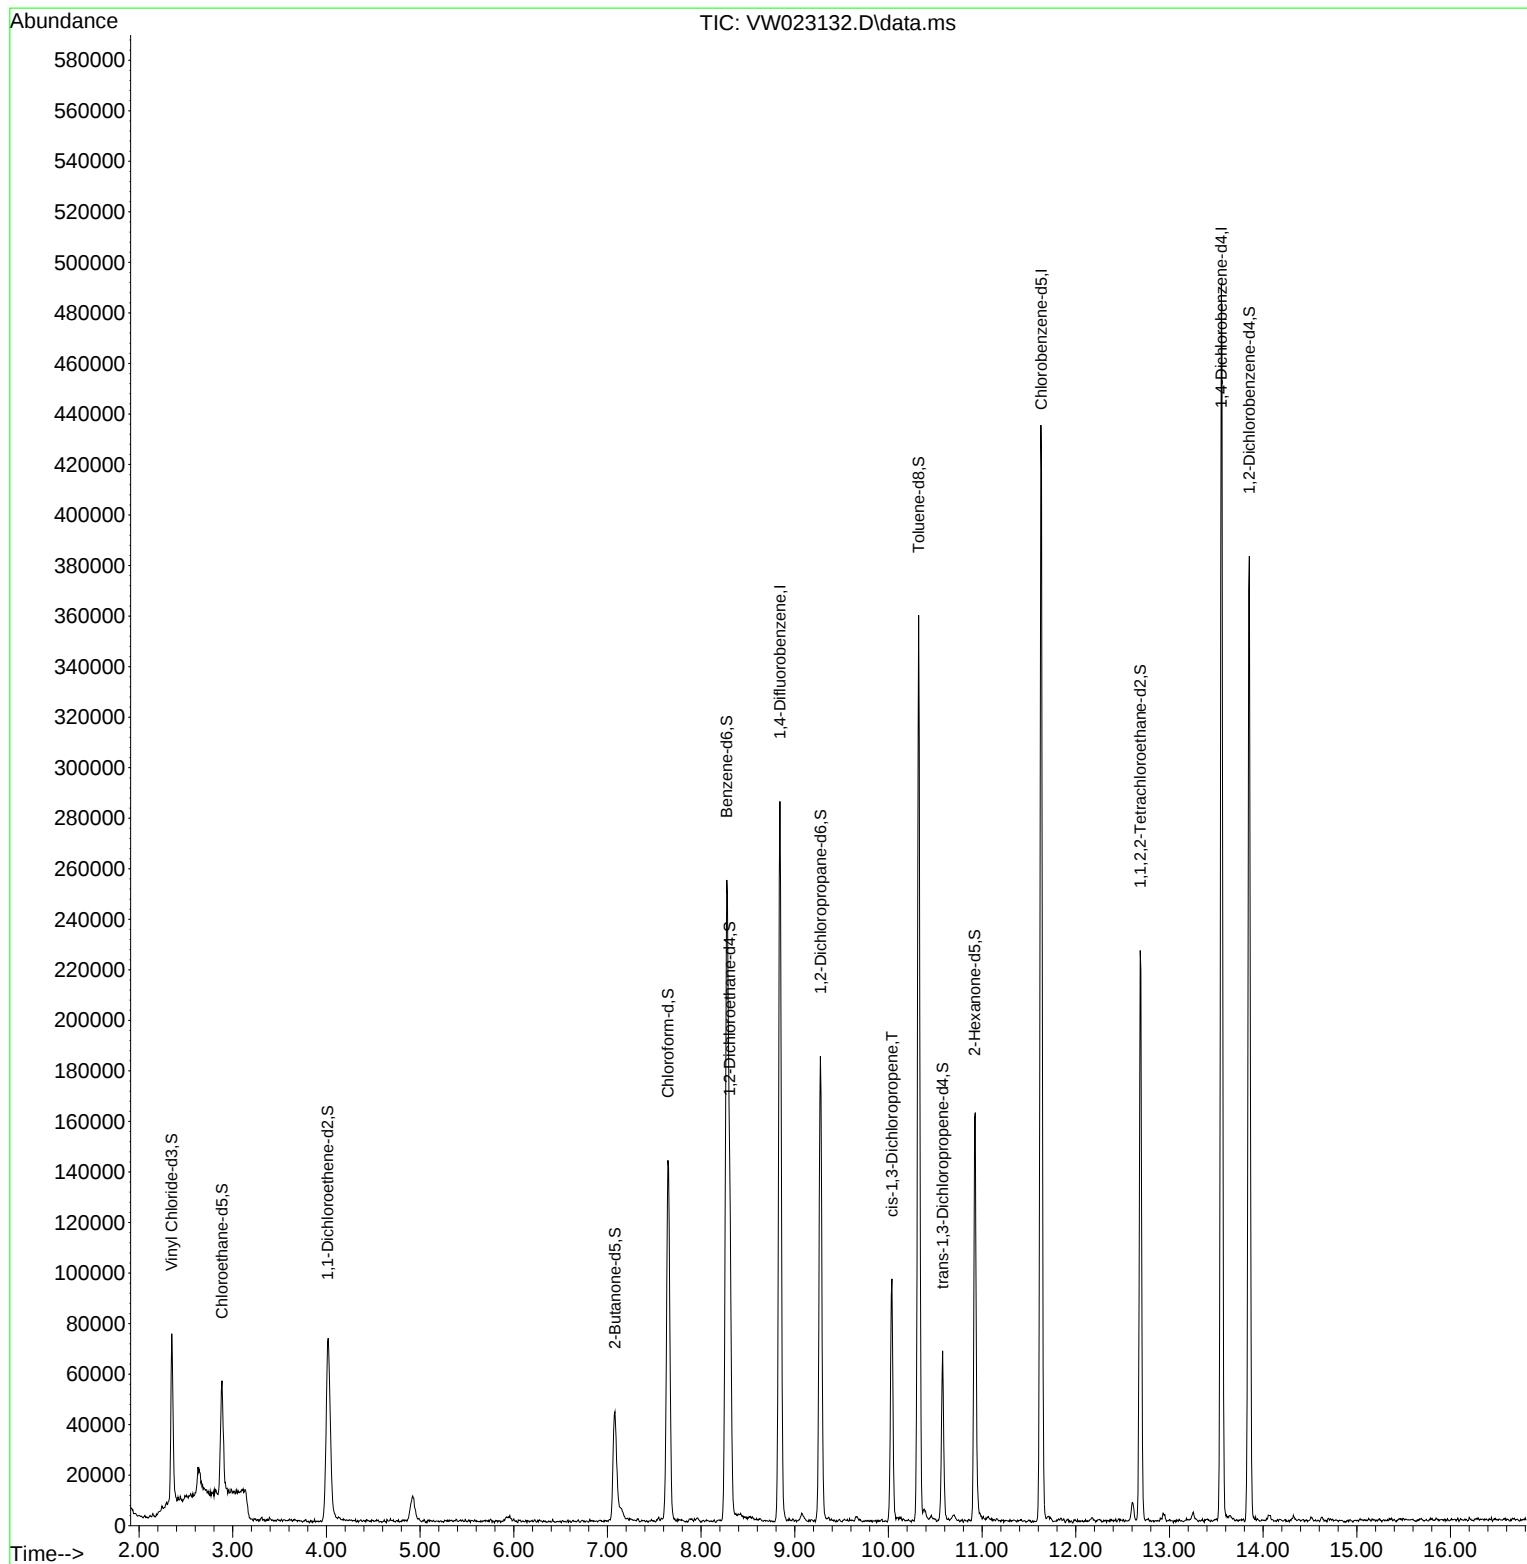

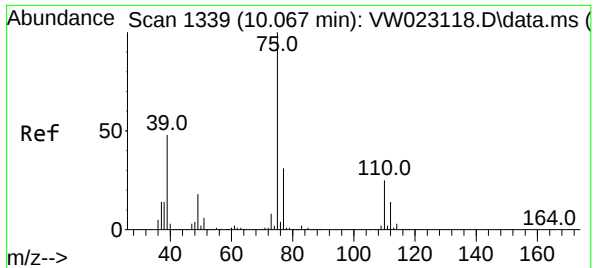

#39
 cis-1,3-Dichloropropene
 Concen: 0.605 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.031 min
 Lab File: VW023132.D
 Acq: 18 May 2022 15:22

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3144
 Ion Ratio Lower Upper
 75 100
 77 45.7 22.1 41.1#

