

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023136.D
 Acq On : 18 May 2022 16:59
 Operator : SY/VA
 Sample : N2926-01
 Misc : 4.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 19 01:25:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	320215	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	296817	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	135389	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	86186	13.119	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.480%
7) Chloroethane-d5	2.885	69	71845	16.809	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.240%
11) 1,1-Dichloroethene-d2	4.147	63	262	0.031	ug/L	0.13
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.120%#
21) 2-Butanone-d5	7.250	46	200	0.160	ug/L	0.18
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.320%#
24) Chloroform-d	7.653	84	191195	20.380	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.520%
26) 1,2-Dichloroethane-d4	8.305	65	105059	20.418	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.680%
32) Benzene-d6	8.275	84	338092	19.762	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.040%
36) 1,2-Dichloropropane-d6	9.274	67	106854	22.234	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.920%
41) Toluene-d8	10.323	98	304067	18.398	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.600%
43) trans-1,3-Dichloroprop...	10.579	79	38420	17.363	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.440%
47) 2-Hexanone-d5	10.920	63	48540	52.910	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.820%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	104842	23.406	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.640%
66) 1,2-Dichlorobenzene-d4	13.853	152	105939	22.384	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.520%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	3924	0.598	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023136.D
Acq On : 18 May 2022 16:59
Operator : SY/VA
Sample : N2926-01
Misc : 4.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 19 01:25:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

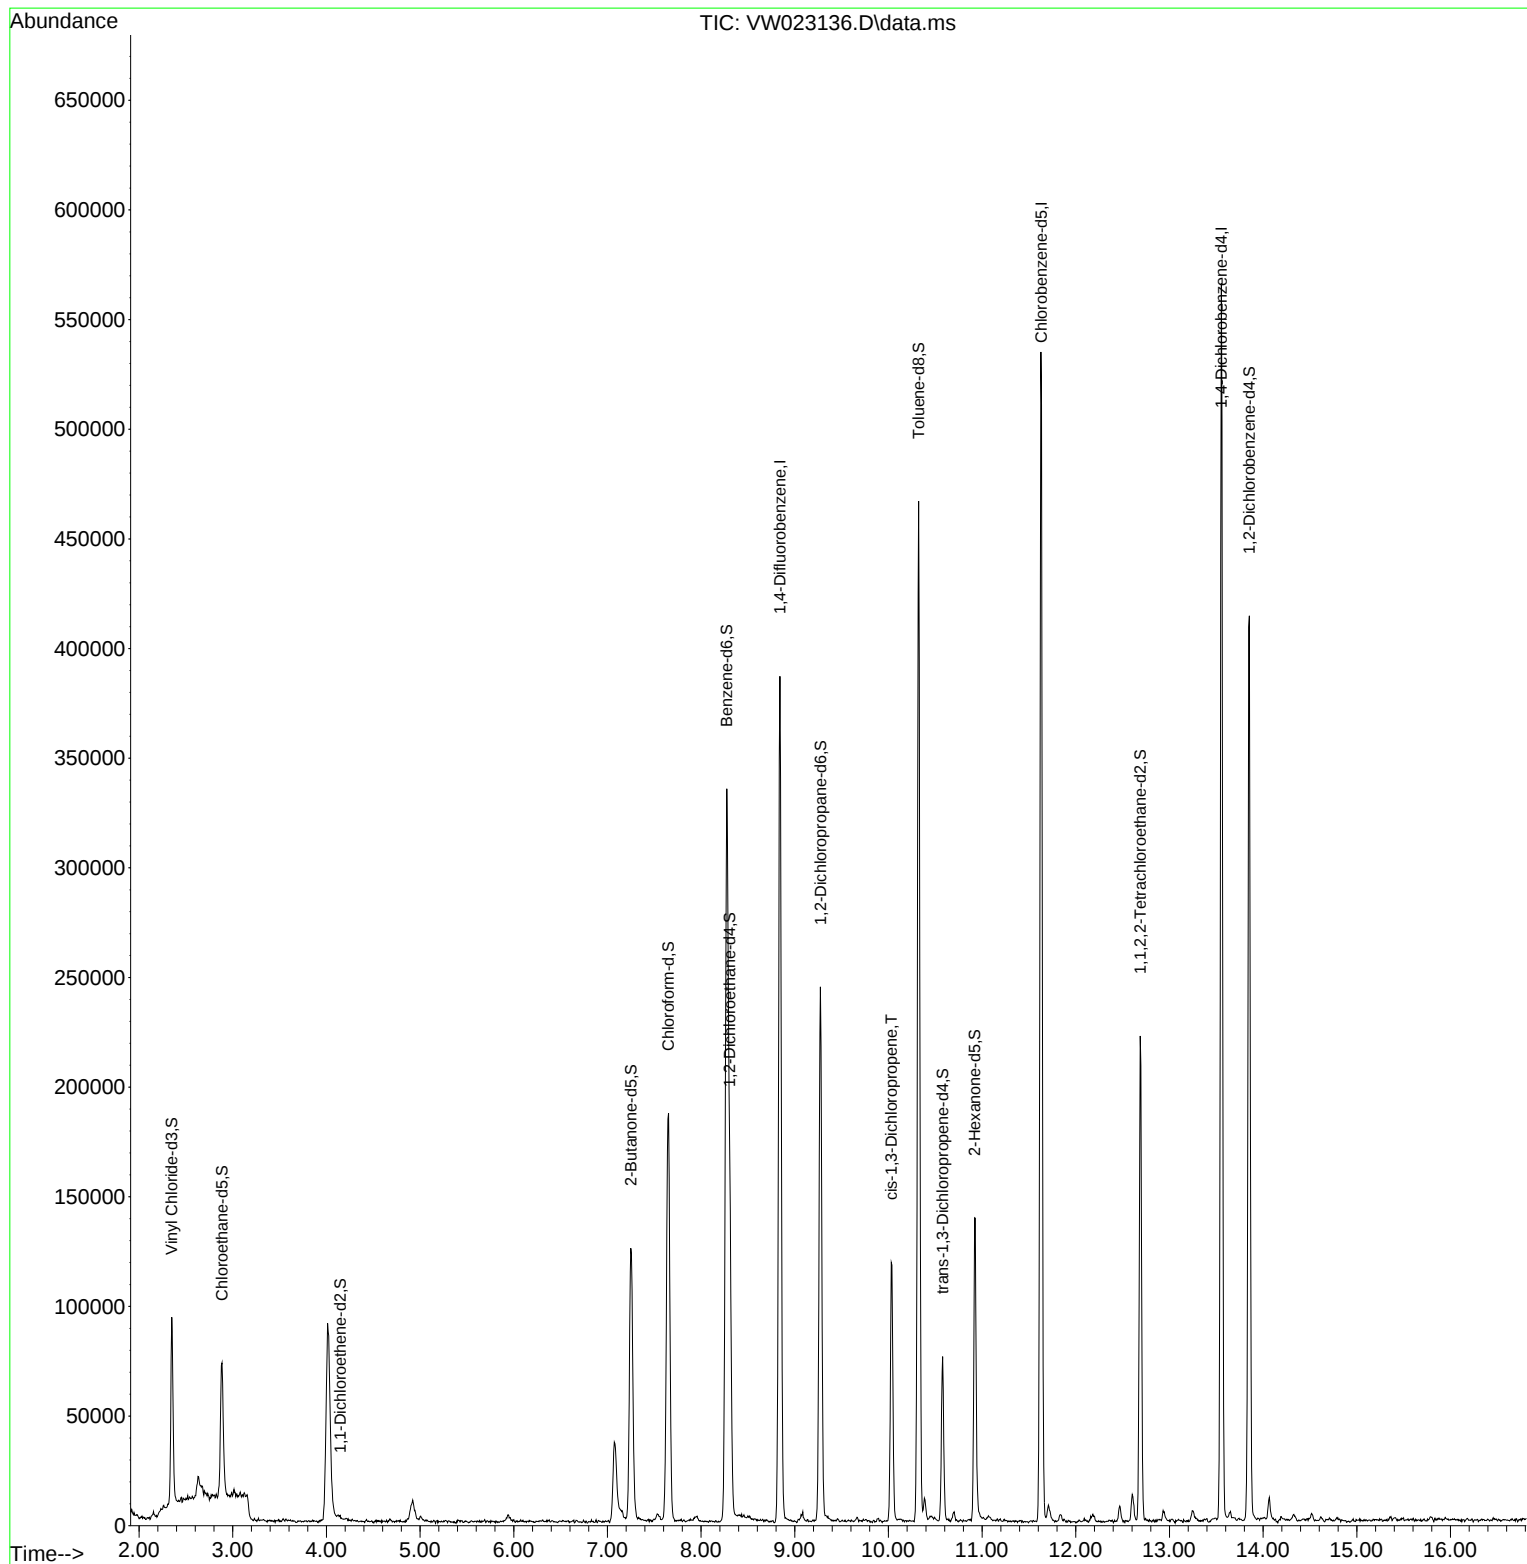

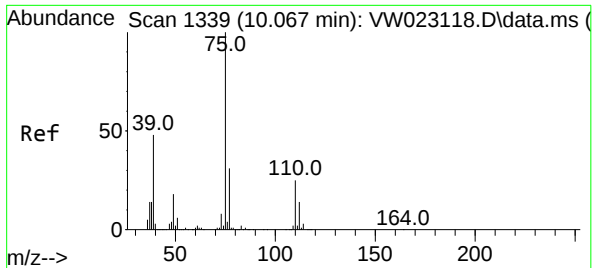

#39
 cis-1,3-Dichloropropene
 Concen: 0.598 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023136.D
 Acq: 18 May 2022 16:59

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3924
 Ion Ratio Lower Upper
 75 100
 77 36.6 22.1 41.1

