

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023138.D
 Acq On : 18 May 2022 17:47
 Operator : SY/VA
 Sample : N2848-02
 Misc : 6.46g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 19 01:25:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	235334	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	229956	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	108343	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	63282	13.107	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.440%
7) Chloroethane-d5	2.885	69	52026	16.563	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.240%
11) 1,1-Dichloroethene-d2	4.019	63	64929	10.408	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	41.640%#
21) 2-Butanone-d5	7.080	46	65513	71.365	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	142.740%#
24) Chloroform-d	7.647	84	135338	19.629	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.520%
26) 1,2-Dichloroethane-d4	8.305	65	84537	22.355	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.440%
32) Benzene-d6	8.275	84	239349	18.058	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	72.240%
36) 1,2-Dichloropropane-d6	9.274	67	76446	20.532	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.120%
41) Toluene-d8	10.323	98	218526	17.067	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.280%
43) trans-1,3-Dichloroprop...	10.579	79	30673	17.892	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.560%
47) 2-Hexanone-d5	10.927	63	49512	69.661	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	139.320%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	97321	28.044	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	112.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	77313	20.414	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.640%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	2601	0.512	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023138.D
Acq On : 18 May 2022 17:47
Operator : SY/VA
Sample : N2848-02
Misc : 6.46g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 19 01:25:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

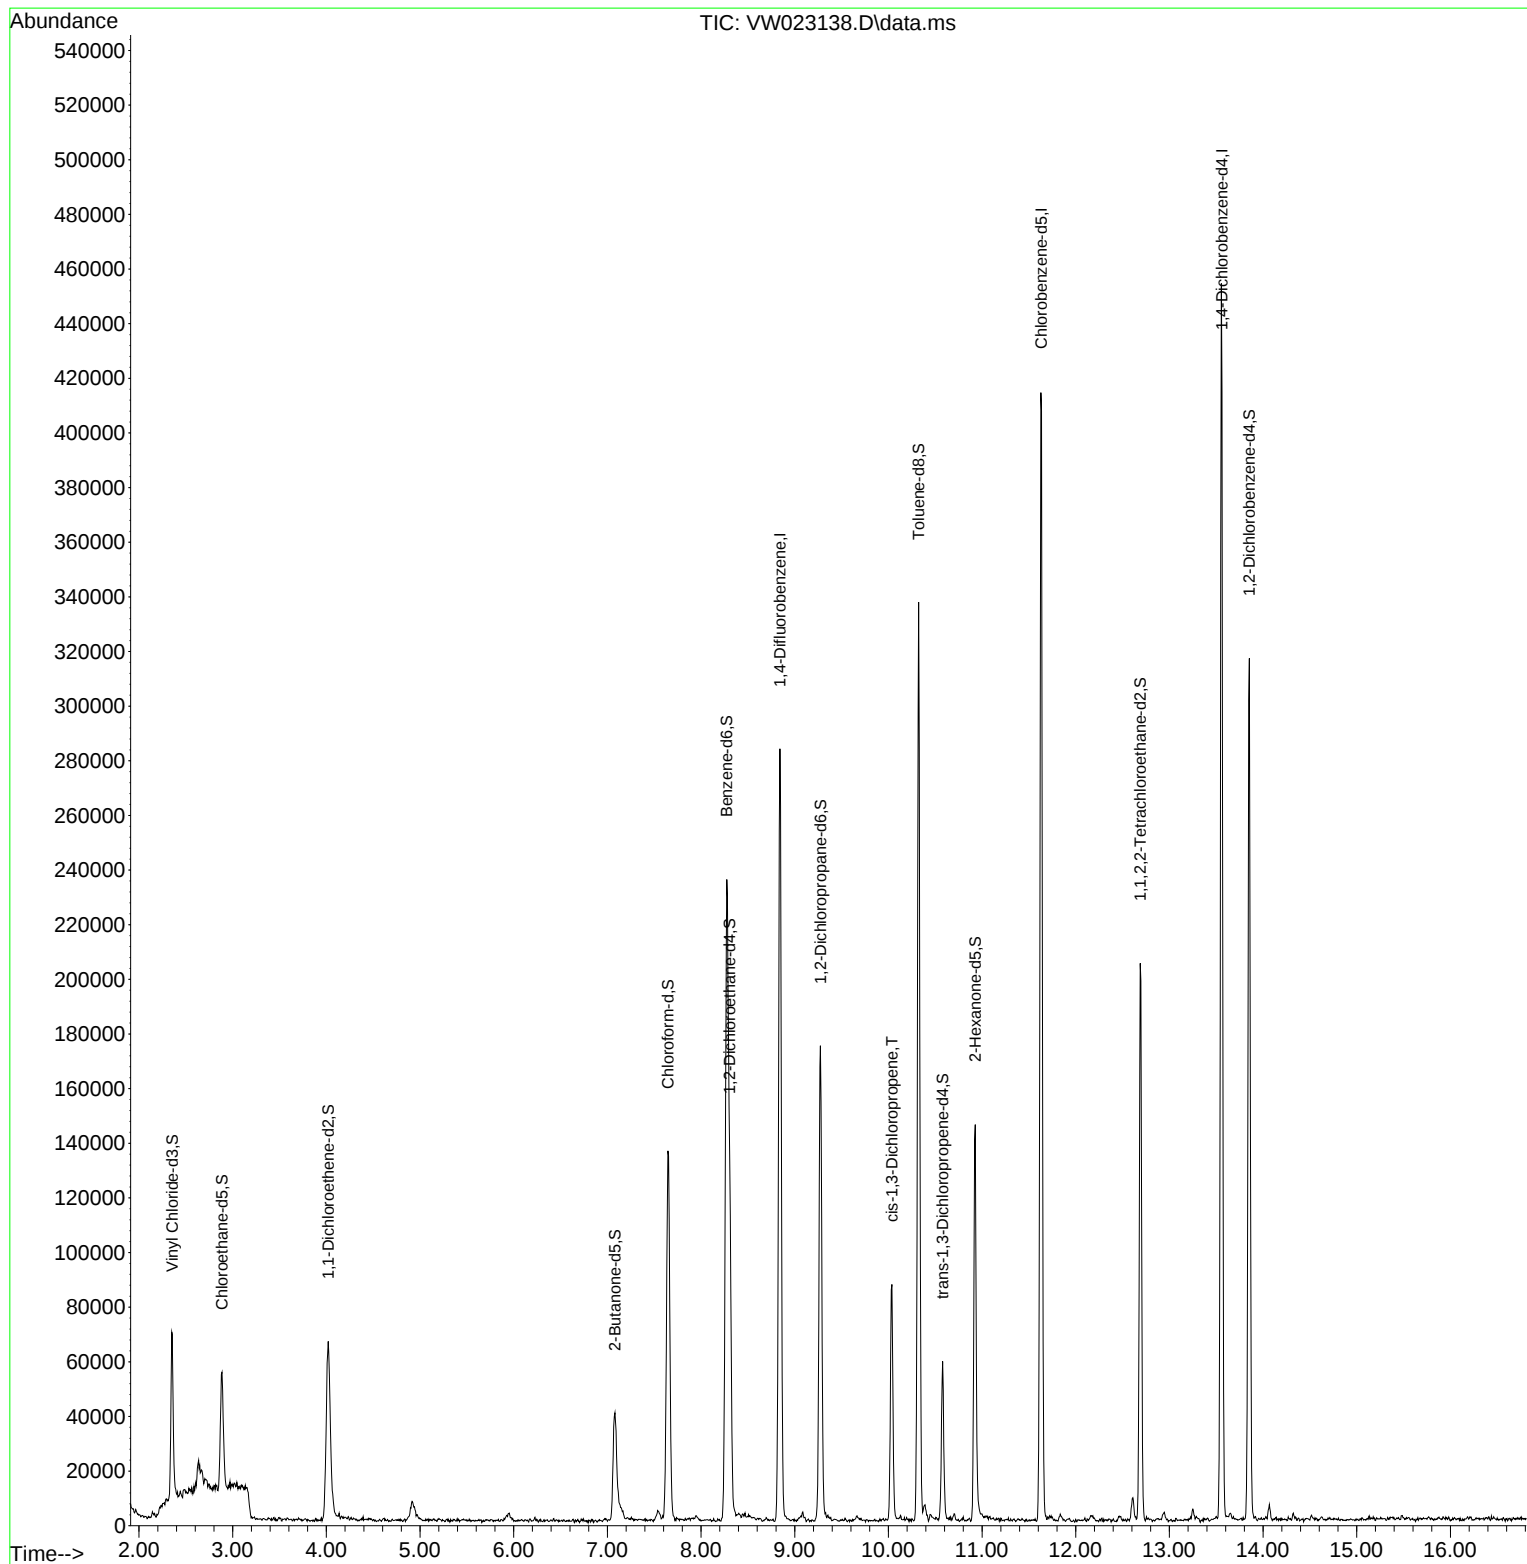

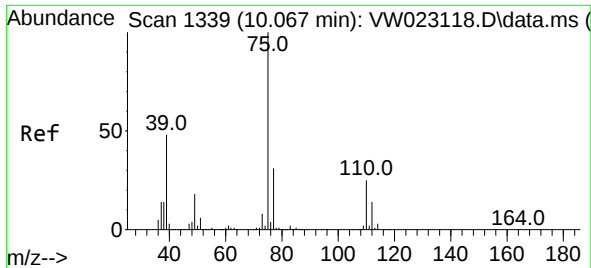

#39

cis-1,3-Dichloropropene

Concen: 0.512 ug/L

RT: 10.037 min Scan# 11

Delta R.T. -0.031 min


Lab File: VW023138.D

Acq: 18 May 2022 17:47

Instrument :

MSVOA_W

ClientSampleId :

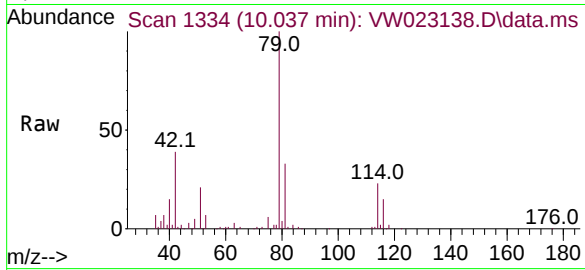

Tgt Ion: 75 Resp: 2601

Ion Ratio Lower Upper

75 100

77 37.9 22.1 41.1

