

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023151.D
 Acq On : 19 May 2022 00:05
 Operator : SY/VA
 Sample : N2848-10
 Misc : 4.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 19 04:55:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 04:23:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	298314	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	280110	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	115026	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	85132	13.910	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.640%
7) Chloroethane-d5	2.885	69	67366	16.919	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.680%
11) 1,1-Dichloroethene-d2	4.141	63	271	0.034	ug/L	0.12
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.120%#
21) 2-Butanone-d5	7.080	46	53817	46.248	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.500%
24) Chloroform-d	7.653	84	197019	22.542	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.160%
26) 1,2-Dichloroethane-d4	8.305	65	108679	22.672	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.680%
32) Benzene-d6	8.275	84	352120	21.809	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.240%
36) 1,2-Dichloropropane-d6	9.274	67	109184	24.074	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.280%
41) Toluene-d8	10.323	98	312781	20.055	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.200%
43) trans-1,3-Dichloroprop...	10.579	79	36837	17.640	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.560%
47) 2-Hexanone-d5	10.927	63	40204	46.437	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.880%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	101181	23.936	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	98302	24.448	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.800%
Target Compounds						
39) cis-1,3-Dichloropropene	10.036	75	3560	0.575	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023151.D
Acq On : 19 May 2022 00:05
Operator : SY/VA
Sample : N2848-10
Misc : 4.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 19 04:55:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 04:23:21 2022
Response via : Initial Calibration

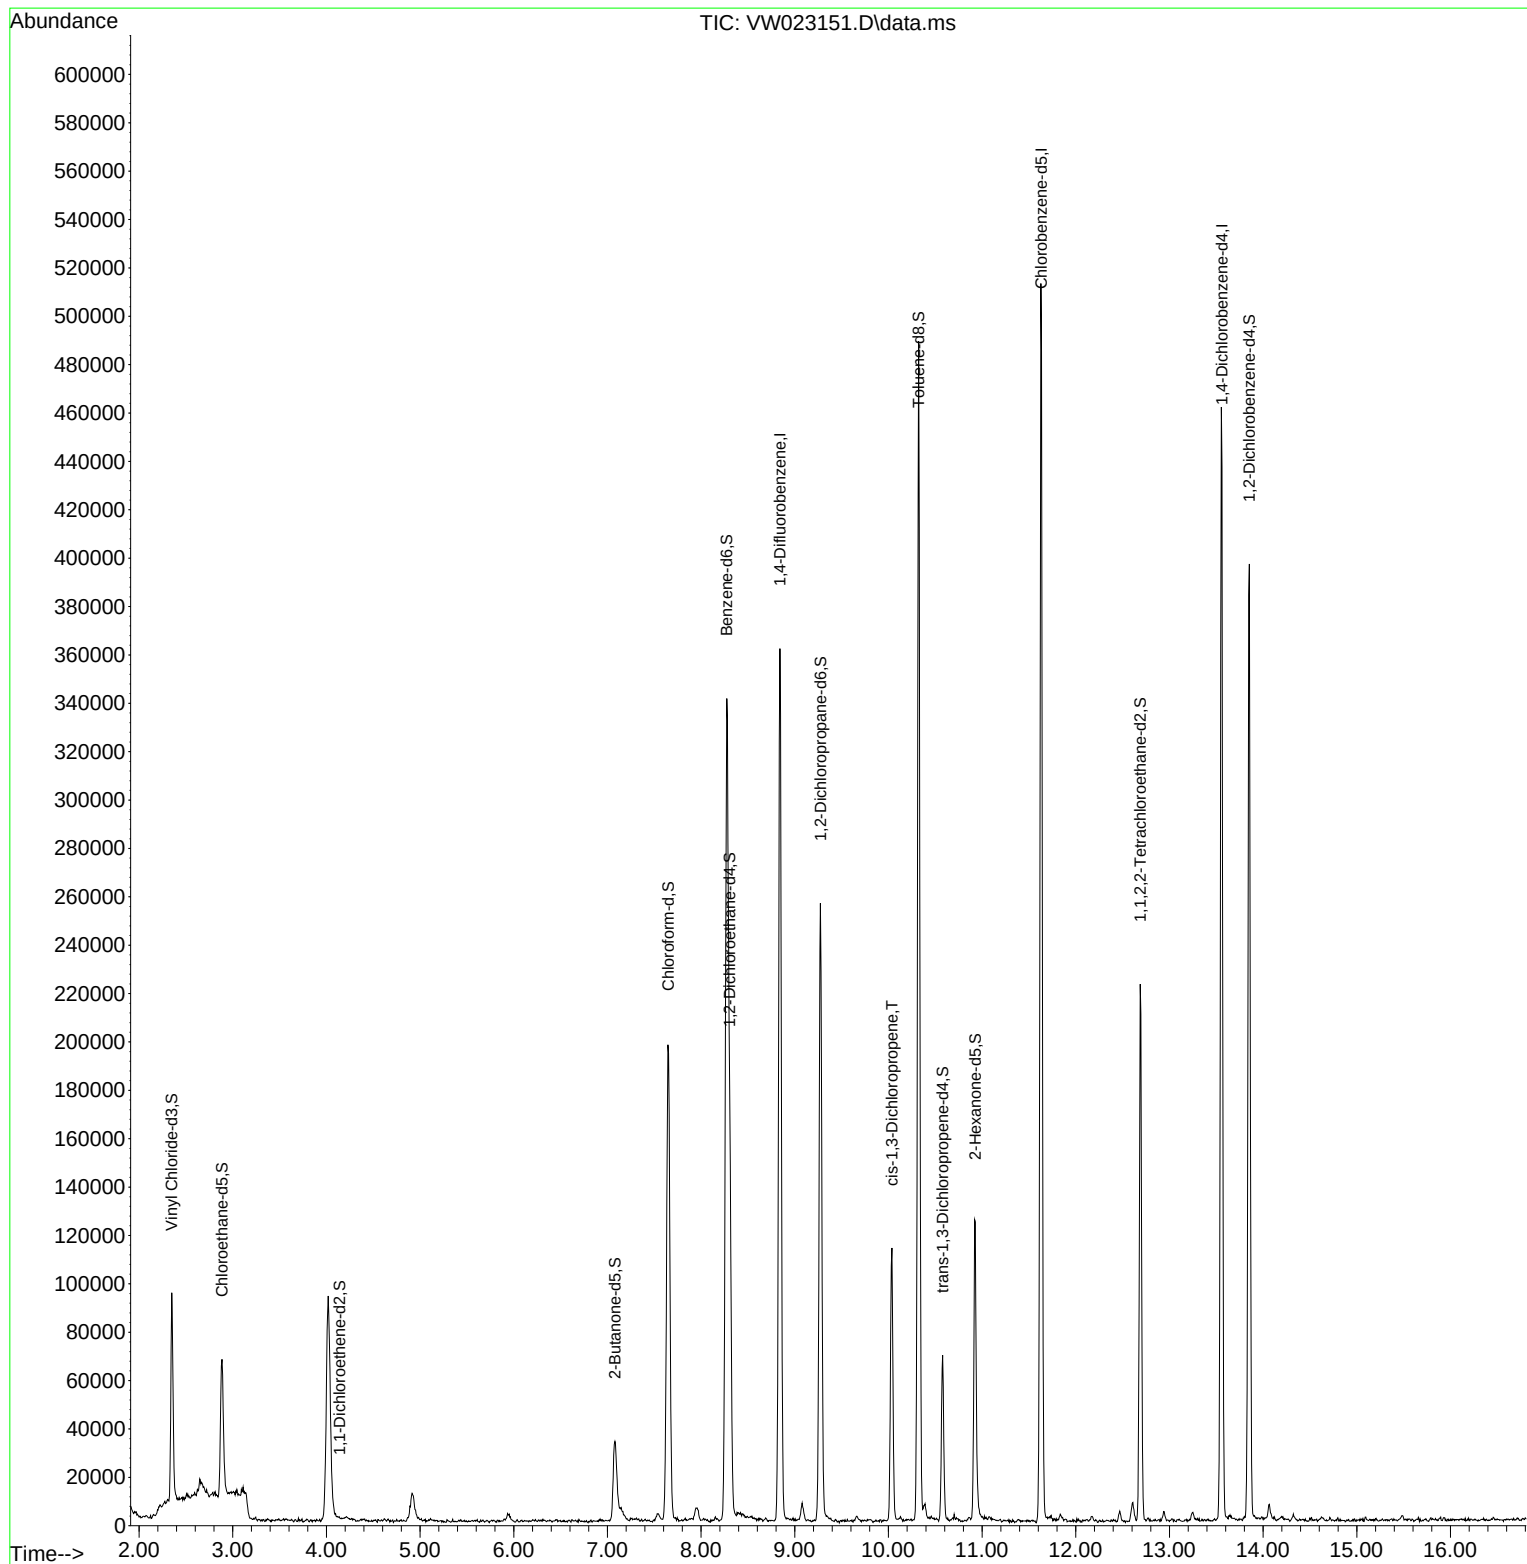

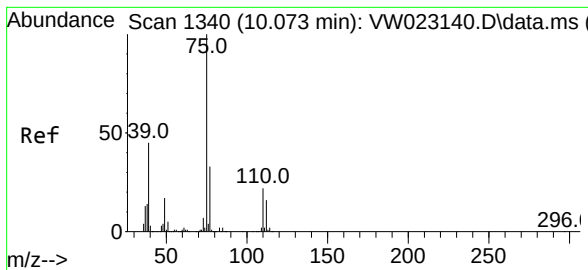

#39
 cis-1,3-Dichloropropene
 Concen: 0.575 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023151.D
 Acq: 19 May 2022 00:05

Instrument :
 MSVOA_W
 ClientSampleId :

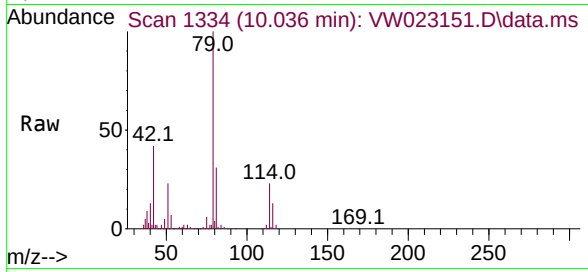

Tgt Ion	Ratio	Lower	Upper
75	100		
77	39.2	22.1	41.1

