

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023156.D
 Acq On : 19 May 2022 02:05
 Operator : SY/VA
 Sample : N2848-18
 Misc : 4.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 19 04:56:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 04:23:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	289592	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	286900	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	108954	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	80381	13.529	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.120%
7) Chloroethane-d5	2.885	69	65308	16.896	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.600%
11) 1,1-Dichloroethene-d2	4.019	63	83010	10.813	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.240%#
21) 2-Butanone-d5	7.079	46	50256	44.488	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.980%
24) Chloroform-d	7.652	84	182604	21.522	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.080%
26) 1,2-Dichloroethane-d4	8.305	65	106296	22.843	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.360%
32) Benzene-d6	8.274	84	319928	19.347	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.400%
36) 1,2-Dichloropropane-d6	9.274	67	103448	22.270	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.080%
41) Toluene-d8	10.323	98	273682	17.132	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.520%
43) trans-1,3-Dichloroprop...	10.579	79	35691	16.687	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.760%
47) 2-Hexanone-d5	10.926	63	41196	46.457	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.920%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	107794	24.897	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	84036	22.064	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.240%
Target Compounds						
39) cis-1,3-Dichloropropene	10.030	75	3500	0.552	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023156.D
Acq On : 19 May 2022 02:05
Operator : SY/VA
Sample : N2848-18
Misc : 4.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 19 04:56:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 04:23:21 2022
Response via : Initial Calibration

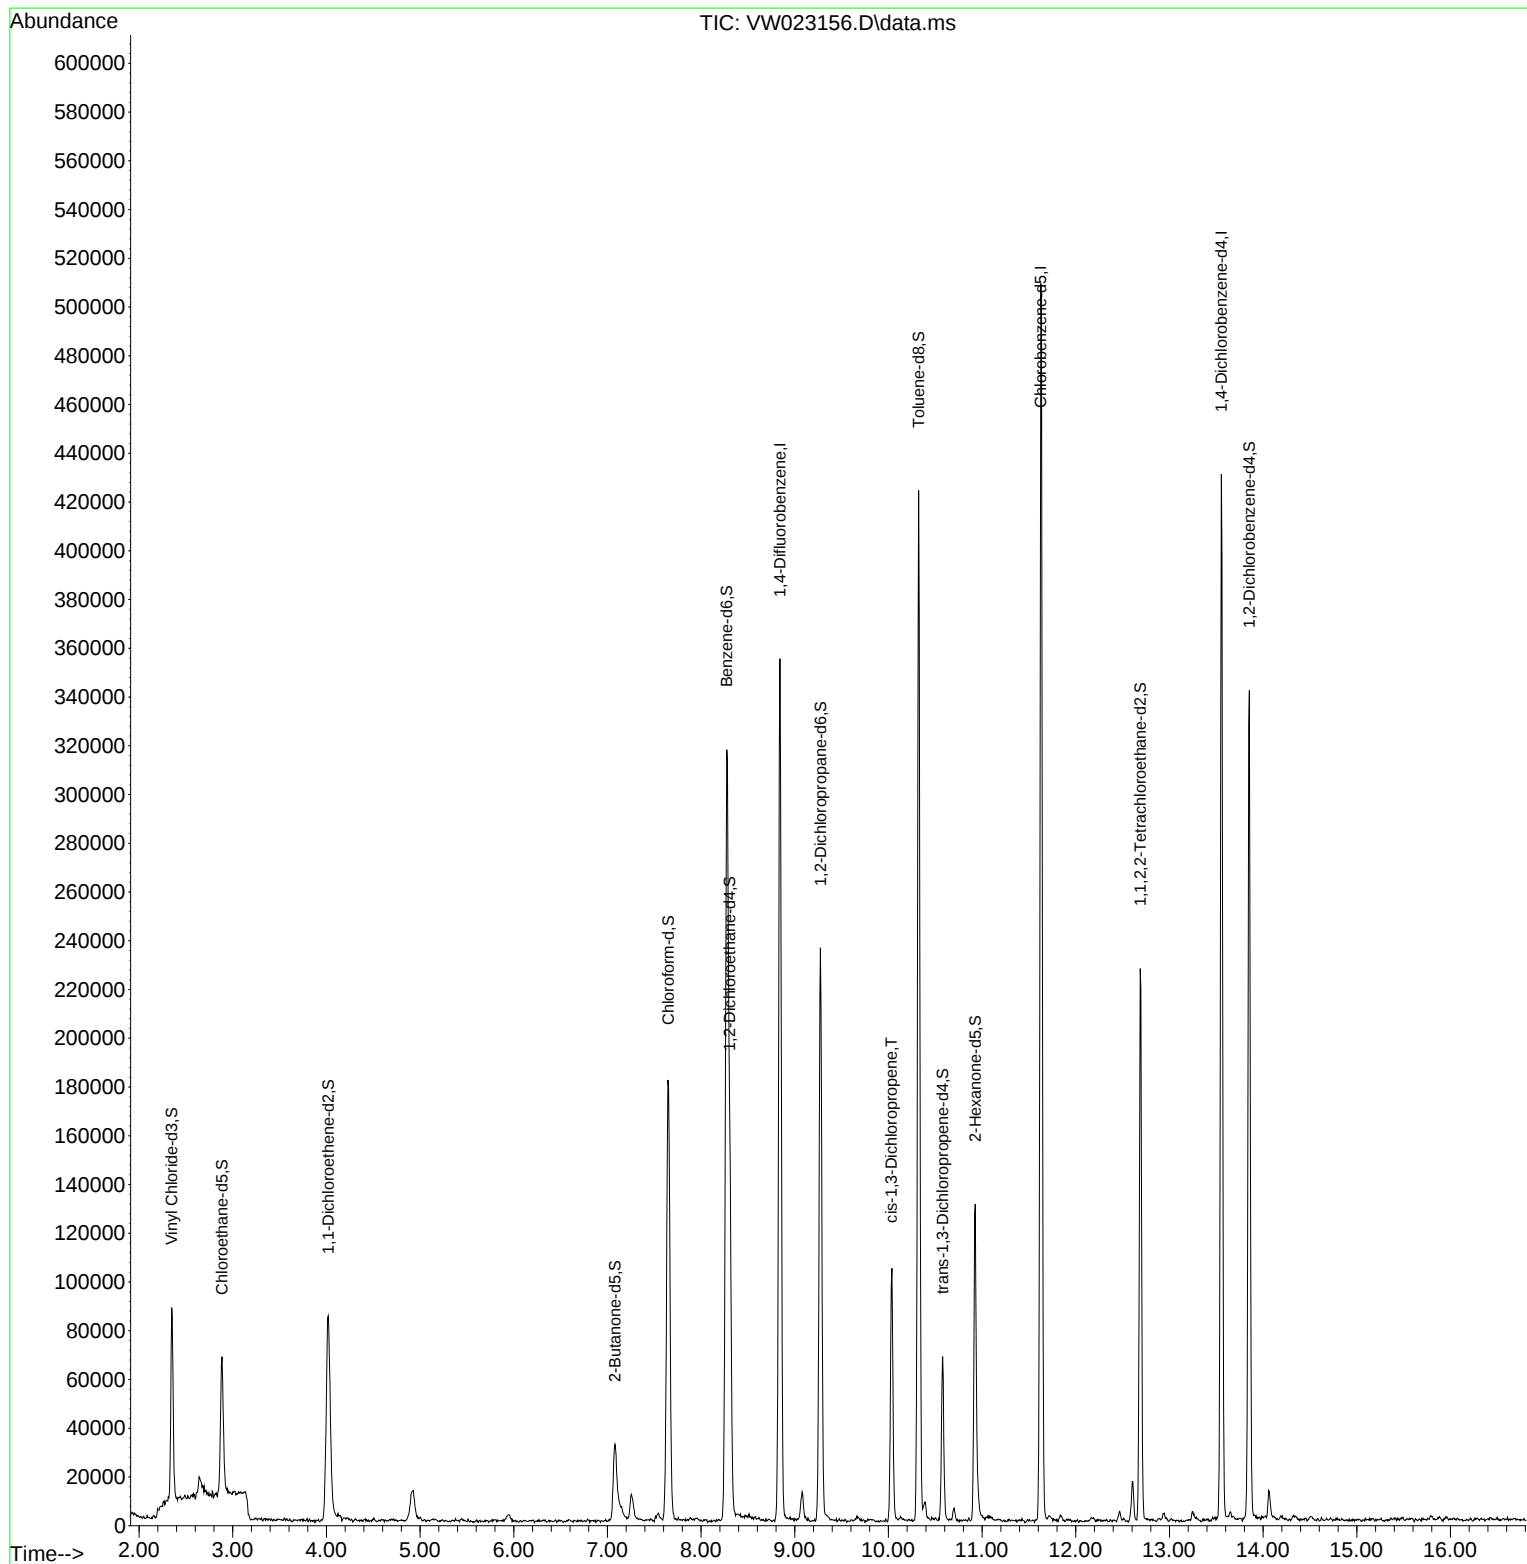

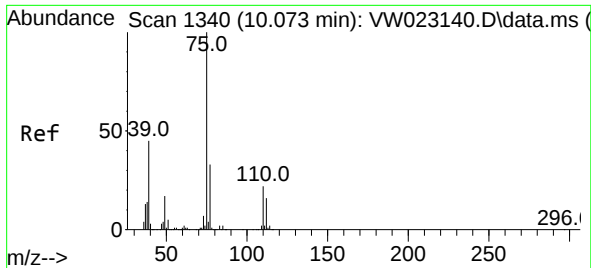

#39
 cis-1,3-Dichloropropene
 Concen: 0.552 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW023156.D
 Acq: 19 May 2022 02:05

Instrument :
 MSVOA_W
 ClientSampleId :

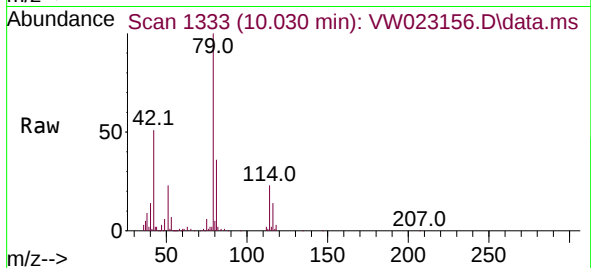

Tgt Ion: 75 Resp: 3500
 Ion Ratio Lower Upper
 75 100
 77 34.4 22.1 41.1

