

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023157.D
 Acq On : 19 May 2022 02:29
 Operator : SY/VA
 Sample : N2848-19
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 19 04:56:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 04:23:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	309309	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	292941	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	126583	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	77895	12.275	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	49.080%
7) Chloroethane-d5	2.885	69	69649	16.870	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.480%
11) 1,1-Dichloroethene-d2	4.019	63	85826	10.467	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	41.880%#
21) 2-Butanone-d5	7.080	46	60047	49.767	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.540%
24) Chloroform-d	7.647	84	195579	21.582	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.320%
26) 1,2-Dichloroethane-d4	8.305	65	113066	22.749	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.000%
32) Benzene-d6	8.275	84	341775	20.241	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.960%
36) 1,2-Dichloropropane-d6	9.274	67	107985	22.767	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.080%
41) Toluene-d8	10.323	98	300529	18.425	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.720%
43) trans-1,3-Dichloroprop...	10.579	79	38667	17.706	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.840%
47) 2-Hexanone-d5	10.927	63	43663	48.223	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.440%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	101293	22.913	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.640%
66) 1,2-Dichlorobenzene-d4	13.853	152	97177	21.961	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.840%
Target Compounds						
39) cis-1,3-Dichloropropene	10.043	75	3697	0.571	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023157.D
Acq On : 19 May 2022 02:29
Operator : SY/VA
Sample : N2848-19
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 19 04:56:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 04:23:21 2022
Response via : Initial Calibration

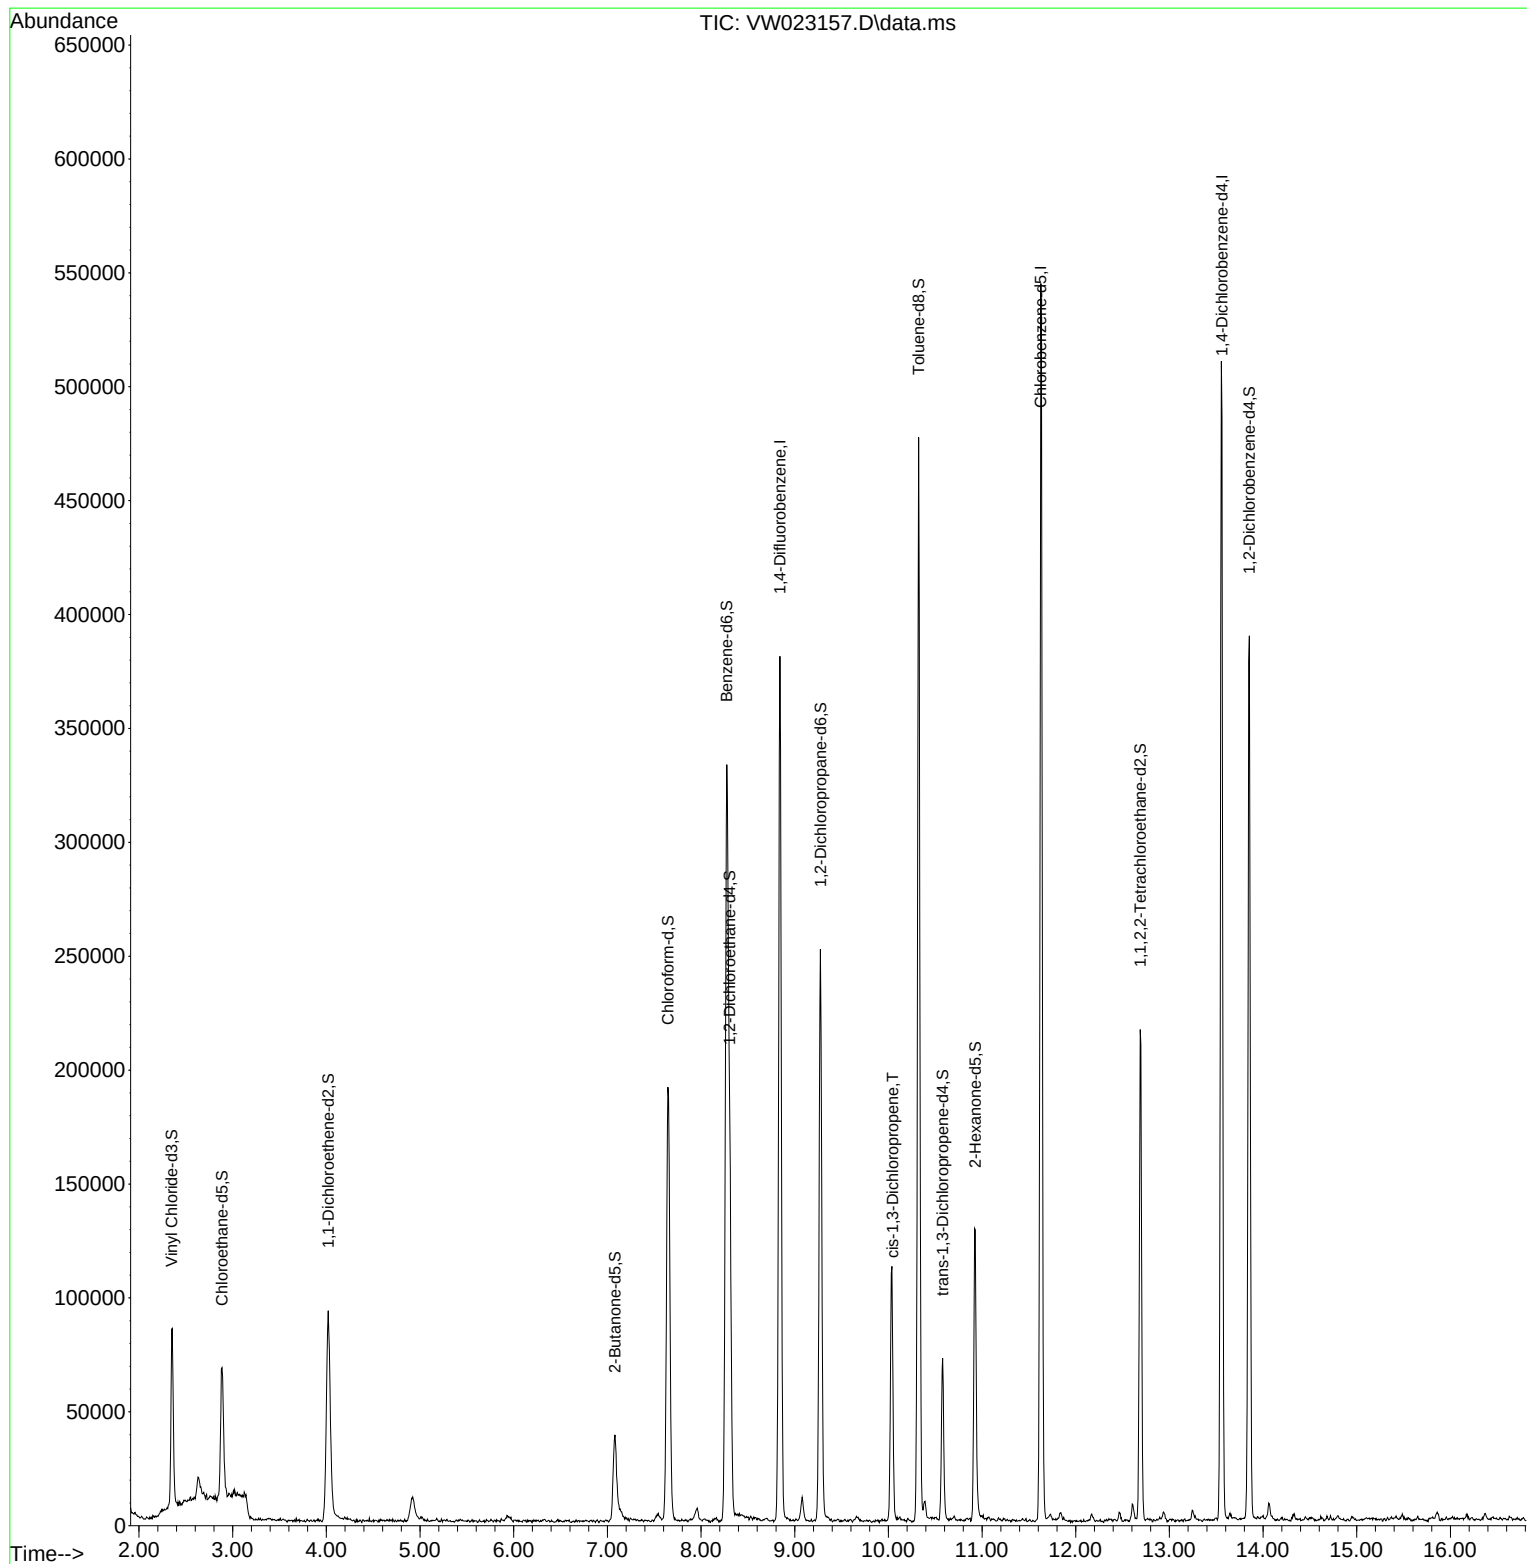

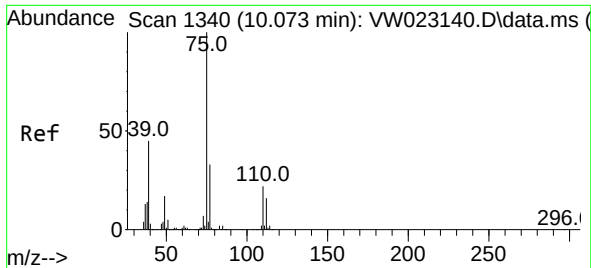

#39
 cis-1,3-Dichloropropene
 Concen: 0.571 ug/L
 RT: 10.043 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW023157.D
 Acq: 19 May 2022 02:29

Instrument :
 MSVOA_W
 ClientSampleId :

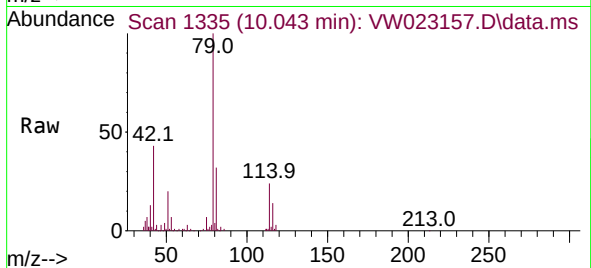

Tgt Ion: 75 Resp: 3697
 Ion Ratio Lower Upper
 75 100
 77 31.4 22.1 41.1

