




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023125.D
 Acq On : 18 May 2022 12:33
 Operator : SY/VA
 Sample : N2883-03RE
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4K5RE

Manual IntegrationsAPPROVED

Quant Time: May 19 01:23:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

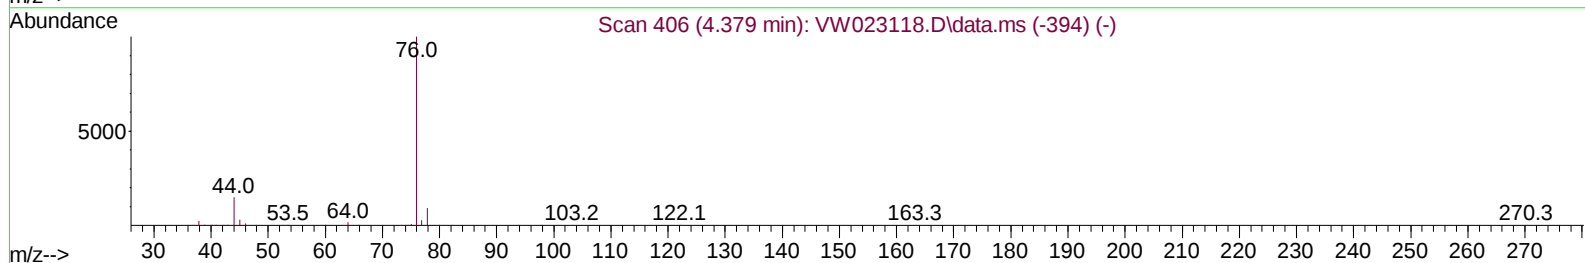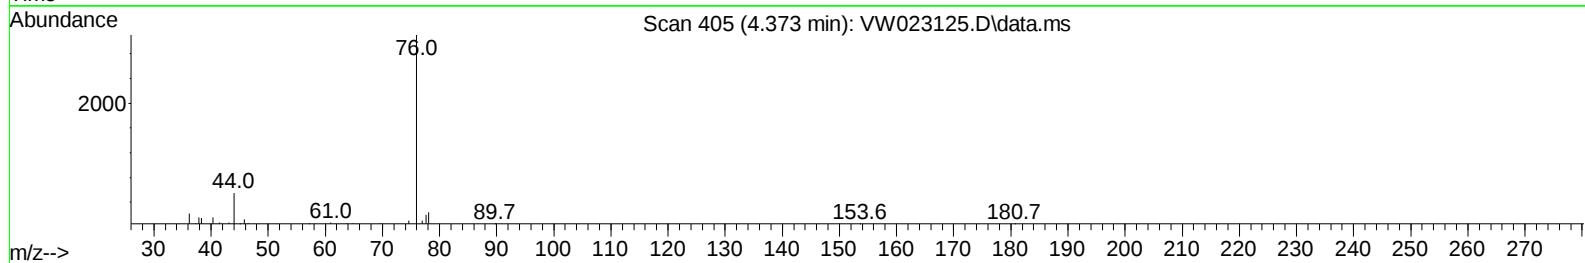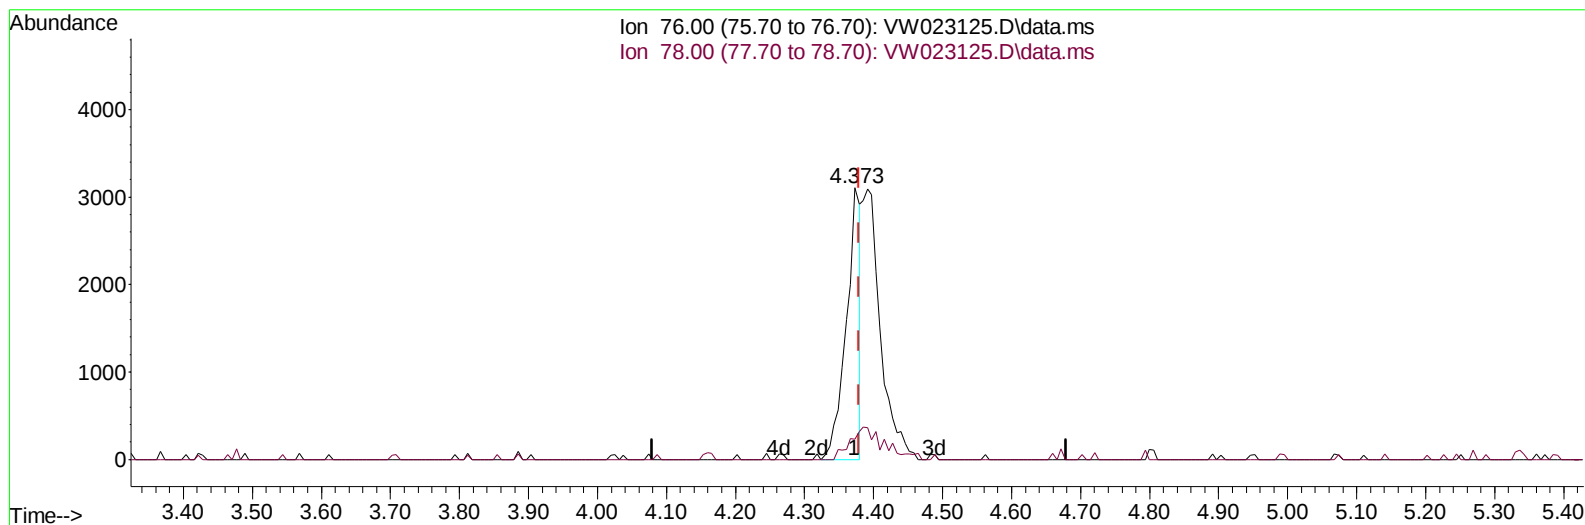

TIC: VW023125.D\data.ms

(14) Carbon disulfide (T)

4.373min (-0.006) 0.56 ug/L

response 4333

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.60	7.57#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023125.D
 Acq On : 18 May 2022 12:33
 Operator : SY/VA
 Sample : N2883-03RE
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4K5RE

Manual IntegrationsAPPROVED

Quant Time: May 19 01:23:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

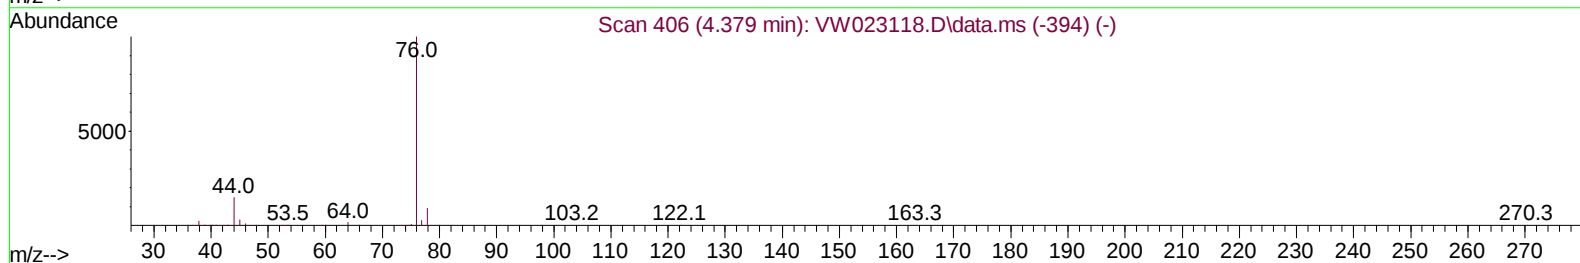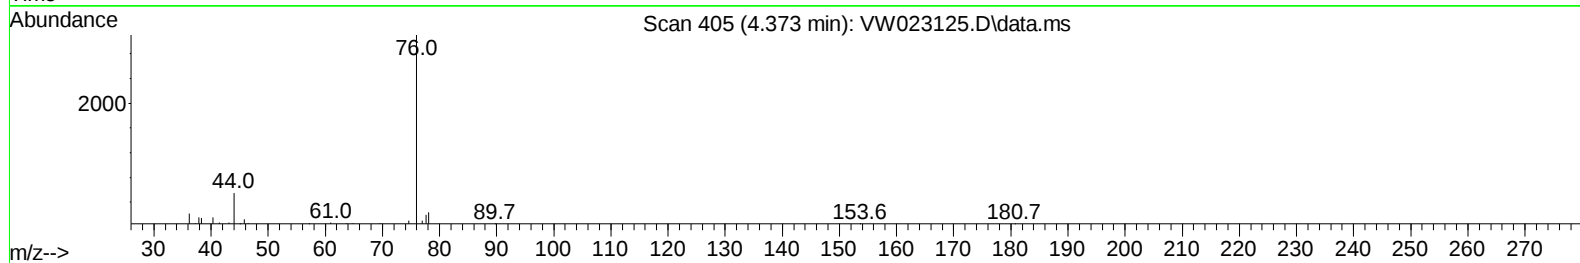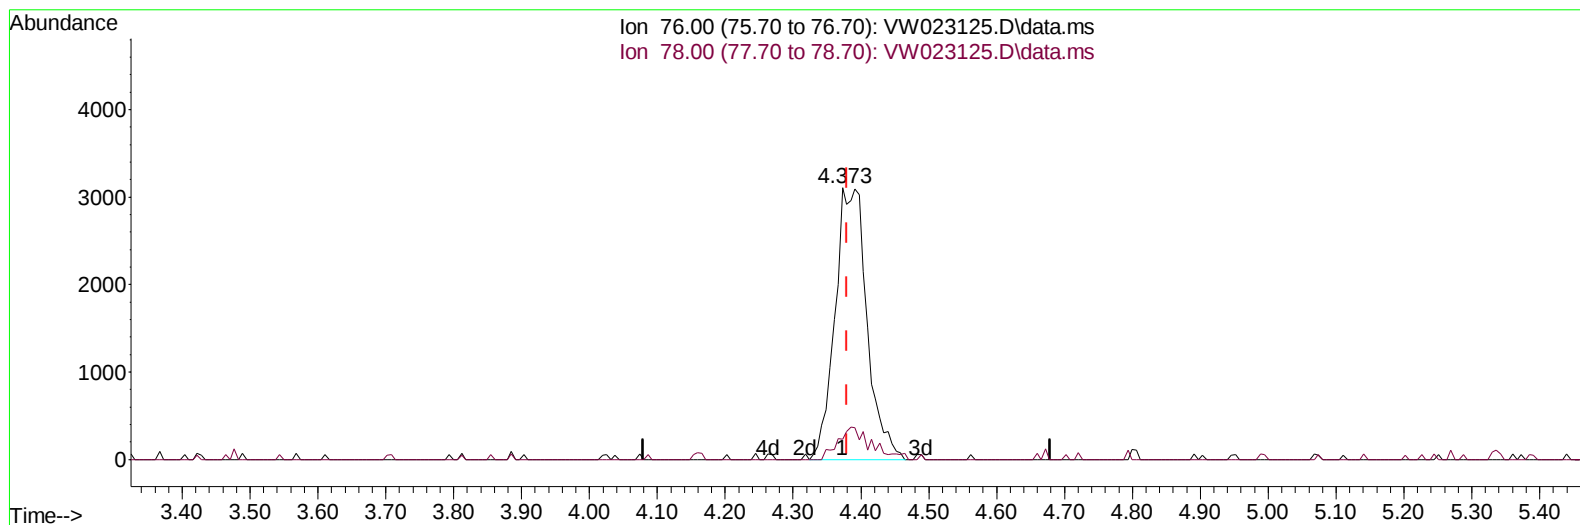

TIC: VW023125.D\data.ms

(14) Carbon disulfide (T)

4.373min (-0.006) 1.31 ug/L m

response 10091

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.60	7.57#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023125.D
 Acq On : 18 May 2022 12:33
 Operator : SY/VA
 Sample : N2883-03RE
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4K5RE

Manual IntegrationsAPPROVED

Quant Time: May 19 01:23:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

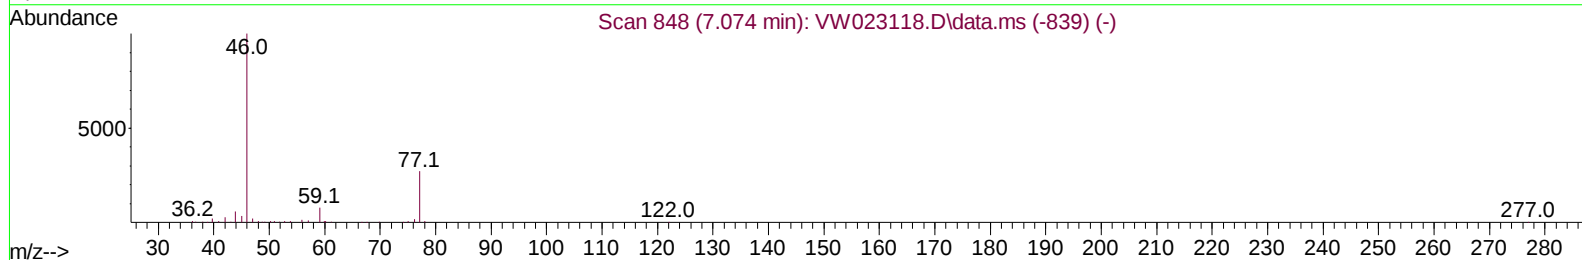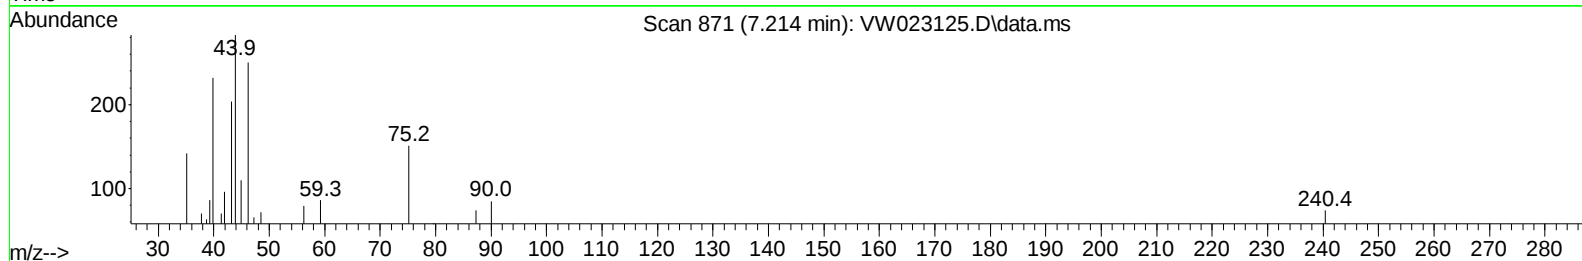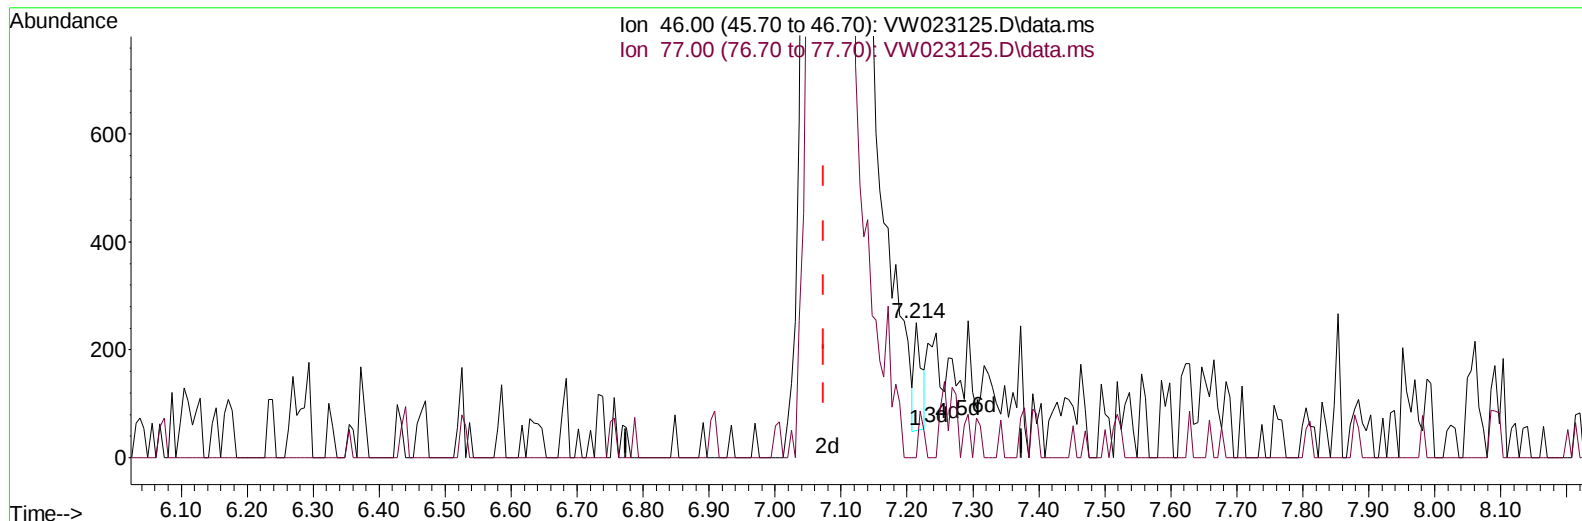

TIC: VW023125.D\data.ms

(21) 2-Butanone-d5 (S)

7.214min (+ 0.140) 0.18 ug/L

response 156

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	32.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023125.D
 Acq On : 18 May 2022 12:33
 Operator : SY/VA
 Sample : N2883-03RE
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4K5RE

Manual IntegrationsAPPROVED

Quant Time: May 19 01:23:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

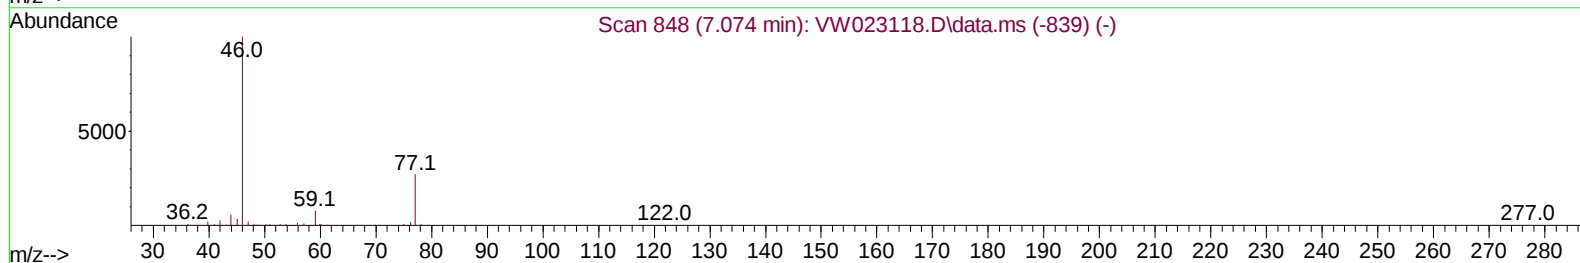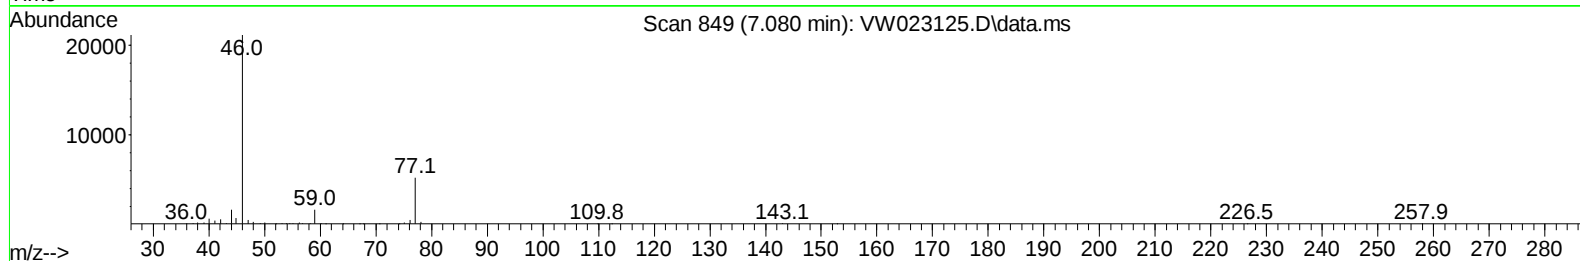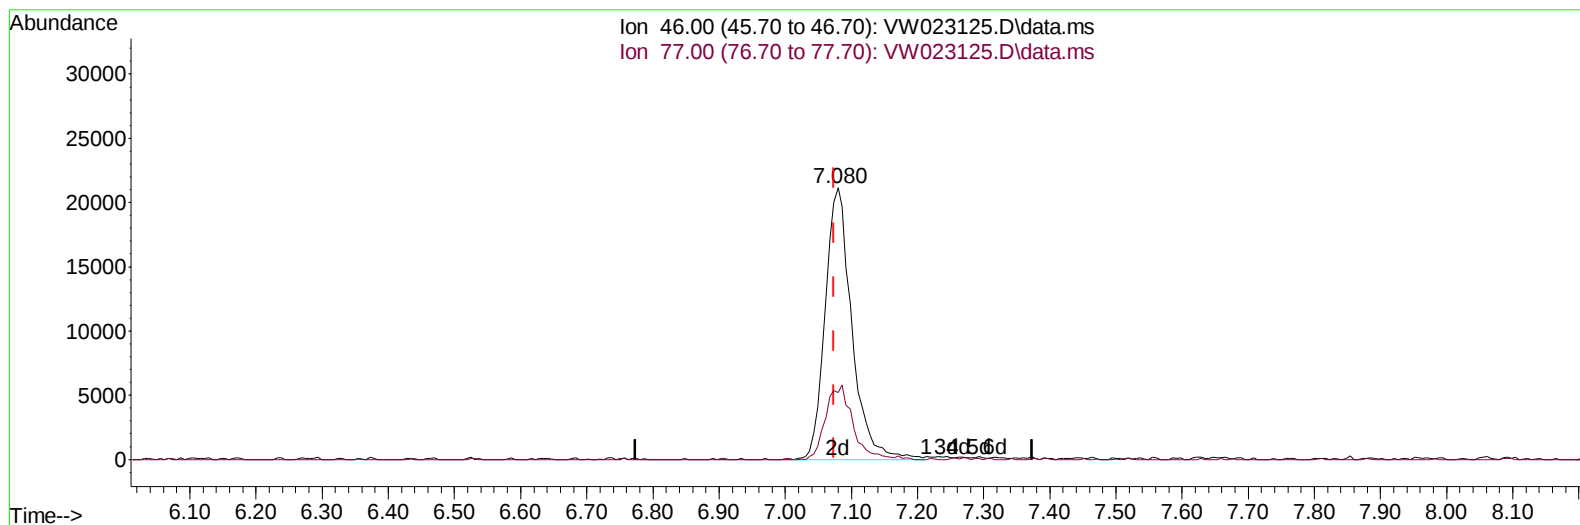

TIC: VW023125.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 68.90 ug/L m

response 59005

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023125.D
 Acq On : 18 May 2022 12:33
 Operator : SY/VA
 Sample : N2883-03RE
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4K5RE

Manual IntegrationsAPPROVED

Quant Time: May 19 01:23:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	219524	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	125304	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	23935	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	77313	17.166	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	68.680%	
7) Chloroethane-d5	2.885	69	63682	21.734	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	86.920%	
11) 1,1-Dichloroethene-d2	4.013	63	72968	12.539	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	50.160%	
21) 2-Butanone-d5	7.080	46	59005m	68.905	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	137.800%#	
24) Chloroform-d	7.653	84	156675	24.360	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	97.440%	
26) 1,2-Dichloroethane-d4	8.305	65	90994	25.796	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.200%	
32) Benzene-d6	8.275	84	263975	36.549	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	146.200%#	
36) 1,2-Dichloropropane-d6	9.274	67	88016	43.383	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	173.520%#	
41) Toluene-d8	10.323	98	175806	25.198	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	100.800%	
43) trans-1,3-Dichloroprop...	10.579	79	22688	24.288	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	97.160%	
47) 2-Hexanone-d5	10.927	63	39750	102.635	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	205.260%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	79342	41.958	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	167.840%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	24653	29.465	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	117.880%	
Target Compounds						
13) Acetone	4.129	43	7742	12.076	ug/L	85
14) Carbon disulfide	4.373	76	10091m	1.309	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023125.D
Acq On : 18 May 2022 12:33
Operator : SY/VA
Sample : N2883-03RE
Misc : 6.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4K5RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
Supervised By :Mahesh Dadoda 05/27/2022

Quant Time: May 19 01:23:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

