




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023136.D
Acq On : 18 May 2022 16:59
Operator : SY/VA
Sample : N2926-01
Misc : 4.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY11

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
Supervised By :Mahesh Dadoda 05/27/2022

Quant Time: May 19 01:25:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

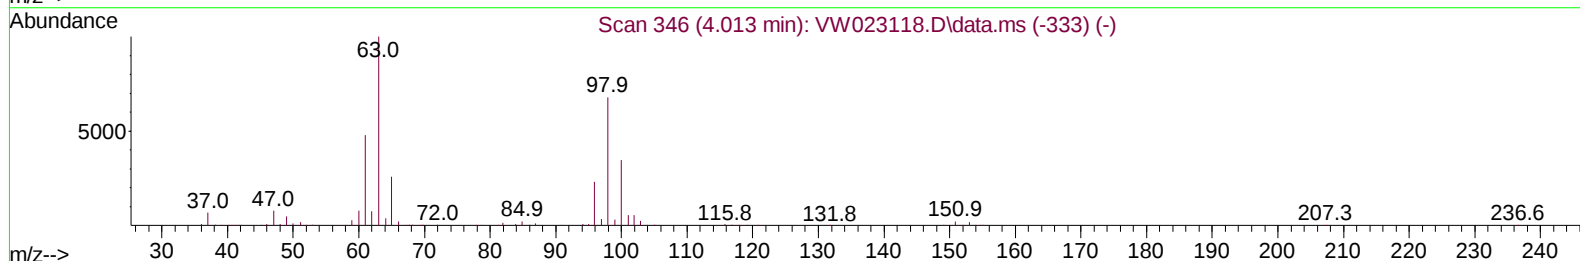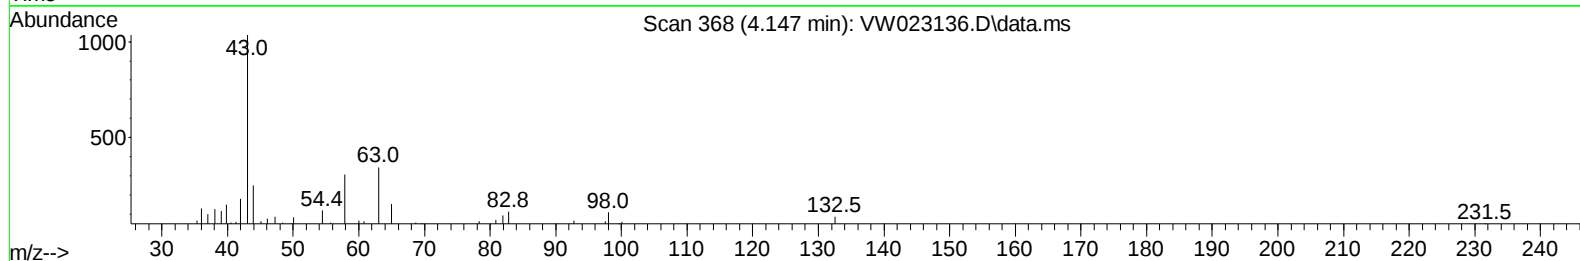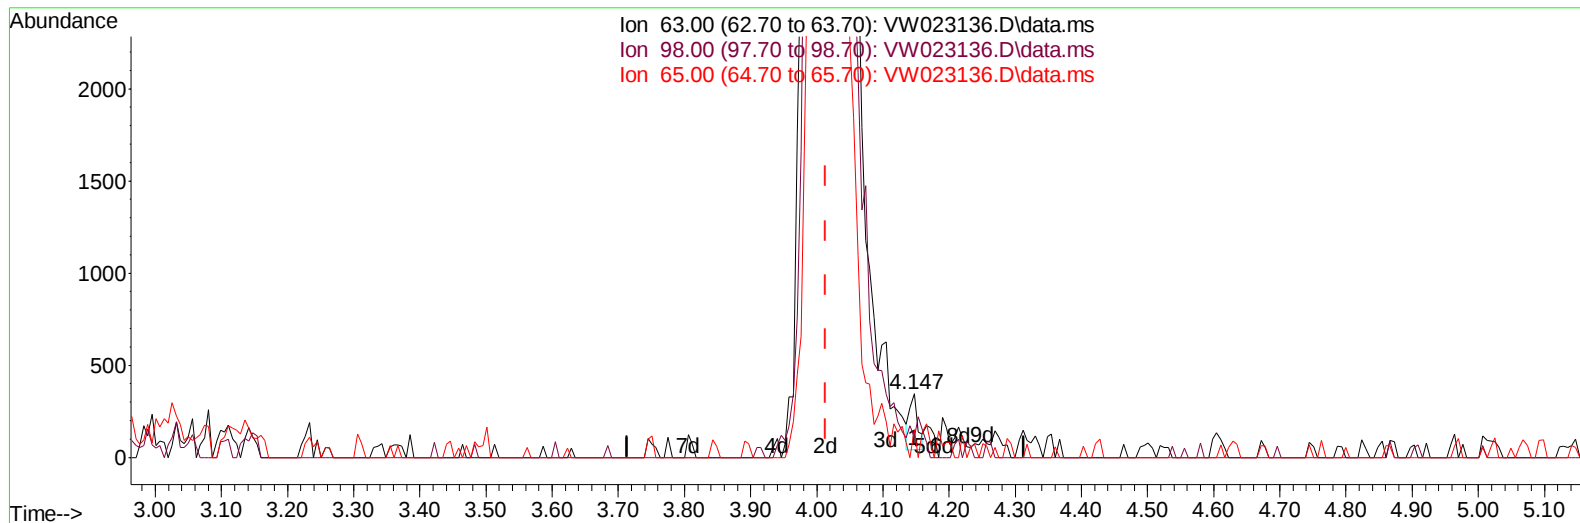

TIC: VW023136.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.147min (+ 0.134) 0.03 ug/L

response 262

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	64.12
65.00	23.30	21.37
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023136.D
 Acq On : 18 May 2022 16:59
 Operator : SY/VA
 Sample : N2926-01
 Misc : 4.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY11

Manual IntegrationsAPPROVED

Quant Time: May 19 01:25:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

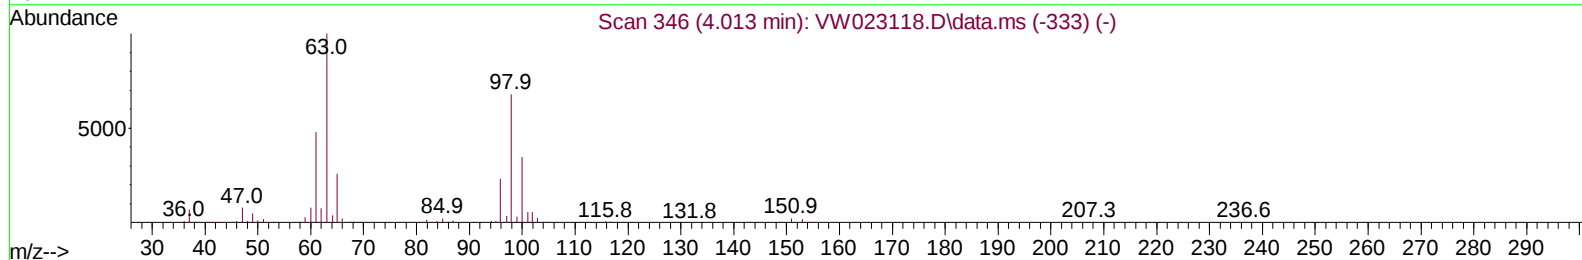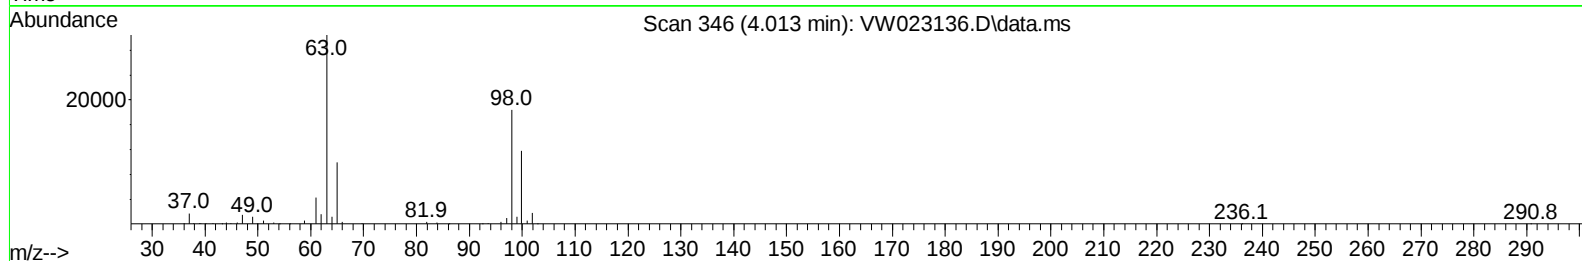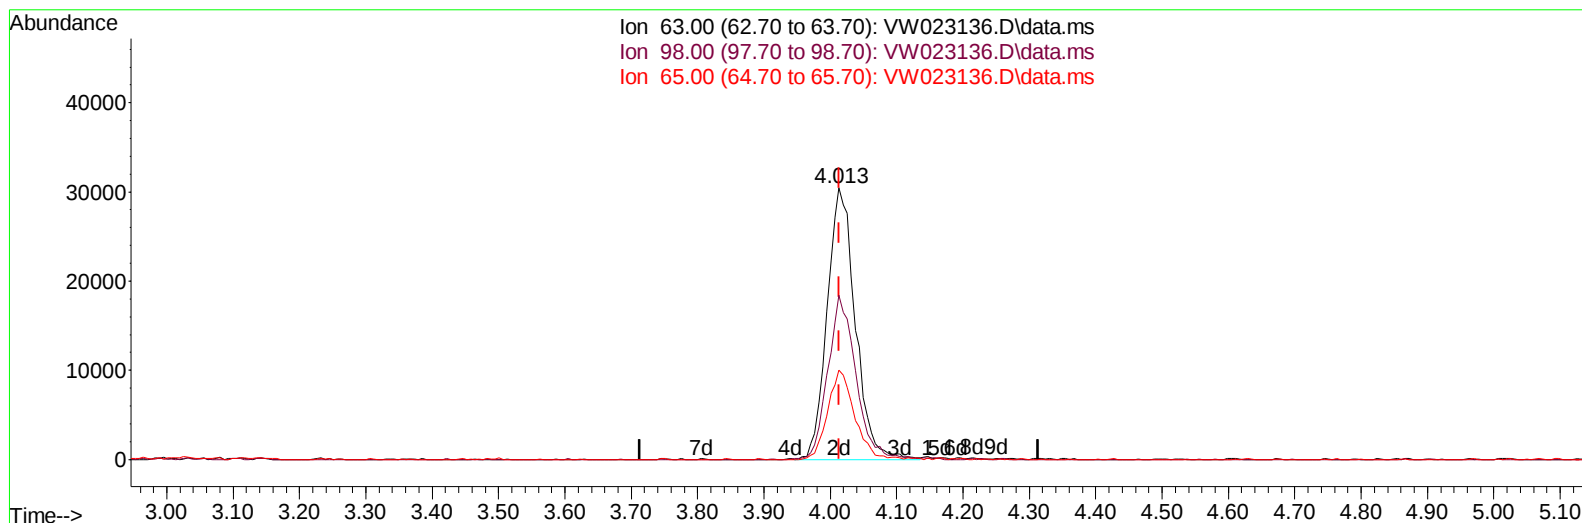

TIC: VW023136.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.000) 10.55 ug/L m

response 89536

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.19#
65.00	23.30	0.06#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023136.D
 Acq On : 18 May 2022 16:59
 Operator : SY/VA
 Sample : N2926-01
 Misc : 4.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY11

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

Quant Time: May 19 01:25:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

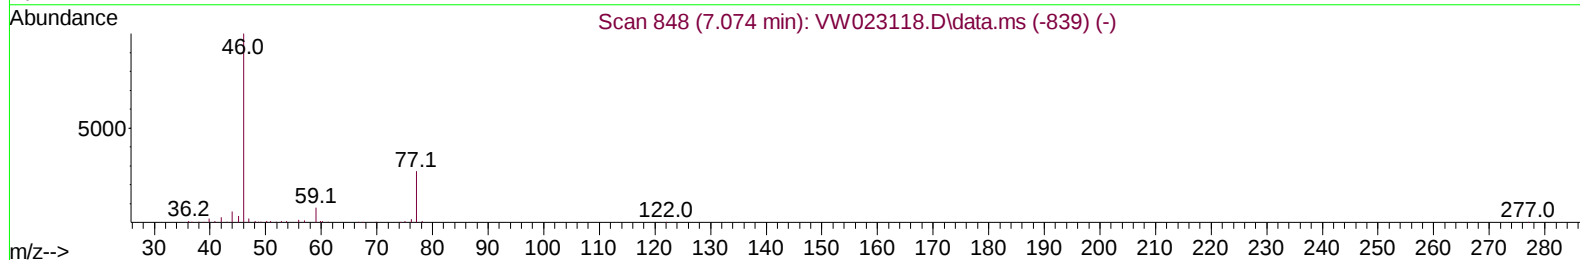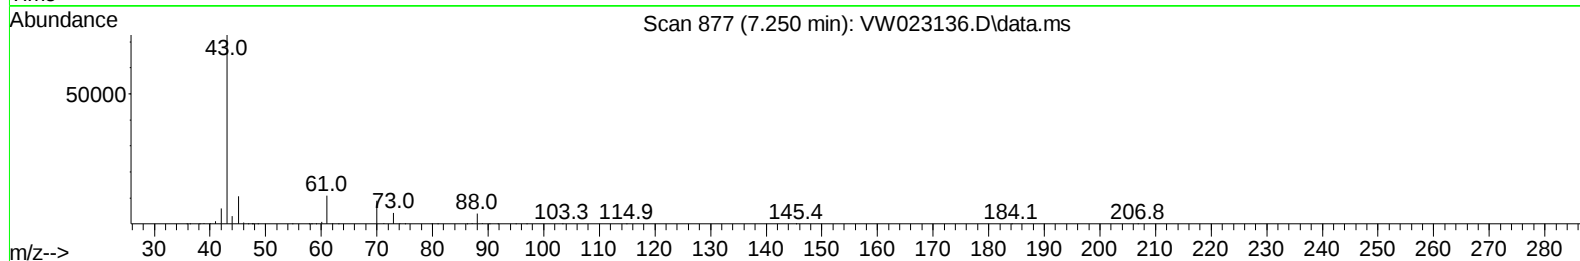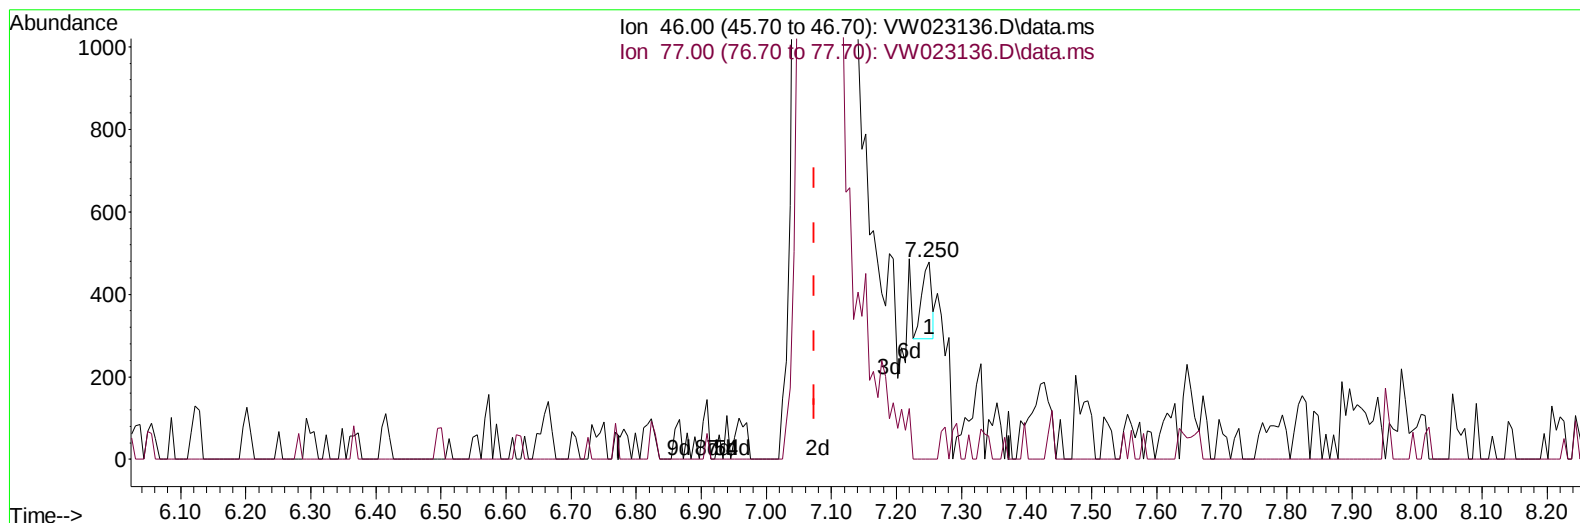

TIC: VW023136.D\data.ms

(21) 2-Butanone-d5 (S)

7.250min (+ 0.177) 0.16 ug/L

response 200

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	26.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023136.D
 Acq On : 18 May 2022 16:59
 Operator : SY/VA
 Sample : N2926-01
 Misc : 4.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY11

Manual IntegrationsAPPROVED

Quant Time: May 19 01:25:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

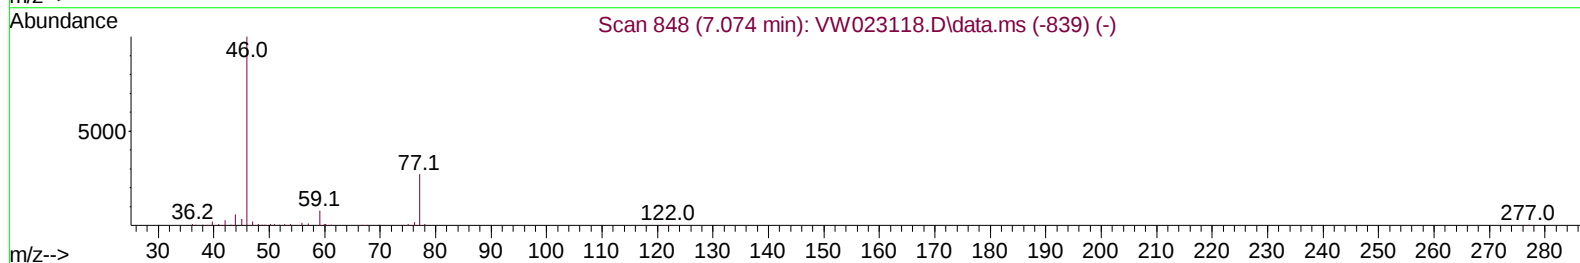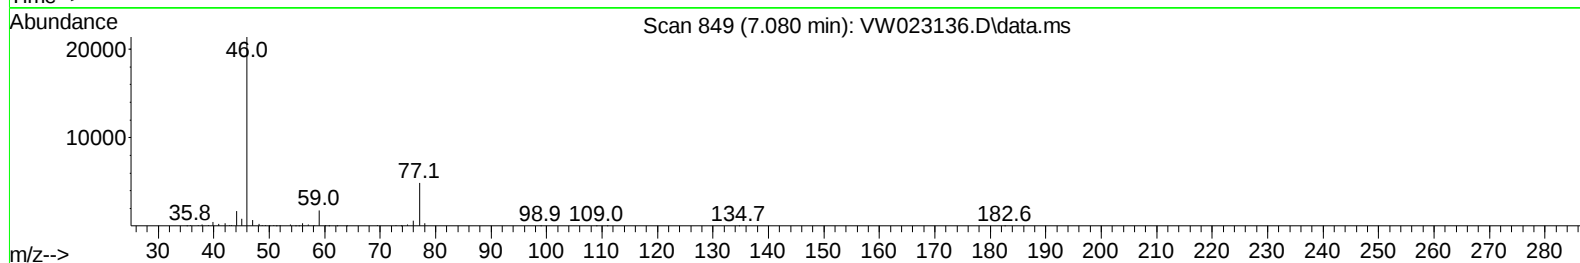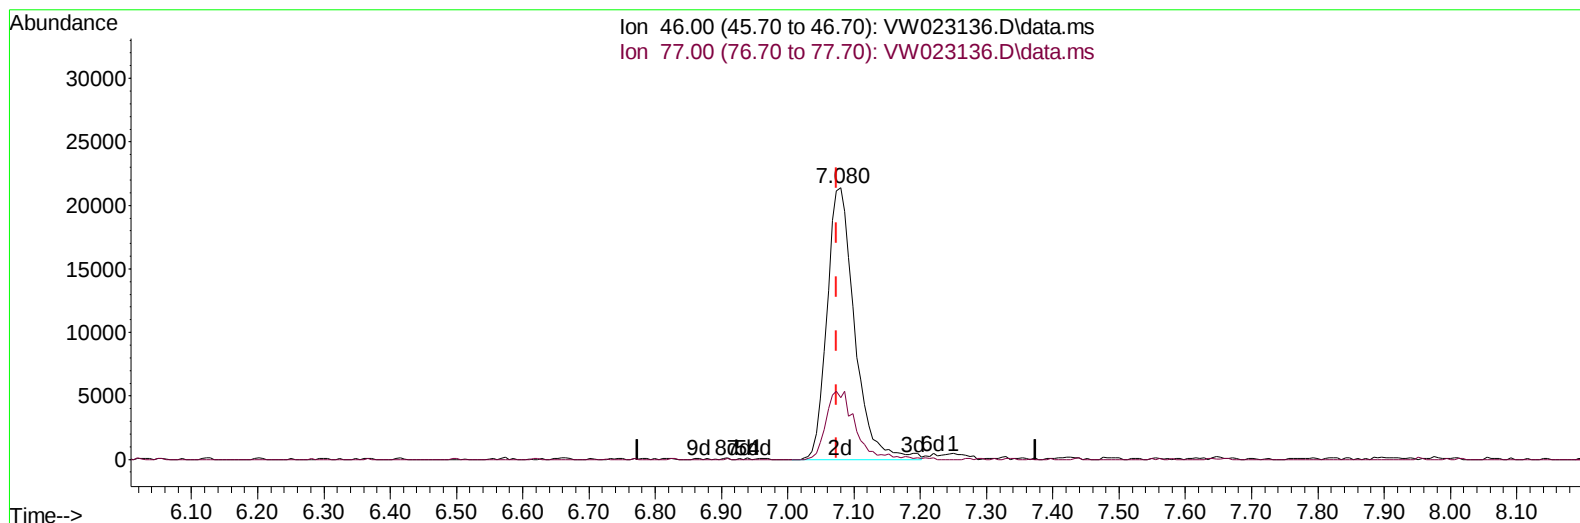

TIC: VW023136.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 49.45 ug/L m

response 61768

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.09#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023136.D
 Acq On : 18 May 2022 16:59
 Operator : SY/VA
 Sample : N2926-01
 Misc : 4.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY11

Manual IntegrationsAPPROVED

Quant Time: May 19 01:25:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		320215	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		296817	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		135389	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		86186	13.119	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.480%	
7) Chloroethane-d5	2.885	69		71845	16.809	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.240%	
11) 1,1-Dichloroethene-d2	4.013	63		89536m	10.548	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	42.200%#	
21) 2-Butanone-d5	7.080	46		61768m	49.450	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.900%	
24) Chloroform-d	7.653	84		191195	20.380	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.520%	
26) 1,2-Dichloroethane-d4	8.305	65		105059	20.418	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.680%	
32) Benzene-d6	8.275	84		338092	19.762	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.040%	
36) 1,2-Dichloropropane-d6	9.274	67		106854	22.234	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.920%	
41) Toluene-d8	10.323	98		304067	18.398	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.600%	
43) trans-1,3-Dichloroprop...	10.579	79		38420	17.363	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.440%	
47) 2-Hexanone-d5	10.920	63		48540	52.910	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.820%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		104842	23.406	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152		105939	22.384	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.520%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023136.D
Acq On : 18 May 2022 16:59
Operator : SY/VA
Sample : N2926-01
Misc : 4.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY11

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
Supervised By :Mahesh Dadoda 05/27/2022

Quant Time: May 19 01:25:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

