

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023137.D
Acq On : 18 May 2022 17:23
Operator : SY/VA
Sample : N2848-01
Misc : 5.39g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
EXXW3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:25:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

05/20/2022
Supervised By :Mahesh
Dadoda
05/27/2022

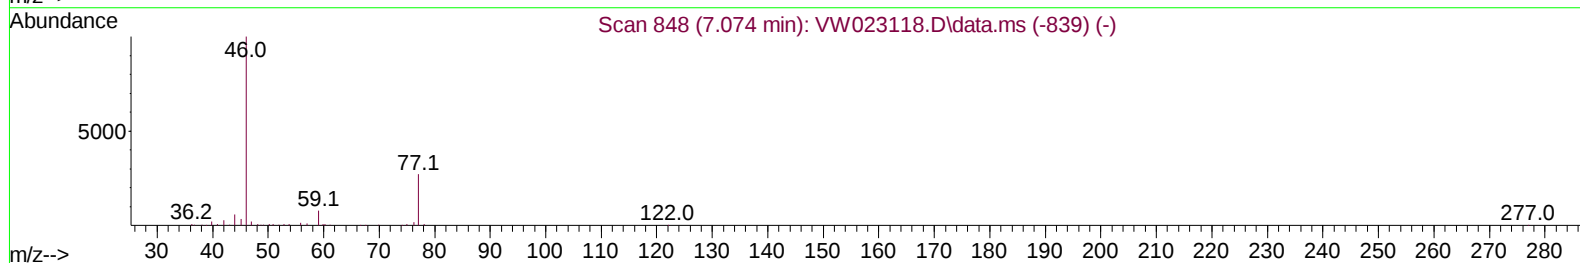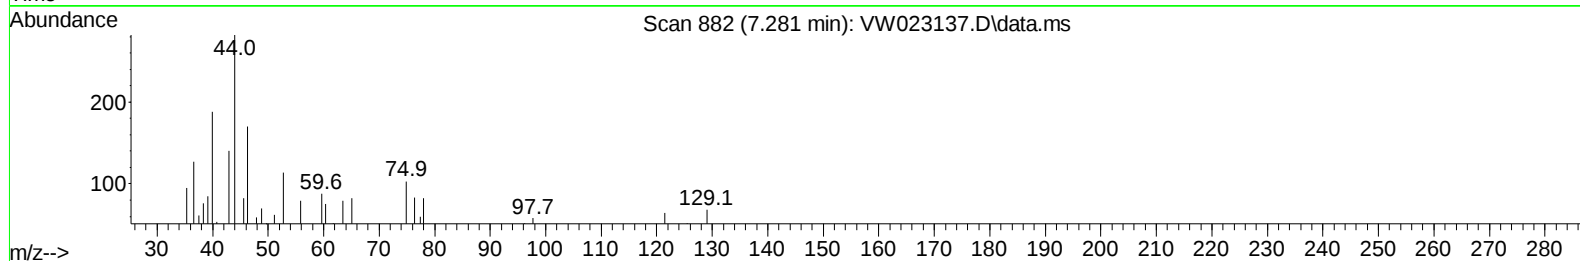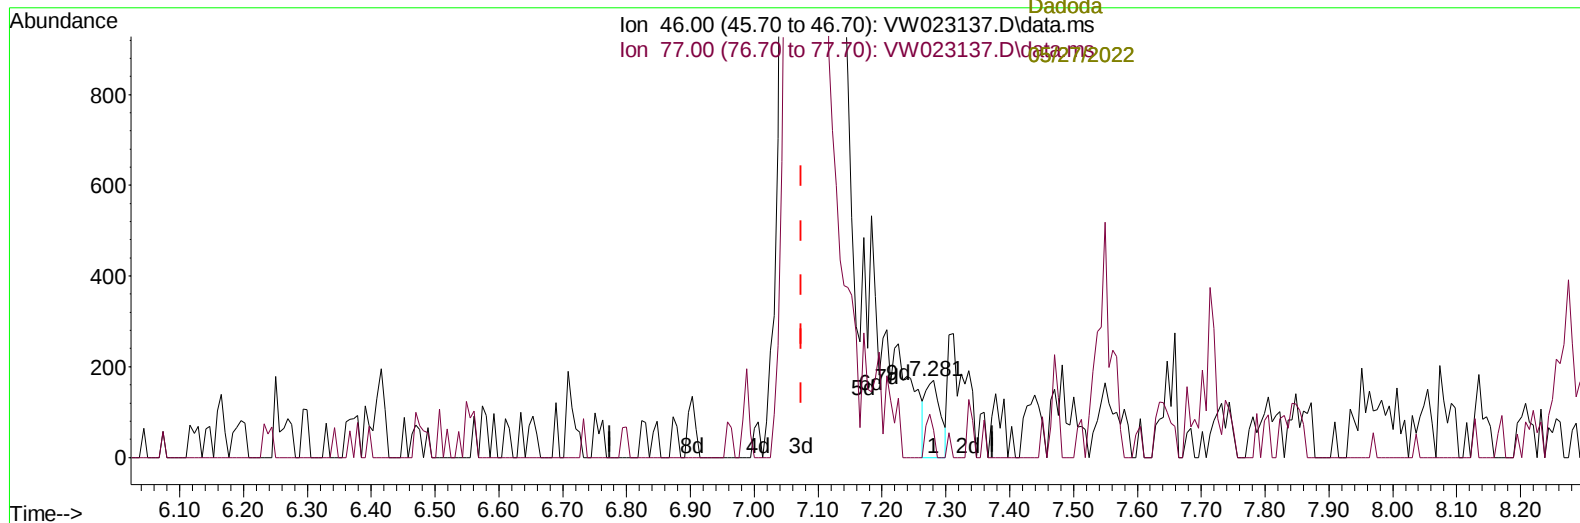

TIC: VW023137.D\data.ms

(21) 2-Butanone-d5 (S)

7.281min (+ 0.207) 0.22 ug/L

response 278

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	29.50
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023137.D
 Acq On : 18 May 2022 17:23
 Operator : SY/VA
 Sample : N2848-01
 Misc : 5.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXW3




Manual IntegrationsAPPROVED

Quant Time: May 19 01:25:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

05/20/2022
 Supervised By :Mahesh

Dadoda
 05/27/2022

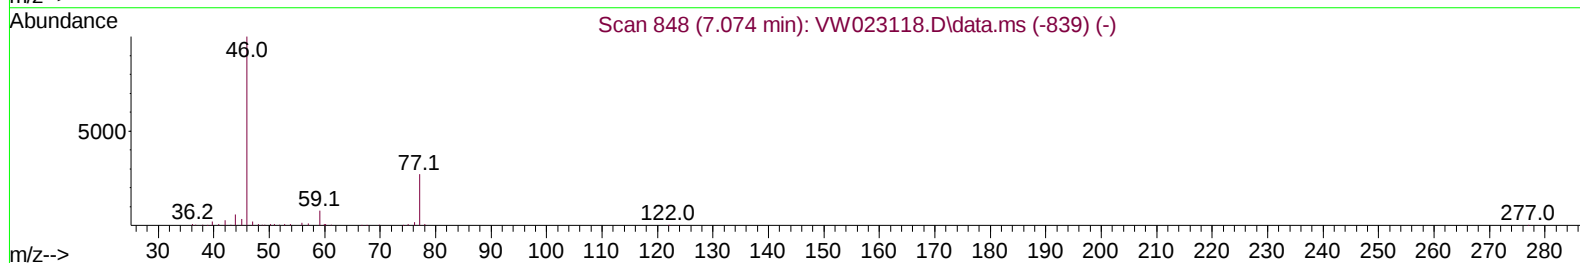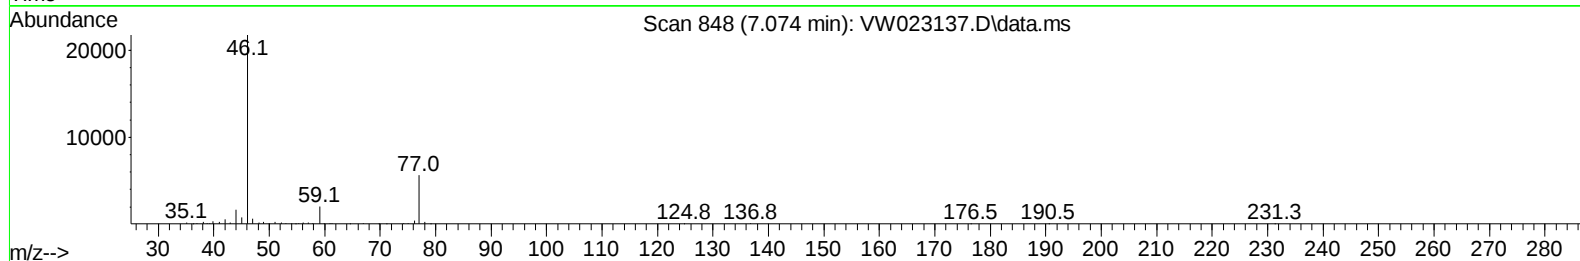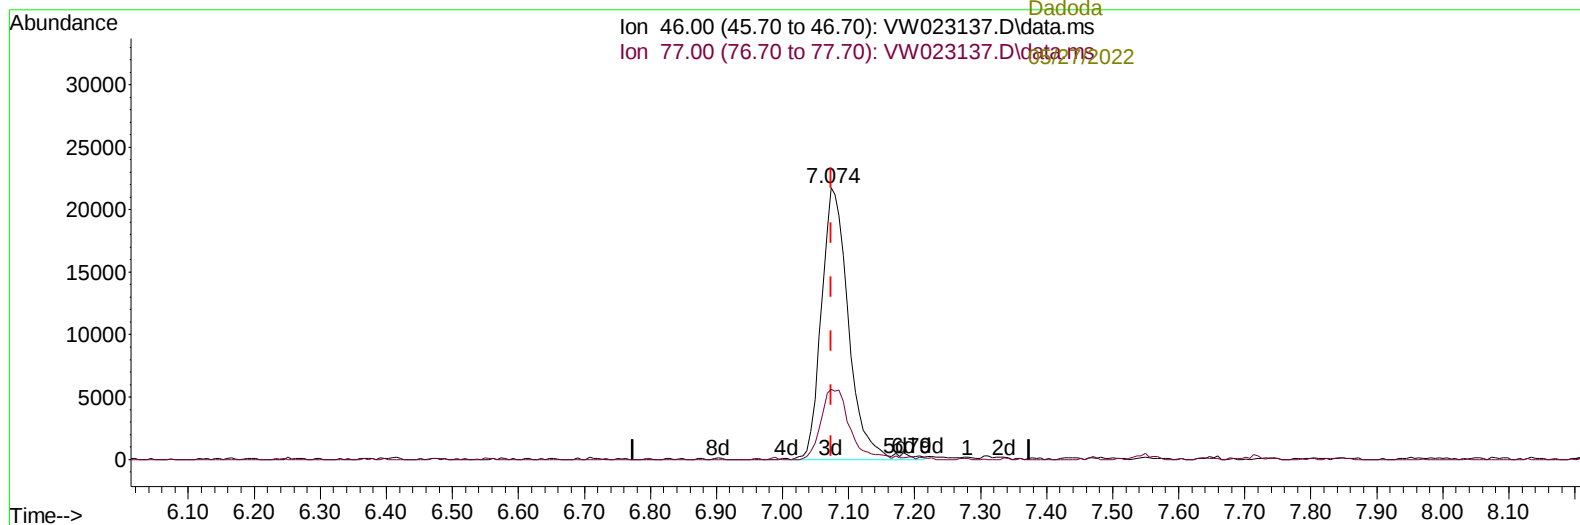

TIC: VW023137.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (-0.000) 49.78 ug/L m

response 62161

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.13#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023137.D
 Acq On : 18 May 2022 17:23
 Operator : SY/VA
 Sample : N2848-01
 Misc : 5.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXW3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:25:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 01:20:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

05/20/2022
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----05/27/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	320117	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	307862	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	155552	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	86322	13.143	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	52.560%	
7) Chloroethane-d5	2.879	69	71847	16.815	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.240%	
11) 1,1-Dichloroethene-d2	4.013	63	89052	10.494	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	41.960%#	
21) 2-Butanone-d5	7.074	46	62161m	49.780	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	99.560%	
24) Chloroform-d	7.647	84	184943	19.720	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	78.880%	
26) 1,2-Dichloroethane-d4	8.305	65	106021	20.611	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	82.440%	
32) Benzene-d6	8.275	84	336029	18.937	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	75.760%	
36) 1,2-Dichloropropane-d6	9.274	67	104813	21.027	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	84.120%	
41) Toluene-d8	10.323	98	306856	17.901	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	71.600%	
43) trans-1,3-Dichloroprop...	10.579	79	41274	17.983	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.920%	
47) 2-Hexanone-d5	10.921	63	47606	50.030	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.060%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	108770	23.412	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	93.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152	112362	20.664	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	82.640%	
Target Compounds						
13) Acetone	4.129	43	5538	5.924	ug/L	Qvalue 66

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023137.D
Acq On : 18 May 2022 17:23
Operator : SY/VA
Sample : N2848-01
Misc : 5.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXXW3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

05/20/2022
Supervised By :Mahesh
Dadoda

05/27/2022

Quant Time: May 19 01:25:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 01:20:33 2022
Response via : Initial Calibration

