




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023151.D
 Acq On : 19 May 2022 00:05
 Operator : SY/VA
 Sample : N2848-10
 Misc : 4.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXY1

Manual IntegrationsAPPROVED

Quant Time: May 19 04:55:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 04:23:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

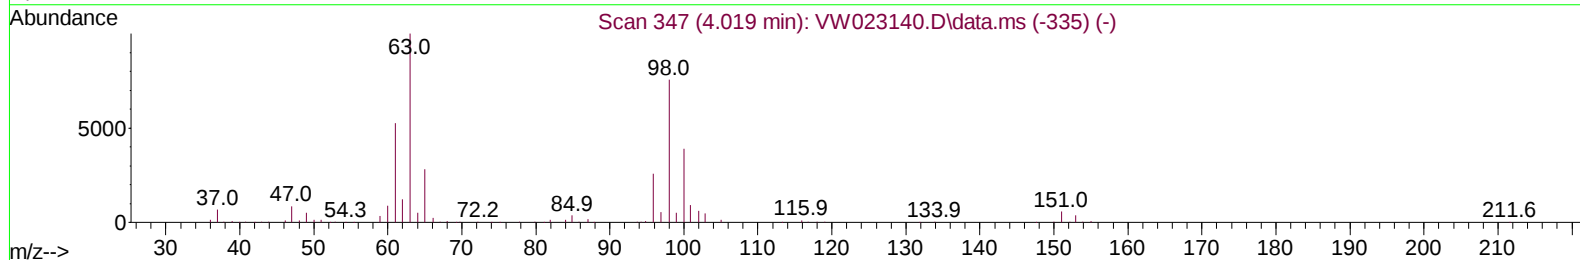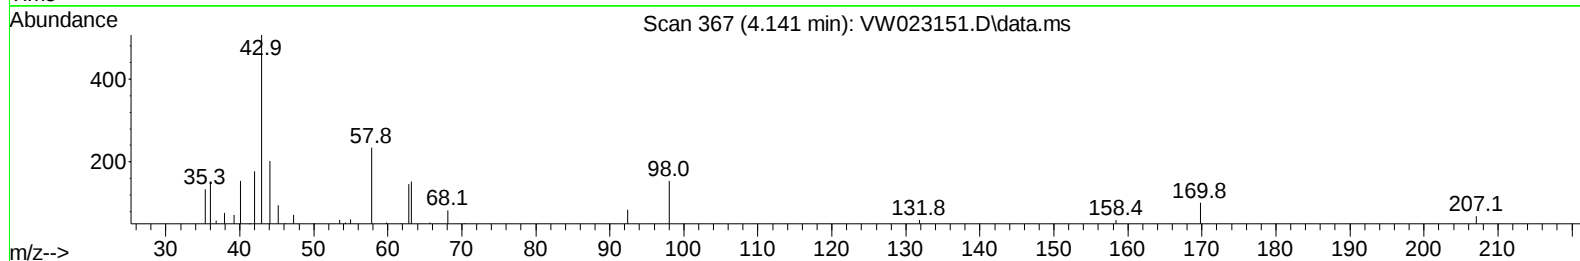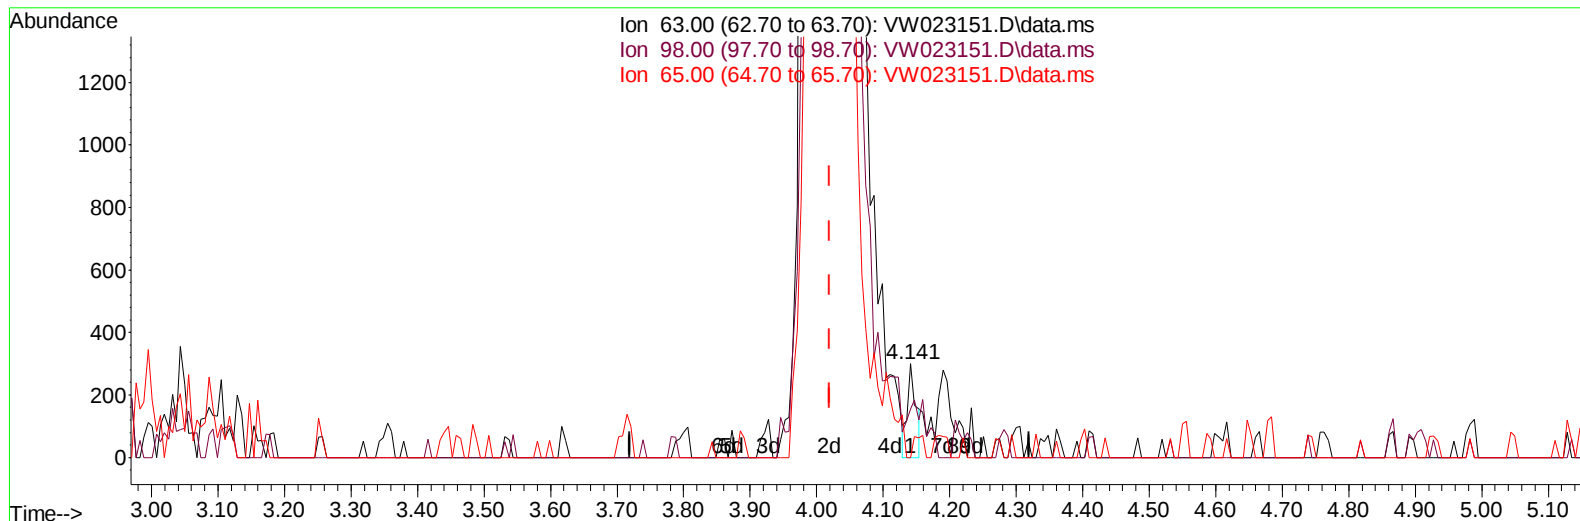

TIC: VW023151.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.141min (+ 0.122) 0.03 ug/L

response 271

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	77.49
65.00	23.30	26.94
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023151.D
 Acq On : 19 May 2022 00:05
 Operator : SY/VA
 Sample : N2848-10
 Misc : 4.38g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXY1

Manual IntegrationsAPPROVED

Quant Time: May 19 04:55:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 04:23:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

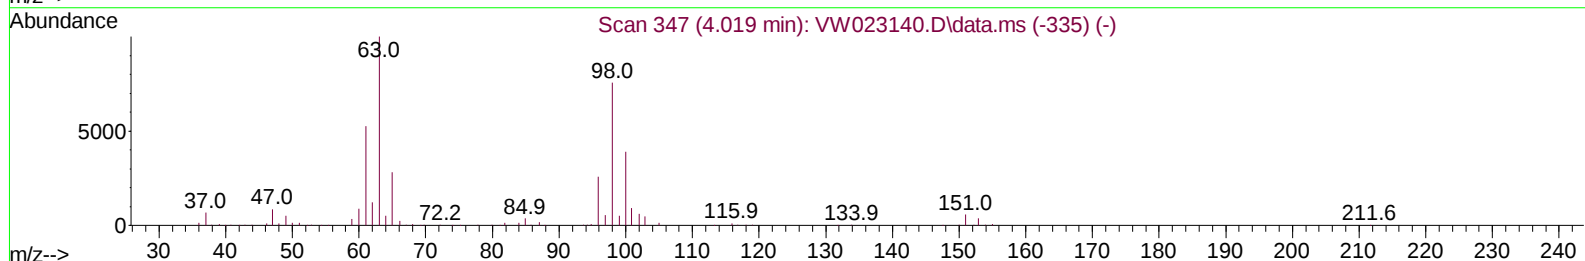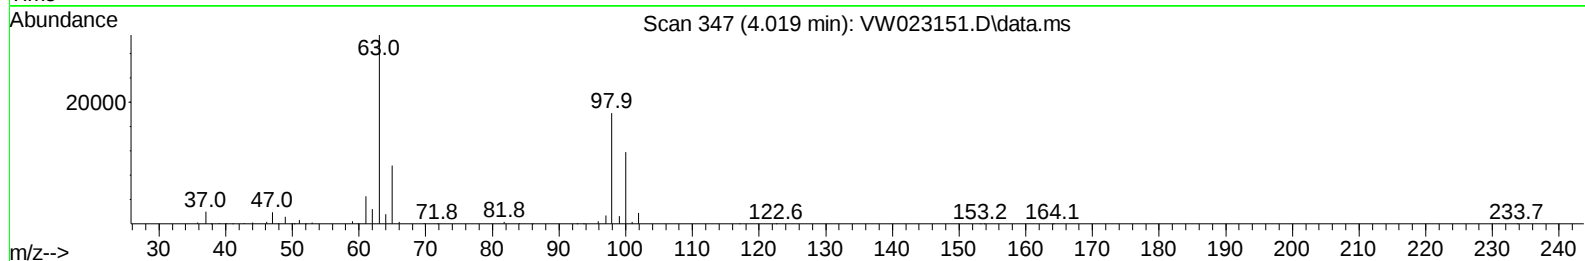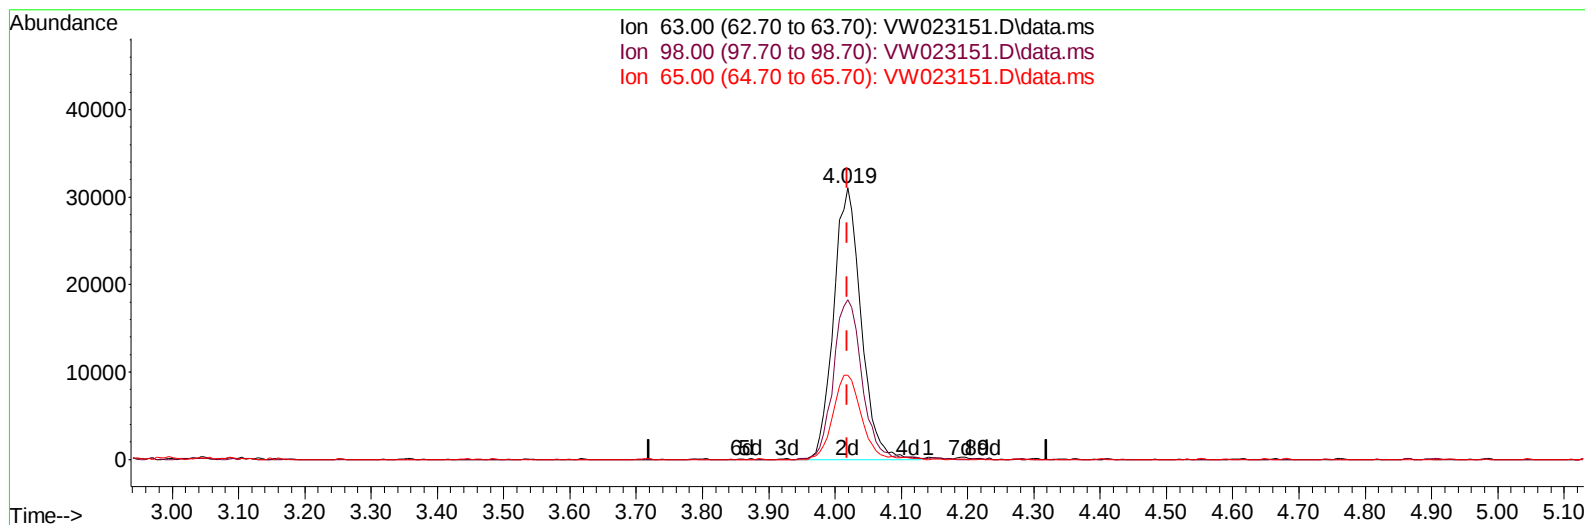

TIC: VW023151.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (+ 0.000) 11.28 ug/L m

response 89227

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.24#
65.00	23.30	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023151.D
 Acq On : 19 May 2022 00:05
 Operator : SY/VA
 Sample : N2848-10
 Misc : 4.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXY1

Manual IntegrationsAPPROVED

Quant Time: May 19 04:55:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 04:23:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	298314	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	280110	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	115026	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	85132	13.910	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	55.640%	
7) Chloroethane-d5	2.885	69	67366	16.919	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.680%	
11) 1,1-Dichloroethene-d2	4.019	63	89227m	11.283	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	45.120%	
21) 2-Butanone-d5	7.080	46	53817	46.248	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	92.500%	
24) Chloroform-d	7.653	84	197019	22.542	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	90.160%	
26) 1,2-Dichloroethane-d4	8.305	65	108679	22.672	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.680%	
32) Benzene-d6	8.275	84	352120	21.809	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	87.240%	
36) 1,2-Dichloropropane-d6	9.274	67	109184	24.074	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	96.280%	
41) Toluene-d8	10.323	98	312781	20.055	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	80.200%	
43) trans-1,3-Dichloroprop...	10.579	79	36837	17.640	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	70.560%	
47) 2-Hexanone-d5	10.927	63	40204	46.437	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	92.880%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	101181	23.936	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	95.760%	
66) 1,2-Dichlorobenzene-d4	13.853	152	98302	24.448	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.800%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023151.D
Acq On : 19 May 2022 00:05
Operator : SY/VA
Sample : N2848-10
Misc : 4.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXXY1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
Supervised By :Mahesh Dadoda 05/27/2022

Quant Time: May 19 04:55:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 04:23:21 2022
Response via : Initial Calibration

