




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023152.D
Acq On : 19 May 2022 00:29
Operator : SY/VA
Sample : N2848-11
Misc : 4.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXXY2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
Supervised By :Mahesh Dadoda 05/27/2022

Quant Time: May 19 04:55:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 04:23:21 2022
Response via : Initial Calibration

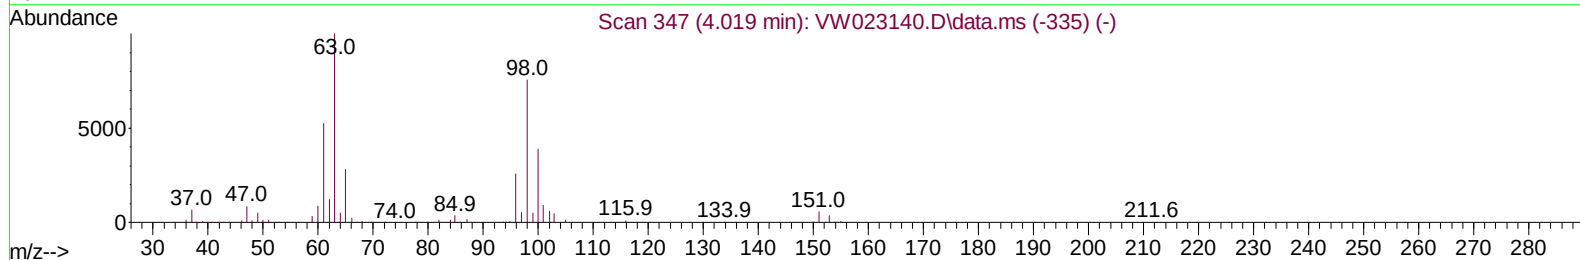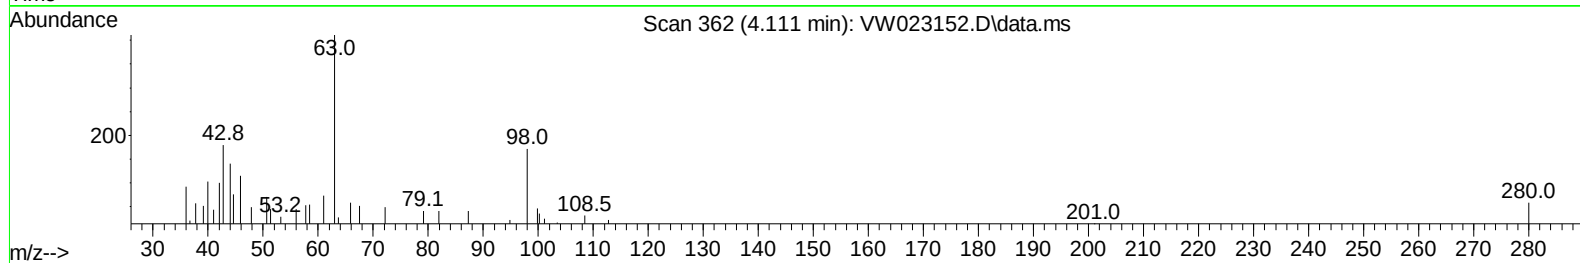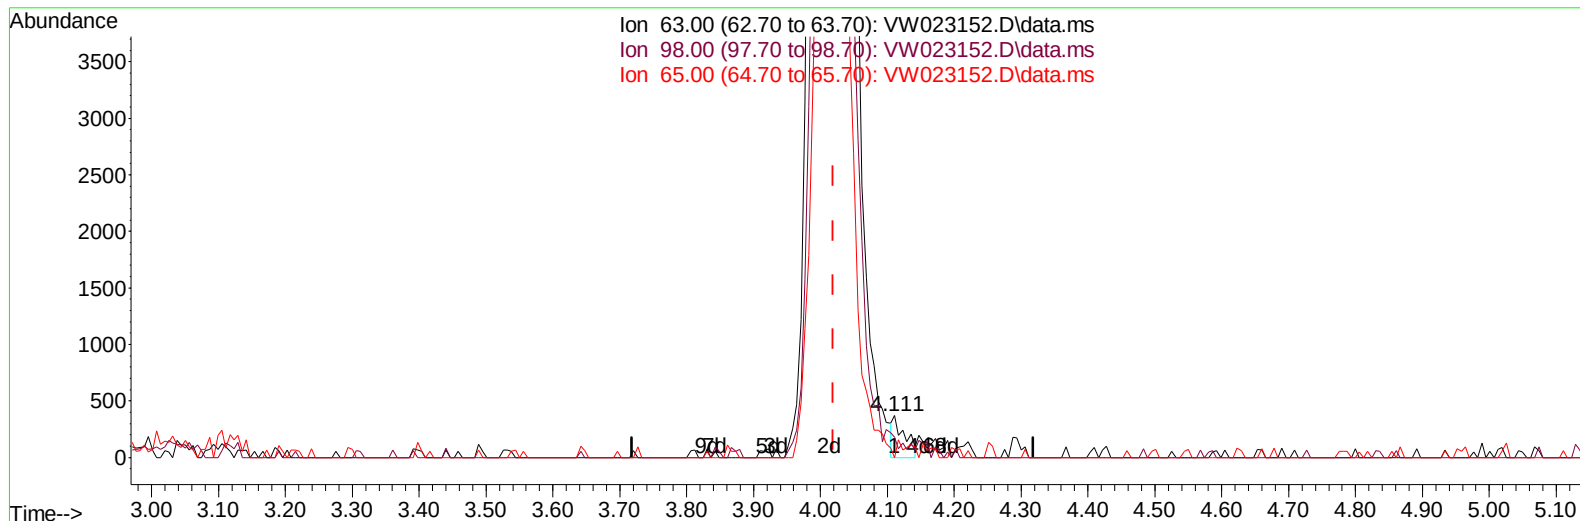

TIC: VW023152.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.111min (+ 0.092) 0.05 ug/L

response 456

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	57.46
65.00	23.30	17.98
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023152.D
Acq On : 19 May 2022 00:29
Operator : SY/VA
Sample : N2848-11
Misc : 4.70g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXXY2

Manual IntegrationsAPPROVED

Quant Time: May 19 04:55:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 04:23:21 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
Supervised By :Mahesh Dadoda 05/27/2022

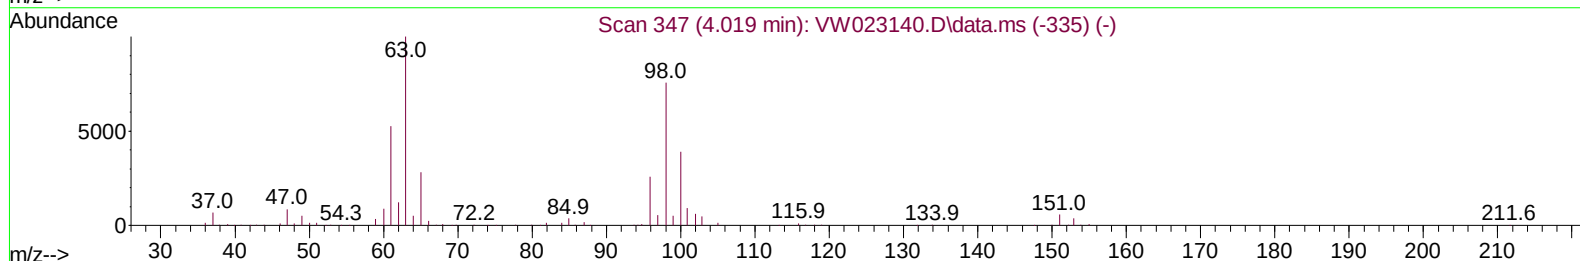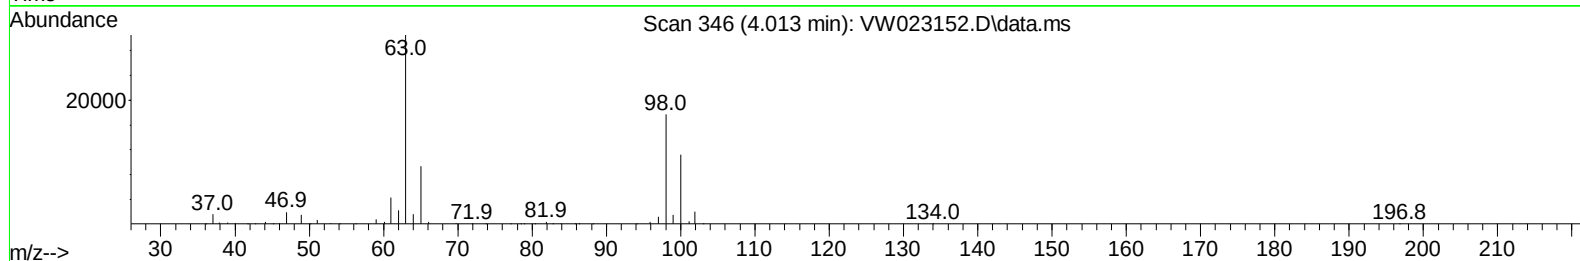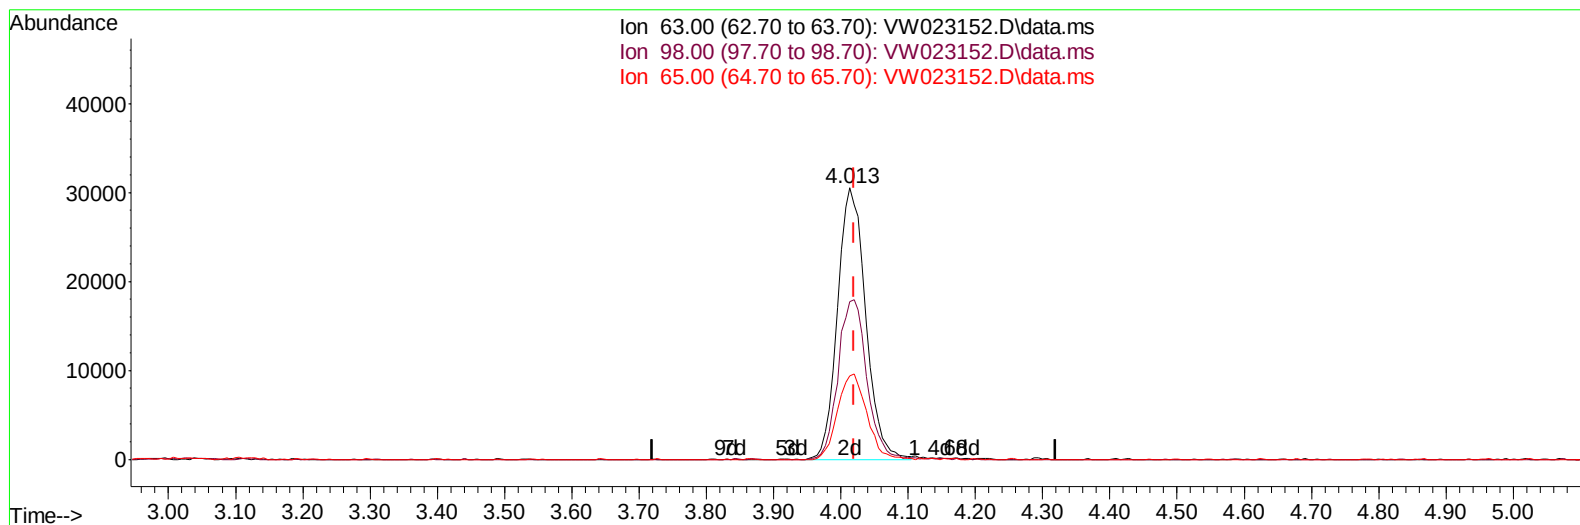

TIC: VW023152.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 10.42 ug/L m

response 88563

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.30#
65.00	23.30	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023152.D
 Acq On : 19 May 2022 00:29
 Operator : SY/VA
 Sample : N2848-11
 Misc : 4.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXY2

Manual IntegrationsAPPROVED

Quant Time: May 19 04:55:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 04:23:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	320766	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	299768	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	133735	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	87491	13.295	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	53.160%	
7) Chloroethane-d5	2.879	69	67326	15.725	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	62.920%	
11) 1,1-Dichloroethene-d2	4.013	63	88563m	10.415	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	41.680%#	
21) 2-Butanone-d5	7.080	46	65634	52.455	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	104.900%	
24) Chloroform-d	7.653	84	203121	21.614	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	86.440%	
26) 1,2-Dichloroethane-d4	8.305	65	118480	22.987	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	91.960%	
32) Benzene-d6	8.275	84	363514	21.039	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	84.160%	
36) 1,2-Dichloropropane-d6	9.275	67	117433	24.195	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	96.800%	
41) Toluene-d8	10.323	98	313261	18.768	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.080%	
43) trans-1,3-Dichloroprop...	10.579	79	39125	17.507	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	70.040%	
47) 2-Hexanone-d5	10.927	63	51164	55.221	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	110.440%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	132113	29.204	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	116.800%	
66) 1,2-Dichlorobenzene-d4	13.847	152	115221	24.647	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	98.600%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023152.D
Acq On : 19 May 2022 00:29
Operator : SY/VA
Sample : N2848-11
Misc : 4.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXXY2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
Supervised By :Mahesh Dadoda 05/27/2022

Quant Time: May 19 04:55:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 04:23:21 2022
Response via : Initial Calibration

