

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
 Data File : VW023147.D
 Acq On : 18 May 2022 22:28
 Operator : SY/VA
 Sample : N2926-03
 Misc : 4.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY11MSD

Quant Time: May 19 04:55:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 19 04:23:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	303938	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	272057	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	106891	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	83756	13.432	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.720%
7) Chloroethane-d5	2.885	69	65913	16.247	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.000%
11) 1,1-Dichloroethene-d2	4.019	63	86340	10.716	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	42.880%#
21) 2-Butanone-d5	7.080	46	56130	47.343	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.680%
24) Chloroform-d	7.647	84	190785	21.425	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.720%
26) 1,2-Dichloroethane-d4	8.311	65	108486	22.213	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.840%
32) Benzene-d6	8.274	84	326546	20.824	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.280%
36) 1,2-Dichloropropane-d6	9.274	67	108339	24.595	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.400%
41) Toluene-d8	10.323	98	293958	19.406	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.640%
43) trans-1,3-Dichloroprop...	10.579	79	35642	17.573	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.280%
47) 2-Hexanone-d5	10.926	63	44441	52.850	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.700%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103541	25.219	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	87343	23.375	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.520%
Target Compounds						
13) Acetone	4.141	43	2846	3.206	ug/L	Qvalue 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051822\
Data File : VW023147.D
Acq On : 18 May 2022 22:28
Operator : SY/VA
Sample : N2926-03
Misc : 4.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY11MSD

Quant Time: May 19 04:55:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 19 04:23:21 2022
Response via : Initial Calibration

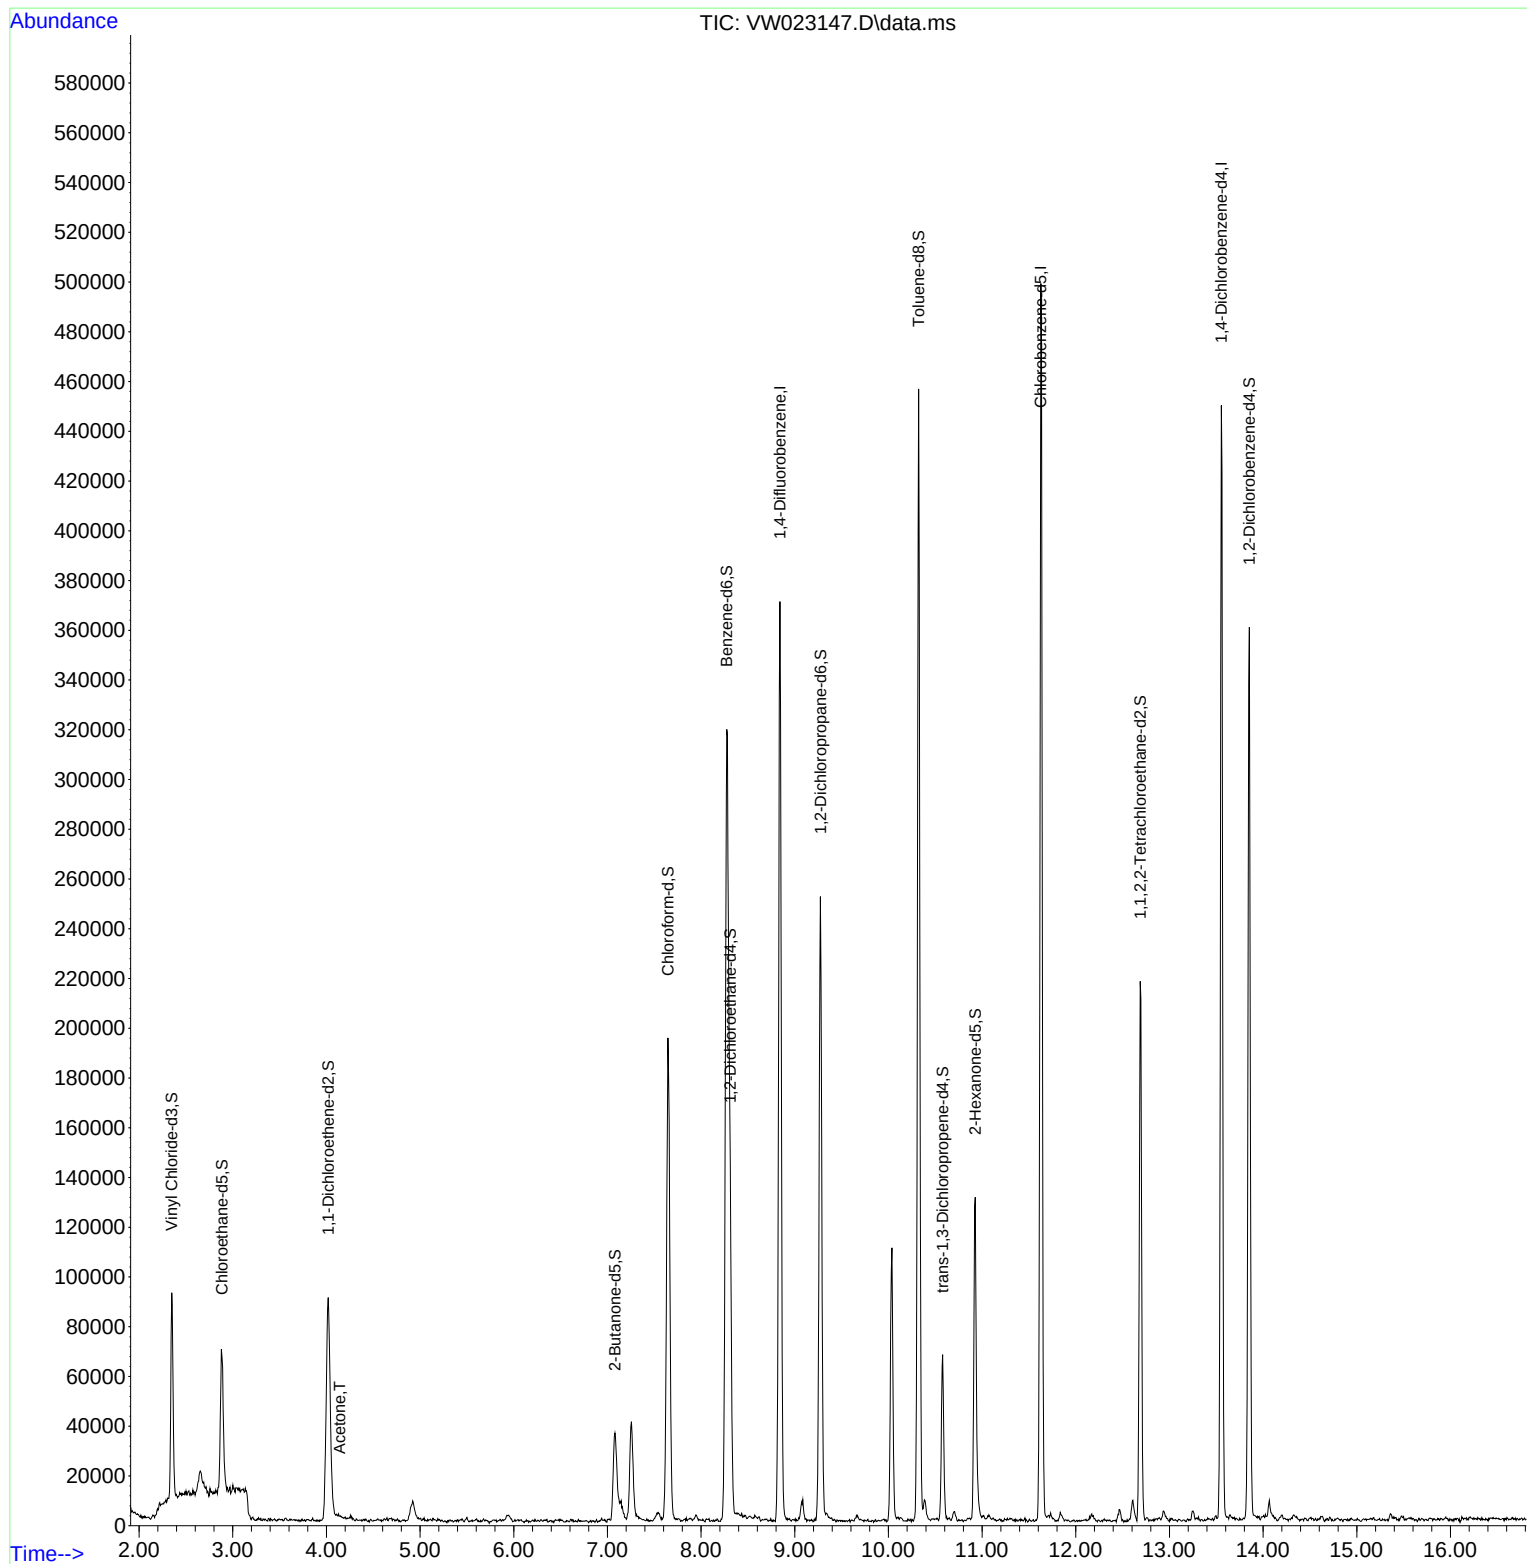

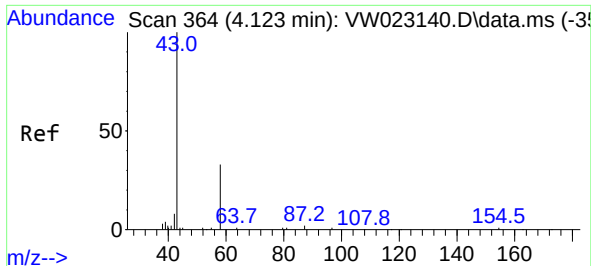

#13
 Acetone
 Concen: 3.206 ug/L
 RT: 4.141 min Scan# 30
 Delta R.T. 0.018 min
 Lab File: VW023147.D
 Acq: 18 May 2022 22:28

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY11MSD

Tgt Ion: 43 Resp: 2846
 Ion Ratio Lower Upper
 43 100
 58 13.0 0.0 64.0

