

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051823\
 Data File : VW025988.D
 Acq On : 18 May 2023 12:24
 Operator : SY/MD
 Sample : 02841-01
 Misc : 5.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11F1

Quant Time: May 19 04:37:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 19 04:36:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	798159	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	735128	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	330834	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	210485	18.610	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.440%
7) Chloroethane-d5	2.893	69	179361	21.390	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.560%
11) 1,1-Dichloroethene-d2	4.021	65	107513	18.983	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.920%
21) 2-Butanone-d5	7.075	46	181978	48.669	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.340%
24) Chloroform-d	7.648	84	505048	21.944	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.760%
26) 1,2-Dichloroethane-d4	8.307	65	293027	22.516	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.080%
32) Benzene-d6	8.276	84	1015957	21.150	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.600%
36) 1,2-Dichloropropane-d6	9.270	67	339945	22.119	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.480%
41) Toluene-d8	10.325	98	875786	20.446	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.800%
43) trans-1,3-Dichloroprop...	10.575	79	127846	20.522	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.080%
47) 2-Hexanone-d5	10.922	63	125505	47.890	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.780%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	278889	23.808	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.240%
66) 1,2-Dichlorobenzene-d4	13.848	152	288331	23.908	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.640%
Target Compounds					Qvalue	
13) Acetone	4.125	43	24773	7.472	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051823\
Data File : VW025988.D
Acq On : 18 May 2023 12:24
Operator : SY/MD
Sample : 02841-01
Misc : 5.35g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C11F1

Quant Time: May 19 04:37:52 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 19 04:36:54 2023
Response via : Initial Calibration

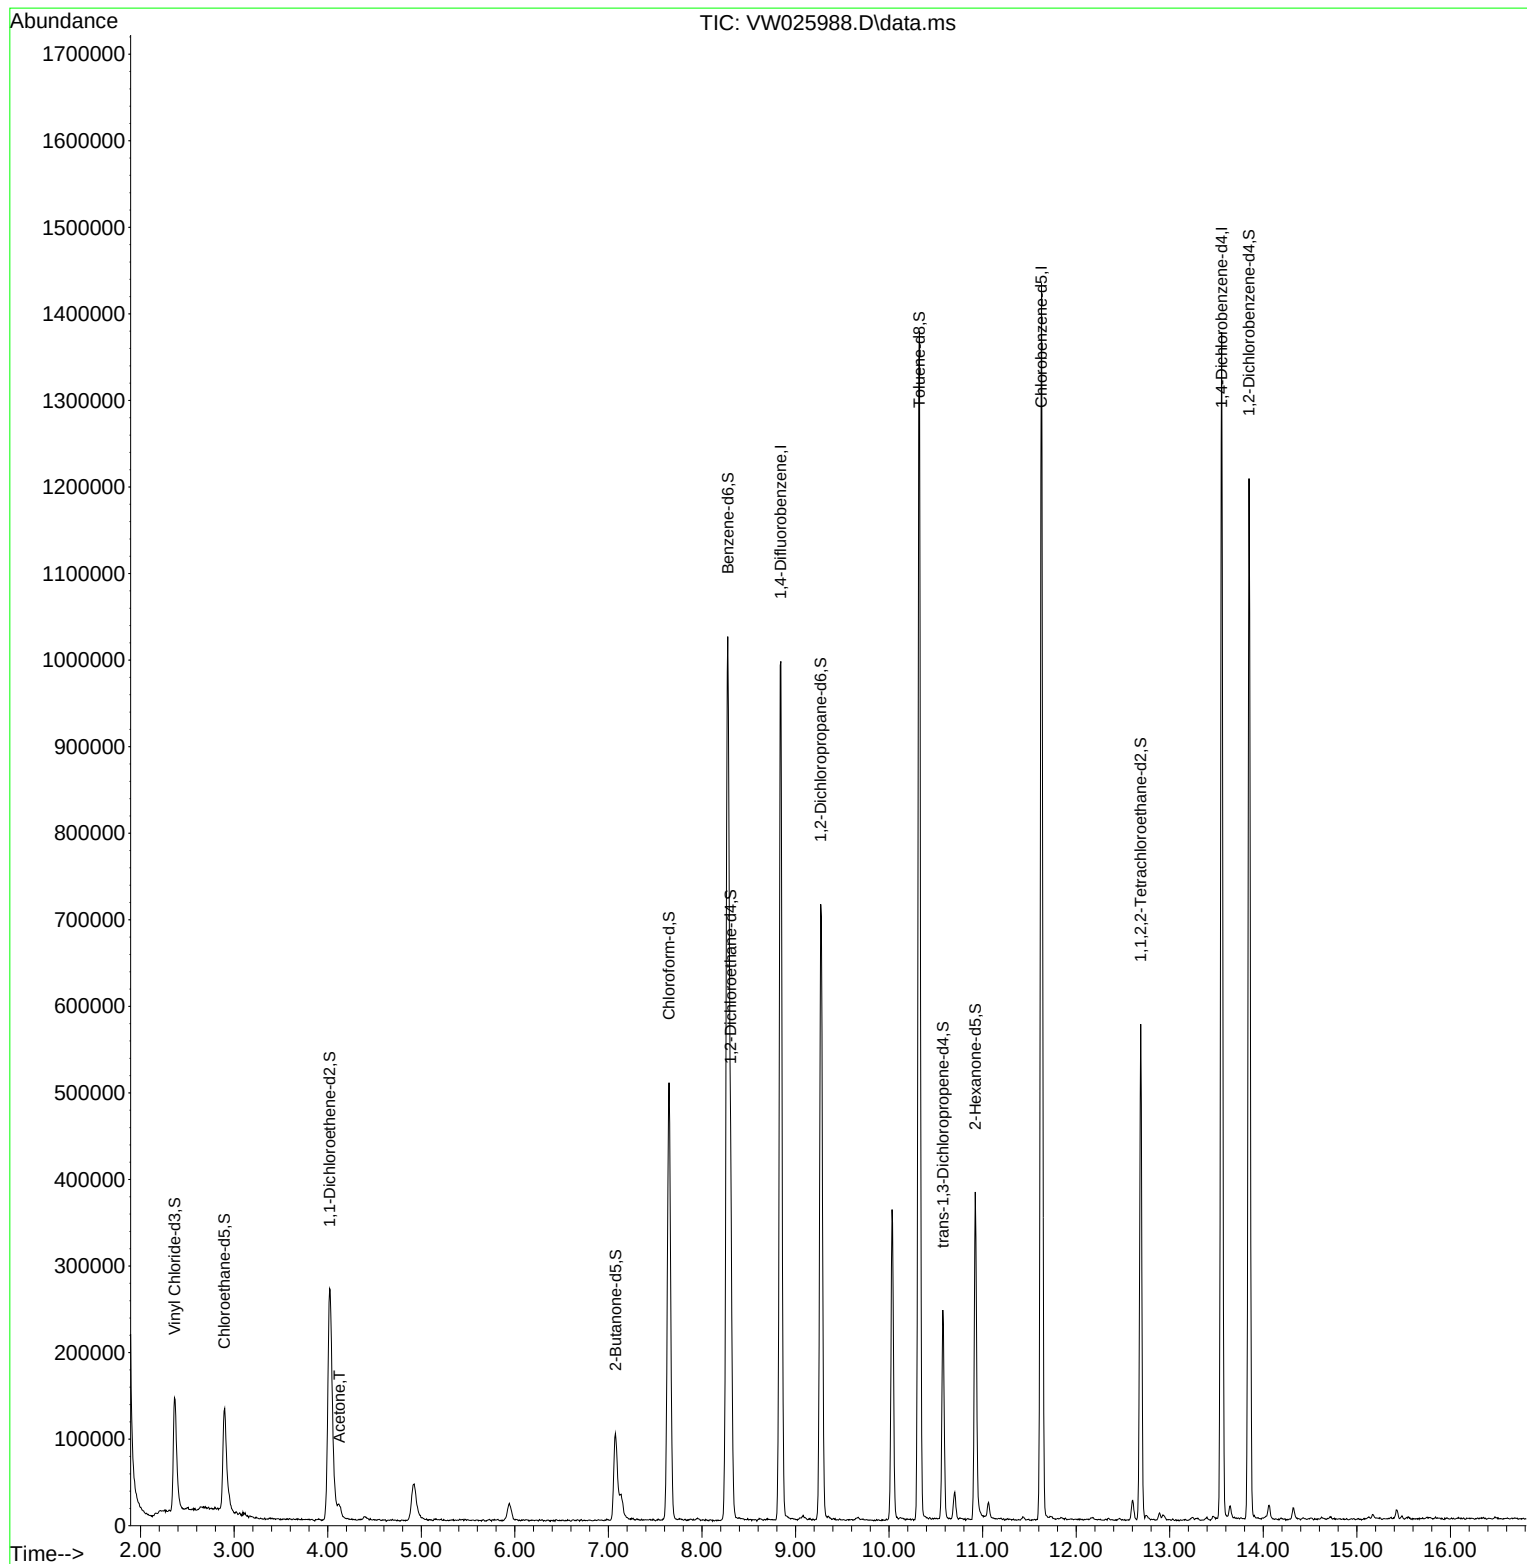

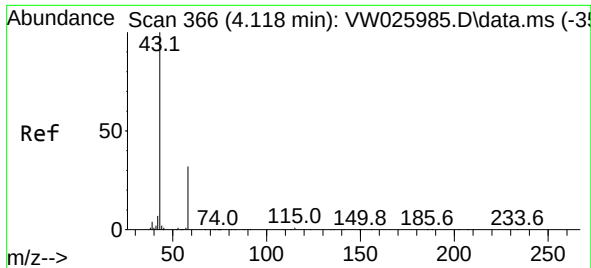

#13
 Acetone
 Concen: 7.472 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW025988.D
 Acq: 18 May 2023 12:24

Instrument :
 MSVOA_W
 ClientSampleId :
 C11F1

Tgt Ion: 43 Resp: 24773
 Ion Ratio Lower Upper
 43 100
 58 29.5 0.0 58.2

