




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051823\
 Data File : VW025986.D
 Acq On : 18 May 2023 10:36
 Operator : SY/MD
 Sample : VW0518SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK503

Manual IntegrationsAPPROVED

Quant Time: May 19 04:37:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 19 04:36:54 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/19/2023
 Supervised By :Mahesh Dadoda 05/19/2023

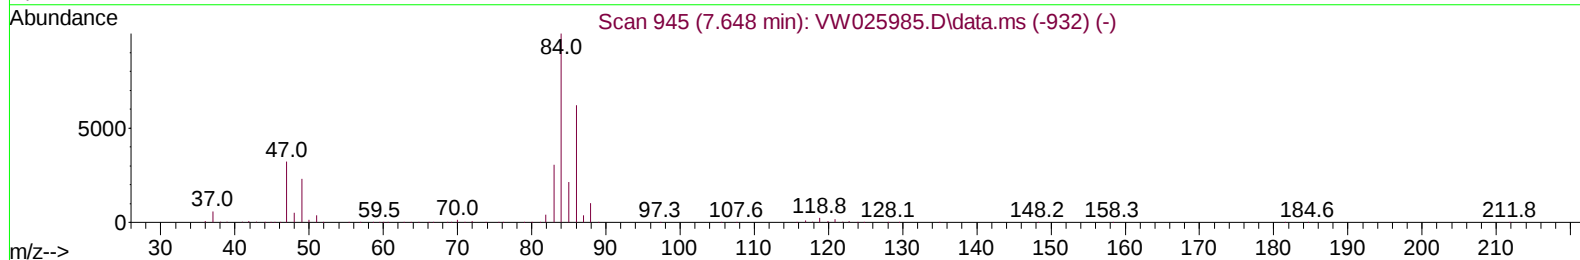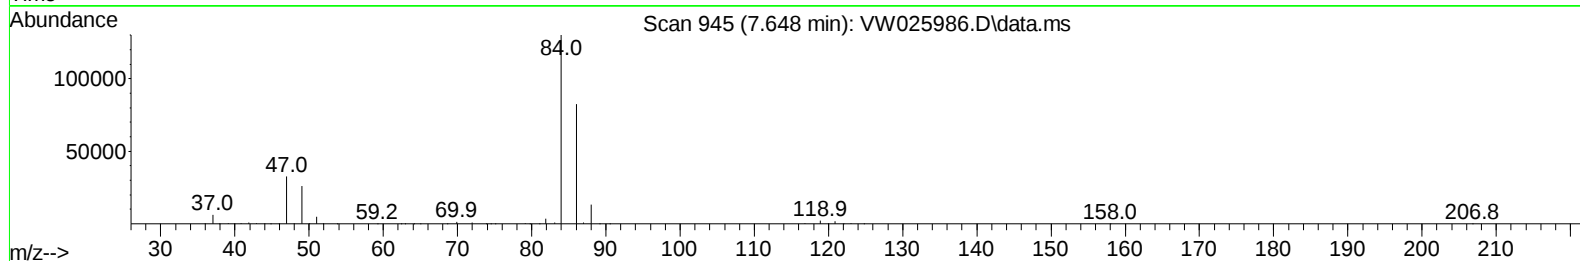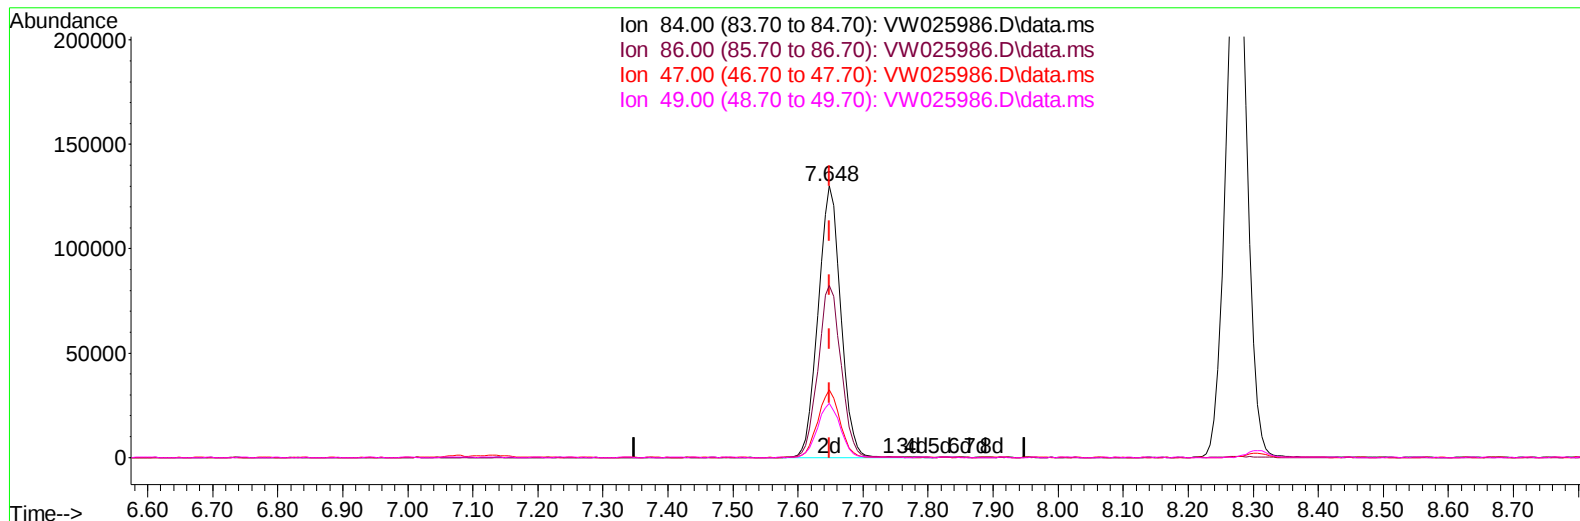

TIC: VW025986.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 23.42 ug/L m

response 311829

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.70	0.09#
47.00	50.20	0.04#
49.00	28.70	0.04#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051823\
 Data File : VW025986.D
 Acq On : 18 May 2023 10:36
 Operator : SY/MD
 Sample : VW0518SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK503

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/19/2023
 Supervised By :Mahesh Dadoda 05/19/2023

Quant Time: May 19 04:37:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 19 04:36:54 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		461653	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		429704	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		202080	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		165080	25.234	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	100.920%	
7) Chloroethane-d5	2.893	69		137760	28.404	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	113.600%	
11) 1,1-Dichloroethene-d2	4.021	65		65900	20.117	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	80.480%	
21) 2-Butanone-d5	7.075	46		99622	46.064	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	92.120%	
24) Chloroform-d	7.648	84		311829m	23.425	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	93.680%	
26) 1,2-Dichloroethane-d4	8.307	65		180781	24.016	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	96.080%	
32) Benzene-d6	8.276	84		607433	21.634	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	86.520%	
36) 1,2-Dichloropropane-d6	9.270	67		201184	22.395	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	89.560%	
41) Toluene-d8	10.319	98		517802	20.681	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	82.720%	
43) trans-1,3-Dichloroprop...	10.575	79		73943	20.306	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	81.240%	
47) 2-Hexanone-d5	10.922	63		67282	43.921	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	87.840%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		161325	23.561	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	94.240%	
66) 1,2-Dichlorobenzene-d4	13.848	152		178787	24.270	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	97.080%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051823\
Data File : VW025986.D
Acq On : 18 May 2023 10:36
Operator : SY/MD
Sample : VW0518SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK503

Manual IntegrationsAPPROVED

Quant Time: May 19 04:37:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 19 04:36:54 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/19/2023
Supervised By :Mahesh Dadoda 05/19/2023

