

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051823\
 Data File : VW025989.D
 Acq On : 18 May 2023 12:48
 Operator : SY/MD
 Sample : 02841-02
 Misc : 5.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11F2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/19/2023
 Supervised By :Mahesh Dadoda 05/19/2023

Quant Time: May 19 04:38:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 19 04:36:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	840523	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	768177	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	342476	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	209298	17.572	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.280%		
7) Chloroethane-d5	2.893	69	180418	20.432	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.720%		
11) 1,1-Dichloroethene-d2	4.021	65	109457	18.353	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	73.400%		
21) 2-Butanone-d5	7.075	46	217611	55.265	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.540%		
24) Chloroform-d	7.648	84	531549	21.932	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.720%		
26) 1,2-Dichloroethane-d4	8.301	65	323534m	23.607	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	94.440%		
32) Benzene-d6	8.270	84	1047194	20.863	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.440%		
36) 1,2-Dichloropropane-d6	9.270	67	357709	22.274	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	89.080%		
41) Toluene-d8	10.318	98	916597	20.478	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.920%		
43) trans-1,3-Dichloroprop...	10.574	79	140437	21.573	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.280%		
47) 2-Hexanone-d5	10.922	63	150368	54.908	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	109.820%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	320313	26.168	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	104.680%		
66) 1,2-Dichlorobenzene-d4	13.848	152	309961	24.827	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.320%		
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	39125	2.257	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051823\
Data File : VW025989.D
Acq On : 18 May 2023 12:48
Operator : SY/MD
Sample : 02841-02
Misc : 5.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C11F2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/19/2023
Supervised By :Mahesh Dadoda 05/19/2023


Quant Time: May 19 04:38:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 19 04:36:54 2023
Response via : Initial Calibration

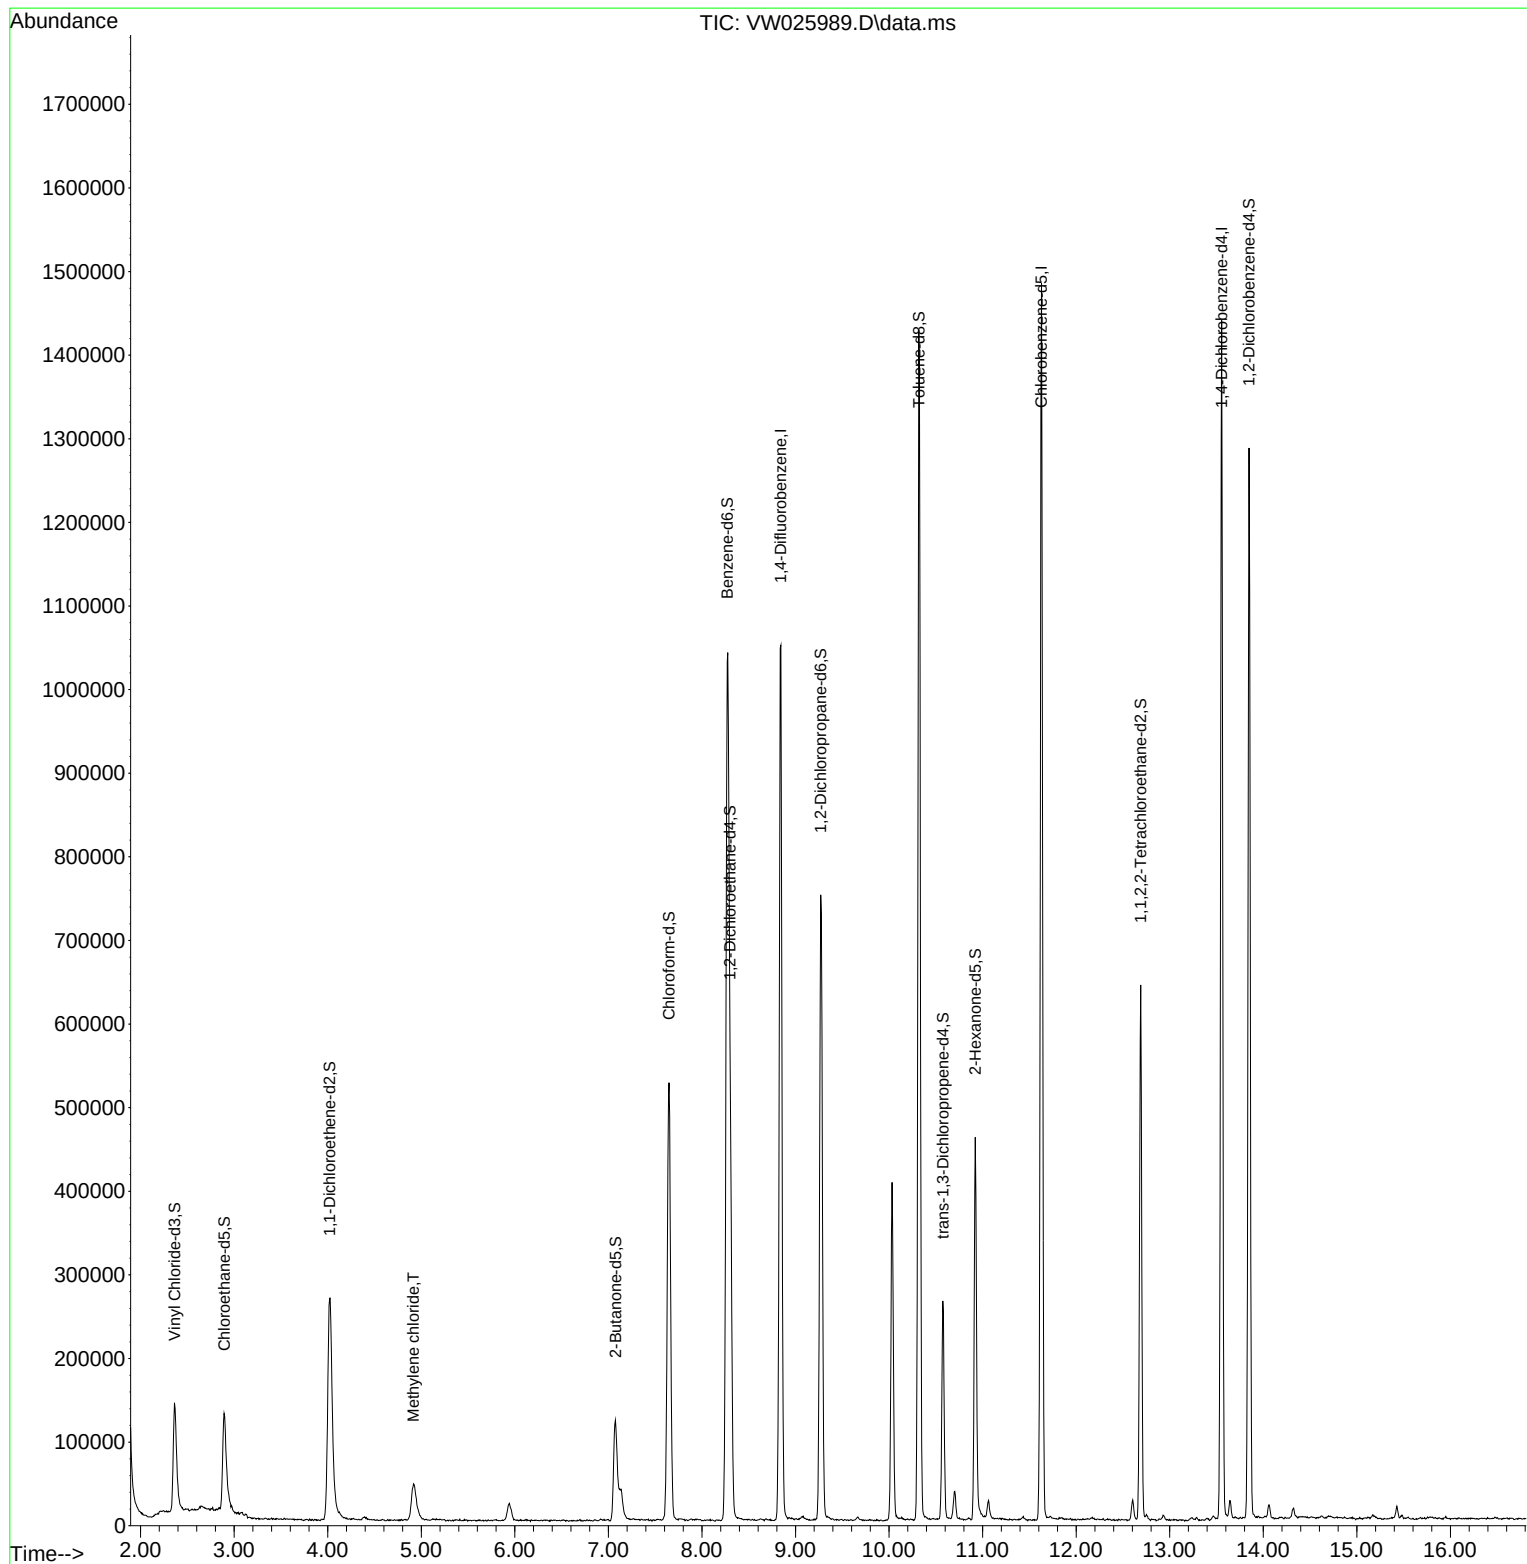

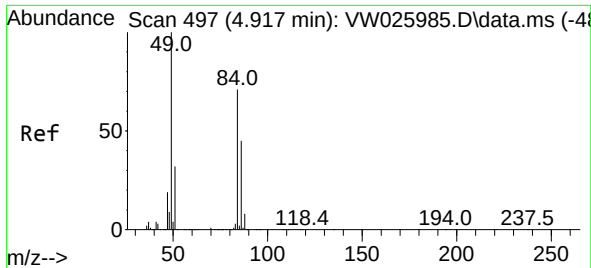

#16
Methylene chloride
Concen: 2.257 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW025989.D
Acq: 18 May 2023 12:48

Instrument :
MSVOA_W
ClientSampleId :
C11F2

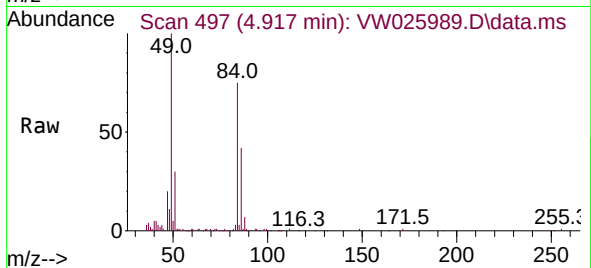

Tgt Ion: 84 Resp: 39125
Ion Ratio Lower Upper
84 100
86 56.4 41.7 77.5
49 132.9 95.3 177.1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/19/2023
Supervised By :Mahesh Dadoda 05/19/2023

