

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
 Data File : VW023176.D
 Acq On : 19 May 2022 16:31
 Operator : SY/VA
 Sample : N2848-14RE
 Misc : 4.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY00

Quant Time: May 20 01:51:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 01:47:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	388470	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	393472	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	159139	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	150391	18.870	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.480%
7) Chloroethane-d5	2.885	69	112432	21.683	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.720%
11) 1,1-Dichloroethene-d2	4.220	63	101	0.010	ug/L	0.21
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.040%#
21) 2-Butanone-d5	7.080	46	58338	38.498	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.000%
24) Chloroform-d	7.647	84	224853	19.756	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.040%
26) 1,2-Dichloroethane-d4	8.305	65	133265	21.349	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.400%
32) Benzene-d6	8.275	84	486021	21.430	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.720%
36) 1,2-Dichloropropane-d6	9.274	67	136136	21.369	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.480%
41) Toluene-d8	10.323	98	475230	21.692	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.760%
43) trans-1,3-Dichloroprop...	10.579	79	55444	18.901	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.600%
47) 2-Hexanone-d5	10.920	63	49581	40.768	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.540%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	115441	19.441	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	126357	22.714	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.840%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	5243	0.603	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
Data File : VW023176.D
Acq On : 19 May 2022 16:31
Operator : SY/VA
Sample : N2848-14RE
Misc : 4.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY00

Quant Time: May 20 01:51:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 20 01:47:53 2022
Response via : Initial Calibration

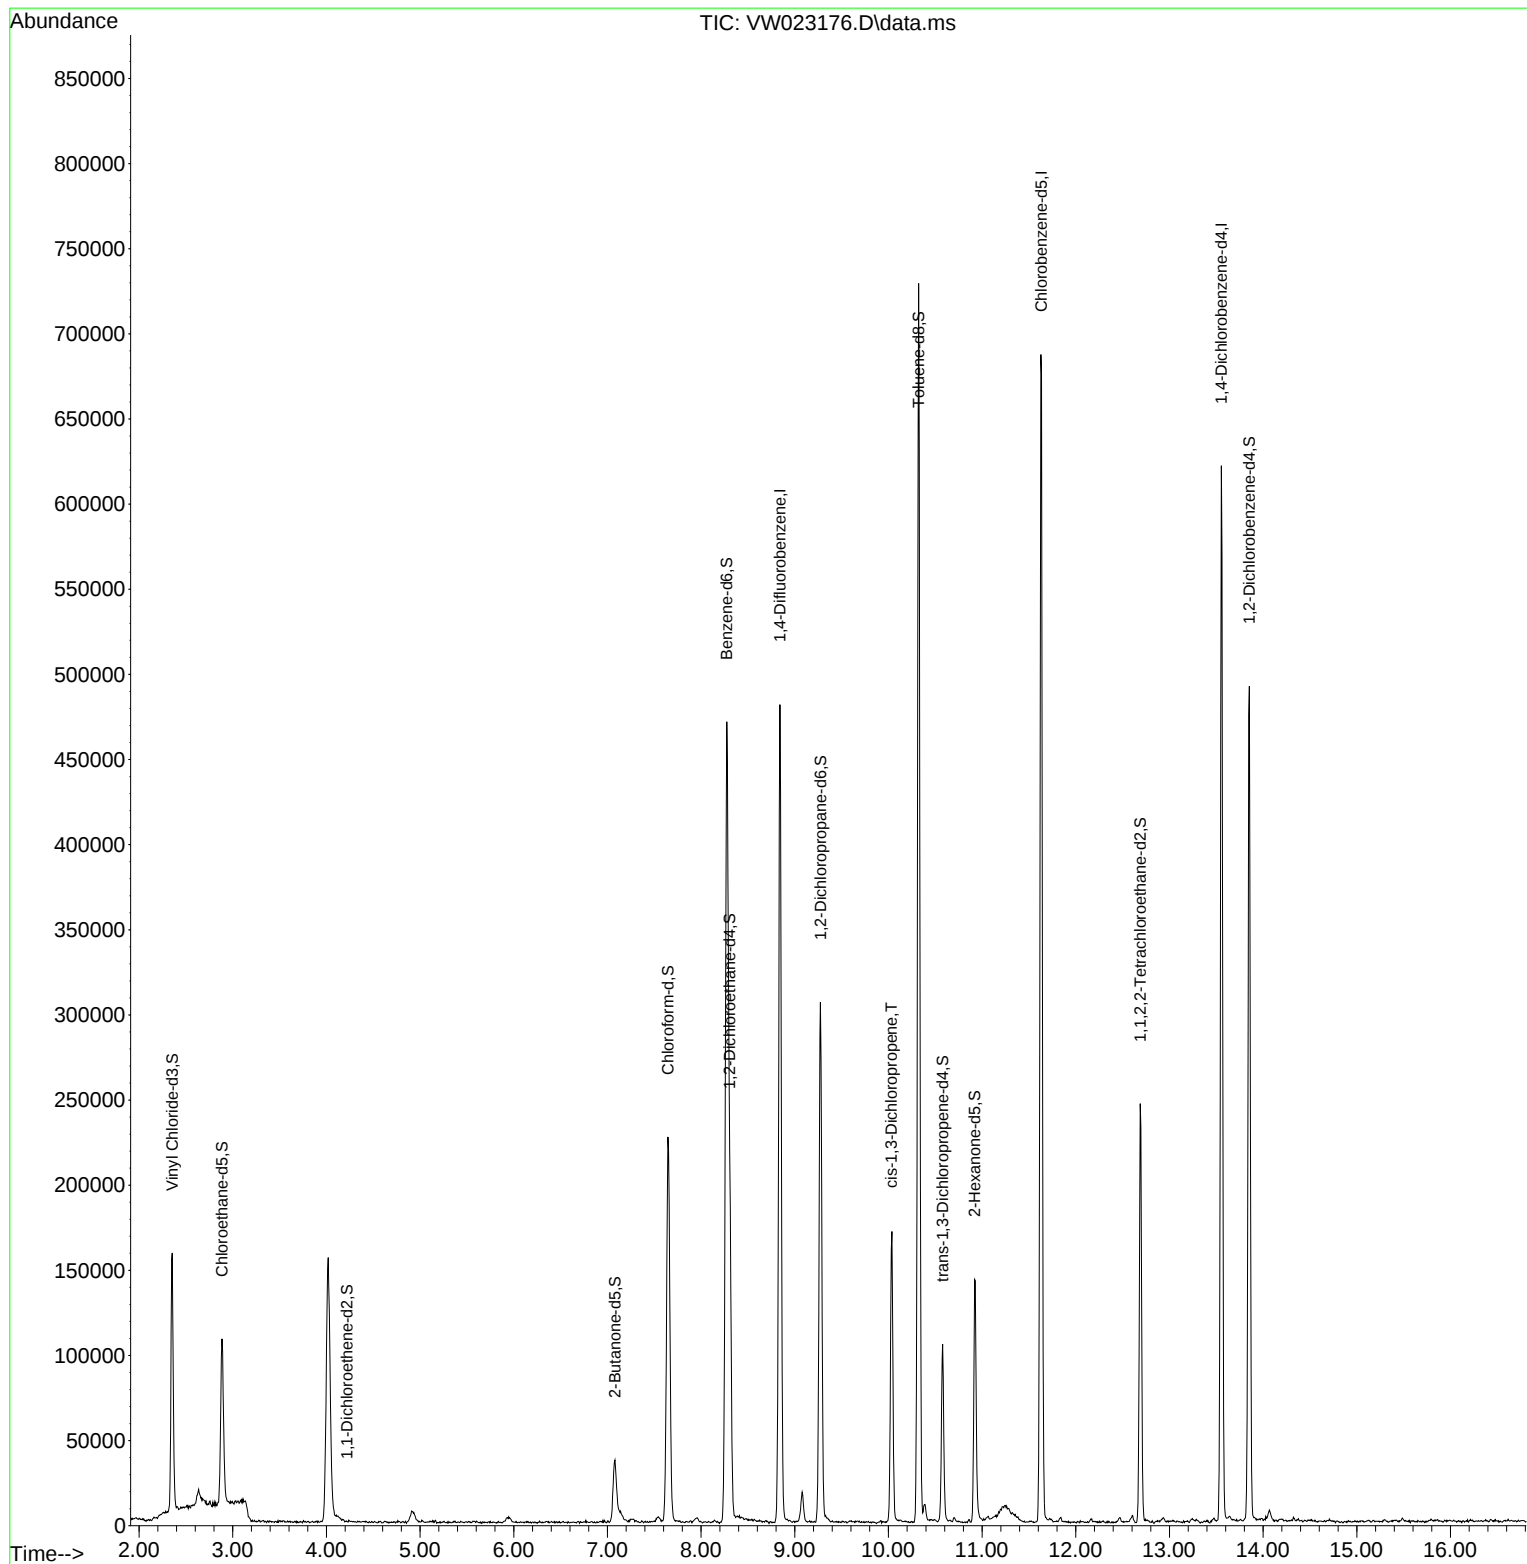

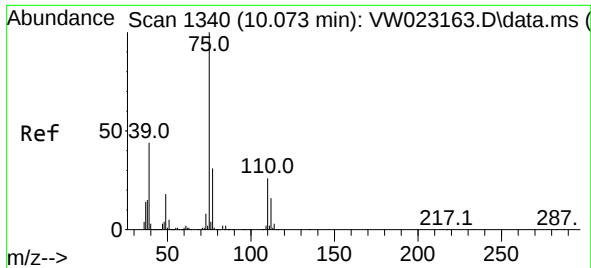

#39
 cis-1,3-Dichloropropene
 Concen: 0.603 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW023176.D
 Acq: 19 May 2022 16:31

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY00

Tgt Ion: 75 Resp: 5243
 Ion Ratio Lower Upper
 75 100
 77 32.5 22.1 41.1

