




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
 Data File : VW023176.D
 Acq On : 19 May 2022 16:31
 Operator : SY/VA
 Sample : N2848-14RE
 Misc : 4.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY00

Manual IntegrationsAPPROVED

Quant Time: May 20 01:51:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 01:47:53 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/26/2022

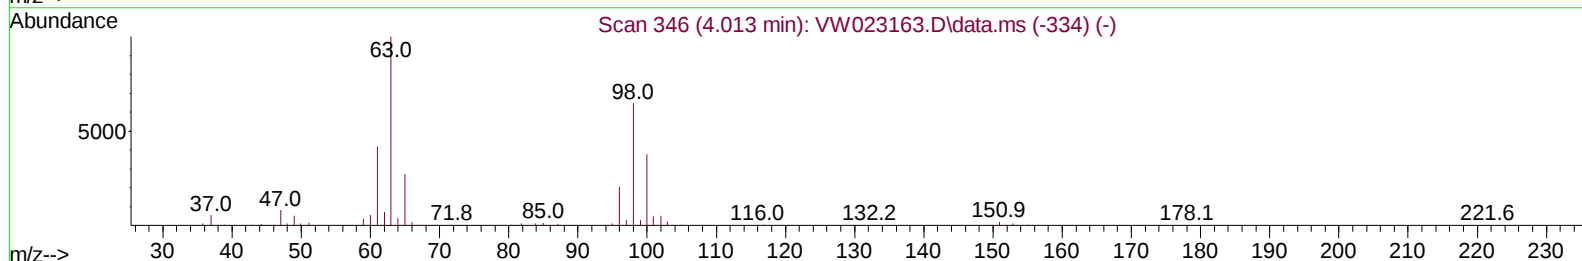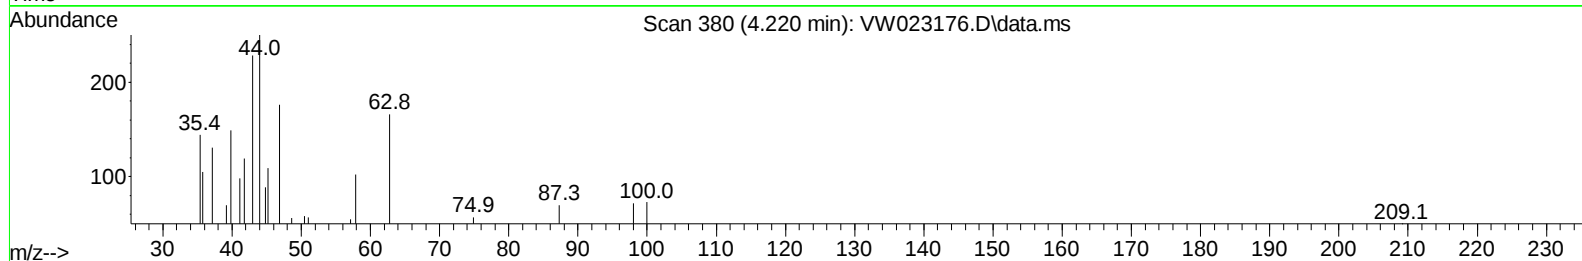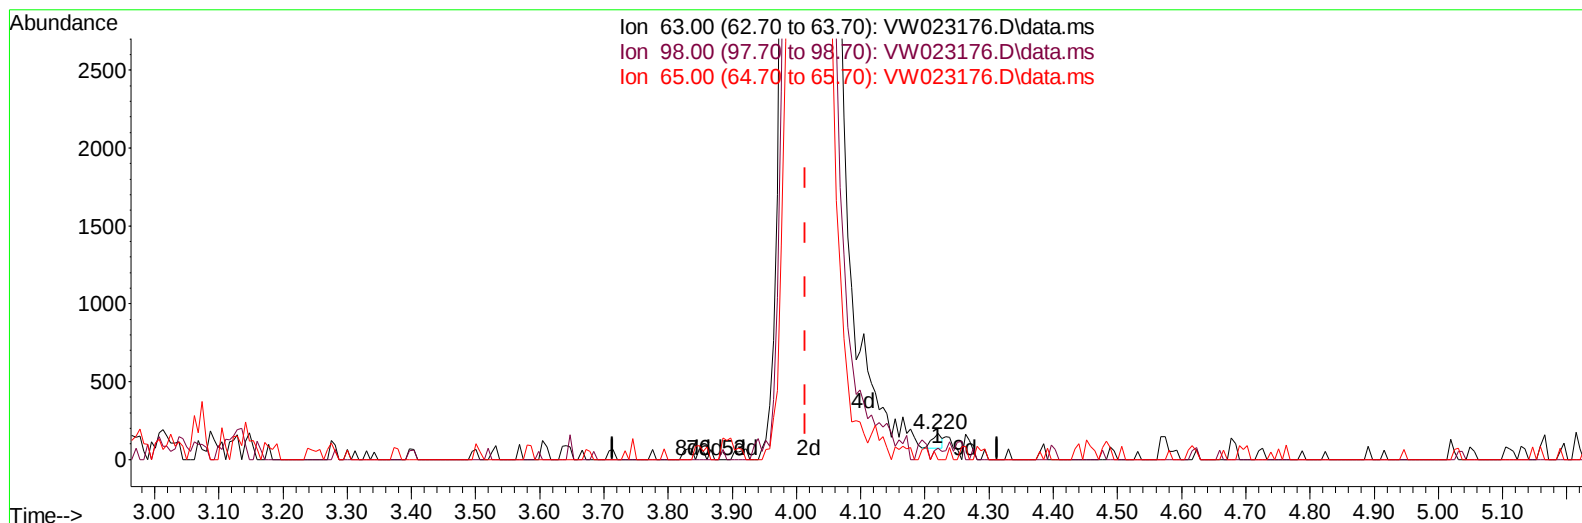

TIC: VW023176.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.220min (+ 0.207) 0.01 ug/L

response 101

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	64.36
65.00	23.30	18.81
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
 Data File : VW023176.D
 Acq On : 19 May 2022 16:31
 Operator : SY/VA
 Sample : N2848-14RE
 Misc : 4.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY00

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 20 01:51:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 01:47:53 2022
 Response via : Initial Calibration

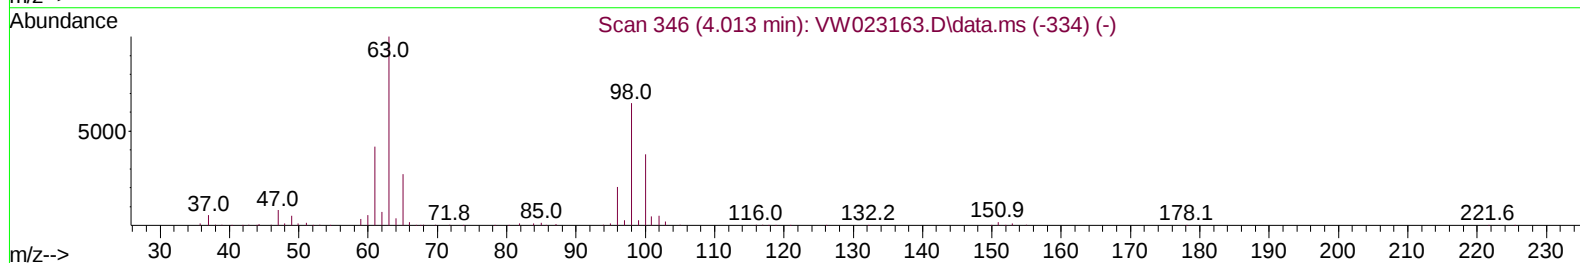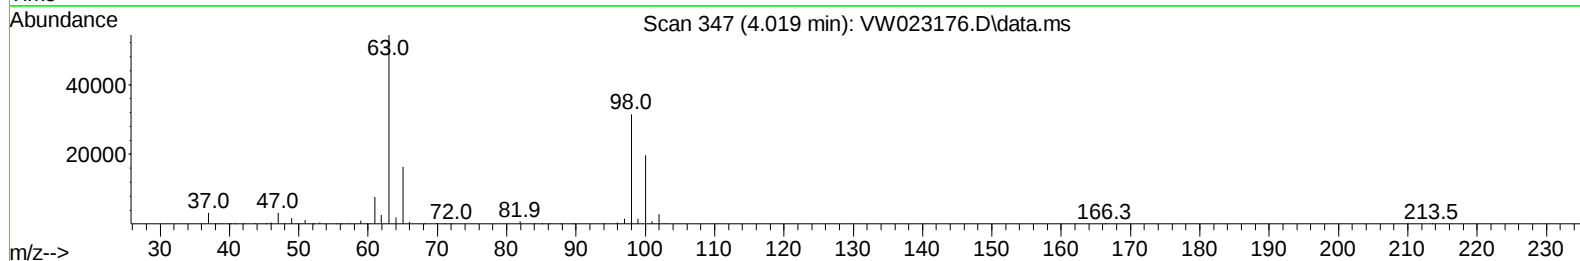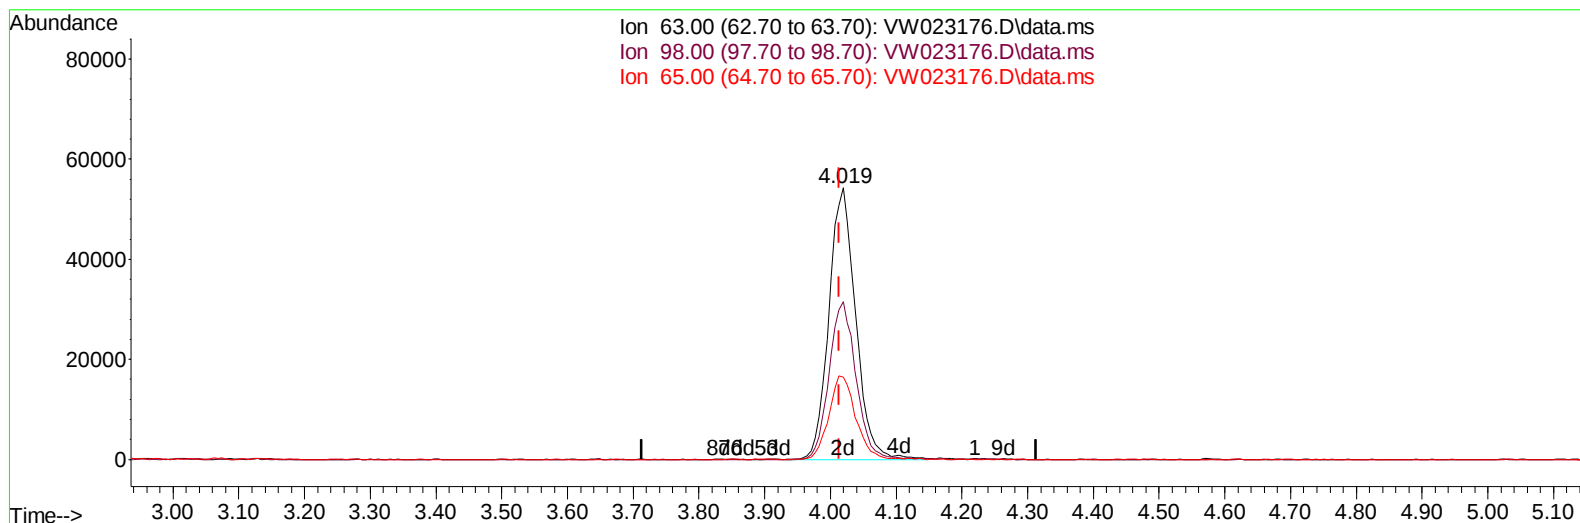

TIC: VW023176.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (+ 0.006) 14.92 ug/L m

response 153637

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.04#
65.00	23.30	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
 Data File : VW023176.D
 Acq On : 19 May 2022 16:31
 Operator : SY/VA
 Sample : N2848-14RE
 Misc : 4.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY00

Manual IntegrationsAPPROVED

Quant Time: May 20 01:51:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 01:47:53 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	388470	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	393472	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	159139	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	150391	18.870	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.480%		
7) Chloroethane-d5	2.885	69	112432	21.683	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	86.720%		
11) 1,1-Dichloroethene-d2	4.019	63	153637m	14.919	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	59.680%		
21) 2-Butanone-d5	7.080	46	58338	38.498	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.000%		
24) Chloroform-d	7.647	84	224853	19.756	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	79.040%		
26) 1,2-Dichloroethane-d4	8.305	65	133265	21.349	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	85.400%		
32) Benzene-d6	8.275	84	486021	21.430	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.720%		
36) 1,2-Dichloropropane-d6	9.274	67	136136	21.369	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	85.480%		
41) Toluene-d8	10.323	98	475230	21.692	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.760%		
43) trans-1,3-Dichloroprop...	10.579	79	55444	18.901	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	75.600%		
47) 2-Hexanone-d5	10.920	63	49581	40.768	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.540%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	115441	19.441	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	77.760%		
66) 1,2-Dichlorobenzene-d4	13.853	152	126357	22.714	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.840%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
Data File : VW023176.D
Acq On : 19 May 2022 16:31
Operator : SY/VA
Sample : N2848-14RE
Misc : 4.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY00

Manual IntegrationsAPPROVED

Quant Time: May 20 01:51:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 20 01:47:53 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
Supervised By :Mahesh Dadoda 05/26/2022

