




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
 Data File : VW023177.D
 Acq On : 19 May 2022 16:55
 Operator : SY/VA
 Sample : N2848-20RE
 Misc : 4.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXZ9RE

Manual IntegrationsAPPROVED

Quant Time: May 20 01:52:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 01:47:53 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/26/2022

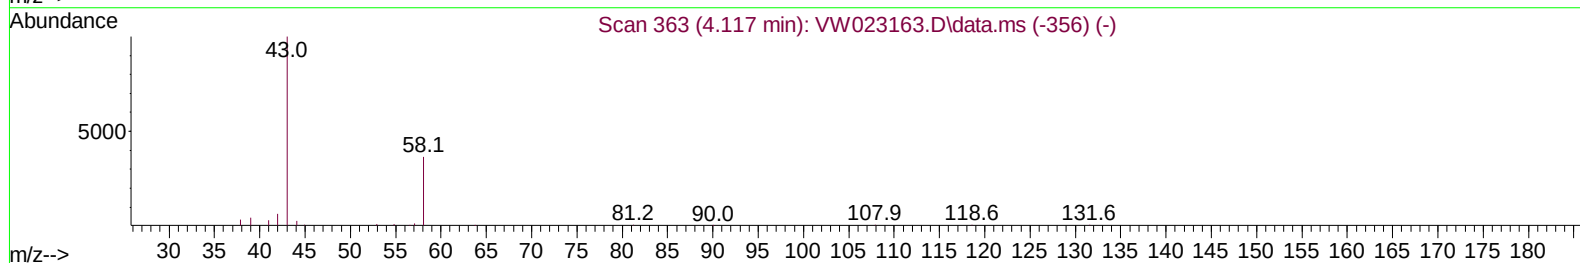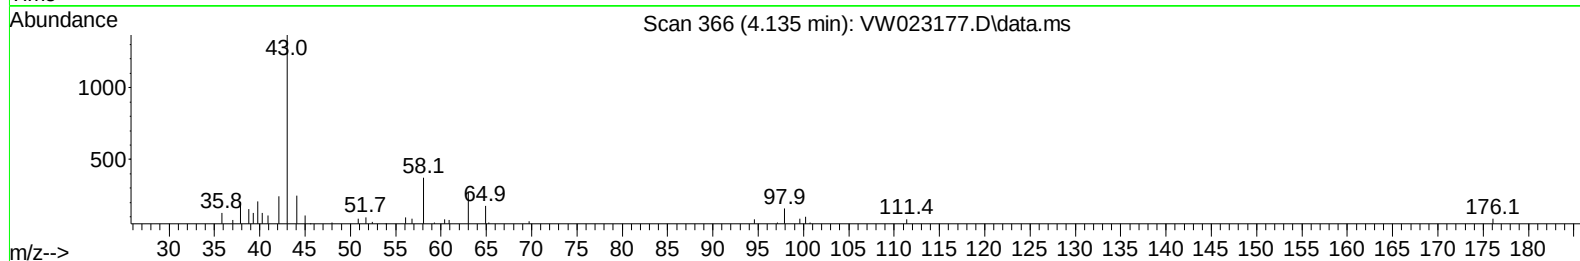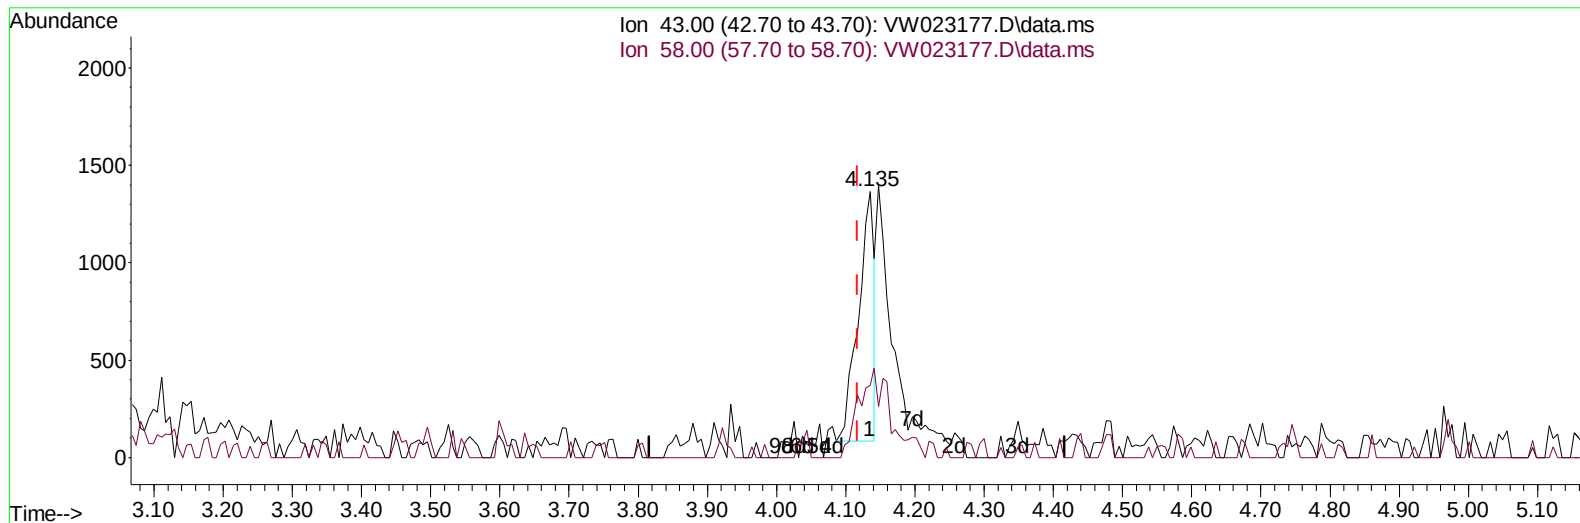

TIC: VW023177.D\data.ms

(13) Acetone (T)

4.135min (+ 0.018) 2.97 ug/L

response 2058

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	42.52
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
 Data File : VW023177.D
 Acq On : 19 May 2022 16:55
 Operator : SY/VA
 Sample : N2848-20RE
 Misc : 4.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXZ9RE

Manual IntegrationsAPPROVED

Quant Time: May 20 01:52:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 01:47:53 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/26/2022

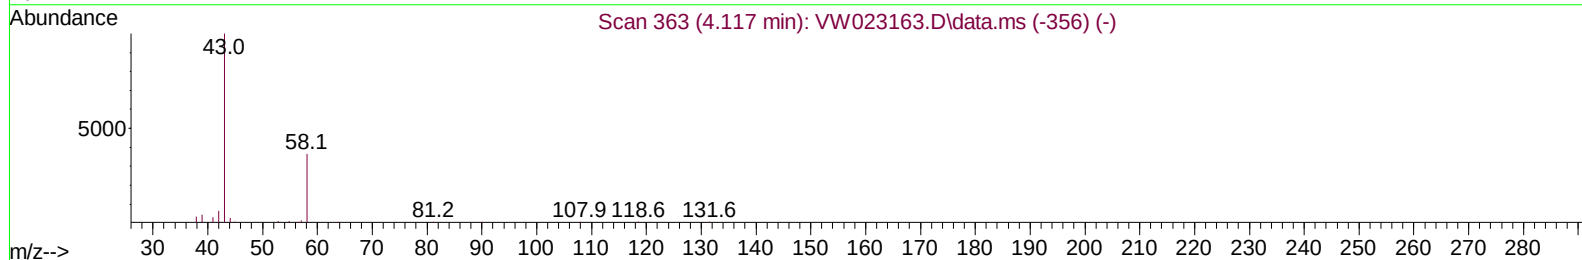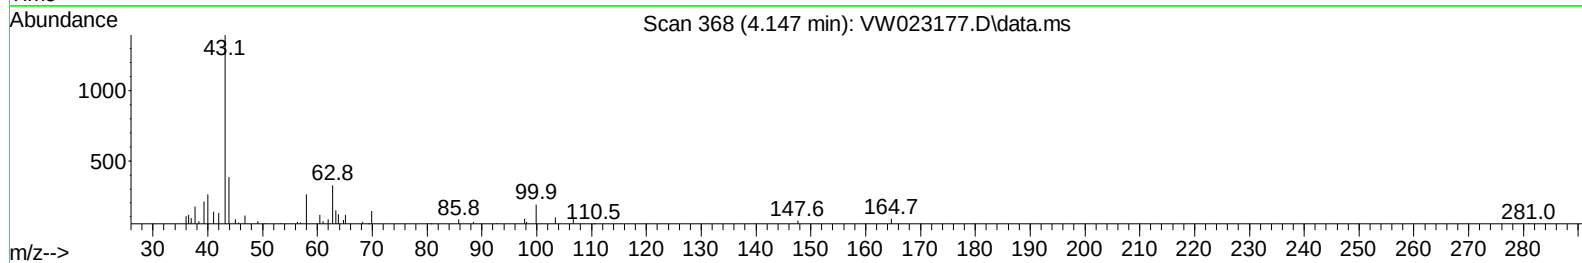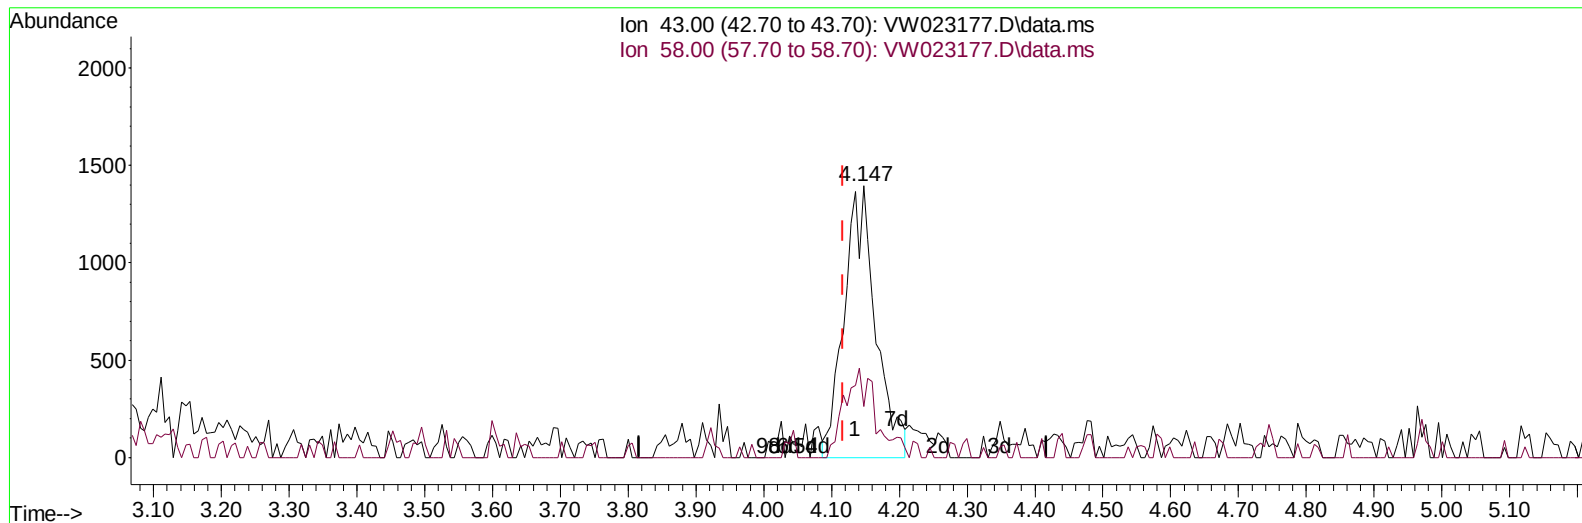

TIC: VW023177.D\data.ms

(13) Acetone (T)

4.147min (+ 0.031) 6.47 ug/L m

response 4478

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	19.54
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
 Data File : VW023177.D
 Acq On : 19 May 2022 16:55
 Operator : SY/VA
 Sample : N2848-20RE
 Misc : 4.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXZ9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 20 01:52:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 01:47:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	236873	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	207373	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	73432	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	166077	34.174	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	136.680%	
7) Chloroethane-d5	2.885	69	118092	37.351	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	149.400%	
11) 1,1-Dichloroethene-d2	4.013	63	156673	24.950	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	99.800%	
21) 2-Butanone-d5	7.086	46	54181	58.637	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	117.280%	
24) Chloroform-d	7.647	84	221660	31.940	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	127.760%	
26) 1,2-Dichloroethane-d4	8.305	65	130186	34.203	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	136.800%#	
32) Benzene-d6	8.275	84	488832	40.897	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	163.600%#	
36) 1,2-Dichloropropane-d6	9.275	67	138066	41.121	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	164.480%#	
41) Toluene-d8	10.323	98	438760	37.999	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	152.000%#	
43) trans-1,3-Dichloroprop...	10.579	79	48703	31.503	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	126.000%	
47) 2-Hexanone-d5	10.927	63	41520	64.778	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	129.560%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	84270	26.928	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	107.720%	
66) 1,2-Dichlorobenzene-d4	13.847	152	102291	39.849	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	159.400%#	
Target Compounds						Qvalue
13) Acetone	4.147	43	4478m	6.473	ug/L	
25) Chloroform	7.677	83	18987	2.968	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051922\
Data File : VW023177.D
Acq On : 19 May 2022 16:55
Operator : SY/VA
Sample : N2848-20RE
Misc : 4.84g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXXZ9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 20 01:52:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 20 01:47:53 2022
Response via : Initial Calibration

