

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW051922\  
 Data File : VW023179.D  
 Acq On : 19 May 2022 17:45  
 Operator : SY/VA  
 Sample : N2926-02MS  
 Misc : 4.83g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 EXY11MS

Manual Integrations  
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/20/2022  
 Supervised By : Mahesh Dadoda 05/26/2022

Quant Time: May 20 01:52:29 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM050222SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Fri May 20 01:47:53 2022  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 8.848  | 114   | 86685    | 25.000   | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 11.634 | 117   | 78459    | 25.000   | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 13.560 | 152   | 35112    | 25.000   | ug/L   | 0.00     |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 2.355  | 65    | 34070    | 19.157   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 30 - 150 | Recovery | =      | 76.640%  |
| 7) Chloroethane-d5            | 2.885  | 69    | 31140    | 26.914   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 30 - 150 | Recovery | =      | 107.640% |
| 11) 1,1-Dichloroethene-d2     | 4.013  | 63    | 46004    | 20.019   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 45 - 110 | Recovery | =      | 80.080%  |
| 21) 2-Butanone-d5             | 7.080  | 46    | 14240    | 42.112   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 20 - 135 | Recovery | =      | 84.220%  |
| 24) Chloroform-d              | 7.653  | 84    | 56642    | 22.303   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 40 - 150 | Recovery | =      | 89.200%  |
| 26) 1,2-Dichloroethane-d4     | 8.305  | 65    | 29524    | 21.196   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 70 - 130 | Recovery | =      | 84.800%  |
| 32) Benzene-d6                | 8.275  | 84    | 105089   | 23.238   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 20 - 135 | Recovery | =      | 92.960%  |
| 36) 1,2-Dichloropropane-d6    | 9.275  | 67    | 30291    | 23.845   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 70 - 120 | Recovery | =      | 95.360%  |
| 41) Toluene-d8                | 10.323 | 98    | 94156    | 21.553   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 30 - 130 | Recovery | =      | 86.200%  |
| 43) trans-1,3-Dichloroprop... | 10.579 | 79    | 11310    | 19.336   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 30 - 135 | Recovery | =      | 77.360%  |
| 47) 2-Hexanone-d5             | 10.921 | 63    | 7973     | 32.878   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 20 - 135 | Recovery | =      | 65.760%  |
| 56) 1,1,2,2-Tetrachloroeth... | 12.689 | 84    | 27480    | 23.209   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 45 - 120 | Recovery | =      | 92.840%  |
| 66) 1,2-Dichlorobenzene-d4    | 13.853 | 152   | 26885    | 21.904   | ug/L   | 0.00     |
| Spiked Amount                 | 25.000 | Range | 75 - 120 | Recovery | =      | 87.600%  |
| Target Compounds              |        |       |          |          |        |          |
|                               |        |       |          |          | Qvalue |          |
| 2) Dichlorodifluoromethane    | 2.001  | 85    | 1774     | 3.754    | ug/L   | 92       |
| 3) Chloromethane              | 2.221  | 50    | 15990    | 17.511   | ug/L   | 93       |
| 5) Vinyl chloride             | 2.361  | 62    | 30721    | 16.764   | ug/L   | 96       |
| 6) Bromomethane               | 2.782  | 94    | 16954    | 14.409   | ug/L   | 91       |
| 8) Chloroethane               | 2.922  | 64    | 21442    | 24.258   | ug/L   | 96       |
| 9) Trichlorofluoromethane     | 3.263  | 101   | 36528    | 43.610   | ug/L   | 97       |
| 10) 1,1,2-Trichloro-1,2,2-... | 4.062  | 101   | 24273    | 19.381   | ug/L   | 95       |
| 12) 1,1-Dichloroethene        | 4.038  | 96    | 19037    | 17.147   | ug/L   | 80       |
| 13) Acetone                   | 4.129  | 43    | 12694    | 50.141   | ug/L   | 80       |
| 14) Carbon disulfide          | 4.391  | 76    | 34683    | 11.395   | ug/L   | 98       |
| 15) Methyl Acetate            | 4.684  | 43    | 9442m    | 18.564   | ug/L   |          |
| 16) Methylene chloride        | 4.916  | 84    | 23100    | 18.212   | ug/L   | 91       |
| 17) trans-1,2-Dichloroethene  | 5.428  | 96    | 19622    | 15.705   | ug/L   | 93       |
| 18) Methyl tert-butyl Ether   | 5.434  | 73    | 47176    | 24.735   | ug/L # | 93       |
| 19) 1,1-Dichloroethane        | 6.220  | 63    | 40173    | 18.972   | ug/L   | 96       |
| 20) cis-1,2-Dichloroethene    | 7.177  | 96    | 22722    | 16.932   | ug/L # | 96       |
| 22) 2-Butanone                | 7.177  | 43    | 11910    | 33.639   | ug/L   | 95       |
| 23) Bromochloromethane        | 7.519  | 128   | 10813    | 17.205   | ug/L   | 95       |
| 25) Chloroform                | 7.677  | 83    | 44991    | 19.215   | ug/L   | 91       |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW051922\  
 Data File : VW023179.D  
 Acq On : 19 May 2022 17:45  
 Operator : SY/VA  
 Sample : N2926-02MS  
 Misc : 4.83g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 EXY11MS

Manual Integrations  
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022  
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 20 01:52:29 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM050222SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Fri May 20 01:47:53 2022  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| 27) 1,2-Dichloroethane        | 8.397  | 62   | 28282    | 18.120 | ug/L # | 94       |
| 29) Cyclohexane               | 7.958  | 56   | 27049    | 15.941 | ug/L   | 95       |
| 30) 1,1,1-Trichloroethane     | 7.872  | 97   | 40069    | 21.611 | ug/L   | 99       |
| 31) Carbon tetrachloride      | 8.067  | 117  | 34447    | 19.861 | ug/L   | 97       |
| 33) Benzene                   | 8.323  | 78   | 90449    | 19.569 | ug/L   | 100      |
| 34) Trichloroethene           | 9.092  | 95   | 23713    | 18.655 | ug/L   | 90       |
| 35) Methylcyclohexane         | 9.335  | 83   | 29280    | 14.022 | ug/L   | 98       |
| 37) 1,2-Dichloropropane       | 9.372  | 63   | 21378    | 19.113 | ug/L   | 98       |
| 38) Bromodichloromethane      | 9.646  | 83   | 30421    | 19.148 | ug/L   | 100      |
| 39) cis-1,3-Dichloropropene   | 10.073 | 75   | 28336    | 16.338 | ug/L   | 99       |
| 40) 4-Methyl-2-pentanone      | 10.213 | 43   | 22637    | 32.109 | ug/L   | 97       |
| 42) Toluene                   | 10.390 | 91   | 96287    | 18.589 | ug/L   | 95       |
| 44) trans-1,3-Dichloropropene | 10.610 | 75   | 24472    | 15.809 | ug/L   | 100      |
| 45) 1,1,2-Trichloroethane     | 10.786 | 97   | 19016    | 20.337 | ug/L   | 98       |
| 46) Tetrachloroethene         | 10.860 | 164  | 17527    | 18.348 | ug/L   | 84       |
| 48) 2-Hexanone                | 10.969 | 43   | 15263    | 32.402 | ug/L   | 97       |
| 49) Dibromochloromethane      | 11.128 | 129  | 20637    | 18.338 | ug/L   | 94       |
| 50) 1,2-Dibromoethane         | 11.238 | 107  | 16933    | 18.035 | ug/L   | 99       |
| 51) Chlorobenzene             | 11.658 | 112  | 61550    | 18.024 | ug/L   | 93       |
| 52) Ethylbenzene              | 11.731 | 91   | 99381    | 17.245 | ug/L   | 97       |
| 53) m,p-Xylene                | 11.841 | 106  | 38971    | 17.163 | ug/L   | 99       |
| 54) o-Xylene                  | 12.164 | 106  | 38200    | 17.531 | ug/L   | 97       |
| 55) Styrene                   | 12.183 | 104  | 62370    | 16.845 | ug/L   | 95       |
| 57) 1,1,2,2-Tetrachloroethane | 12.713 | 83   | 21822    | 18.685 | ug/L   | 98       |
| 59) Bromoform                 | 12.347 | 173  | 9163     | 18.414 | ug/L   | 92       |
| 60) Isopropylbenzene          | 12.463 | 105  | 103698   | 21.558 | ug/L   | 99       |
| 61) 1,2,3-Trichloropropane    | 12.768 | 75   | 15941    | 22.722 | ug/L   | 98       |
| 62) 1,3,5-Trimethylbenzene    | 12.938 | 105  | 49567    | 18.522 | ug/L   | 100      |
| 63) 1,2,4-Trimethylbenzene    | 13.249 | 105  | 74530    | 18.548 | ug/L   | 97       |
| 64) 1,3-Dichlorobenzene       | 13.499 | 146  | 38266    | 17.818 | ug/L   | 95       |
| 65) 1,4-Dichlorobenzene       | 13.579 | 146  | 40198    | 18.121 | ug/L   | 97       |
| 67) 1,2-Dichlorobenzene       | 13.865 | 146  | 38638    | 19.661 | ug/L   | 98       |
| 68) 1,2-Dibromo-3-chloropr... | 14.481 | 75   | 2517     | 16.416 | ug/L   | 83       |
| 69) 1,3,5-Trichlorobenzene    | 14.627 | 180  | 19039    | 13.355 | ug/L   | 97       |
| 70) 1,2,4-trichlorobenzene    | 15.127 | 180  | 11254    | 9.814  | ug/L   | 95       |
| 71) Naphthalene               | 15.365 | 128  | 20107    | 8.067  | ug/L   | 98       |
| 72) 1,2,3-Trichlorobenzene    | 15.554 | 180  | 8097     | 7.967  | ug/L   | 96       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW051922\  
 Data File : VW023179.D  
 Acq On : 19 May 2022 17:45  
 Operator : SY/VA  
 Sample : N2926-02MS  
 Misc : 4.83g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1


Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 EXY11MS

Quant Time: May 20 01:52:29 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM050222SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Fri May 20 01:47:53 2022  
 Response via : Initial Calibration

### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 05/20/2022  
 Supervised By : Mahesh Dadoda 05/26/2022

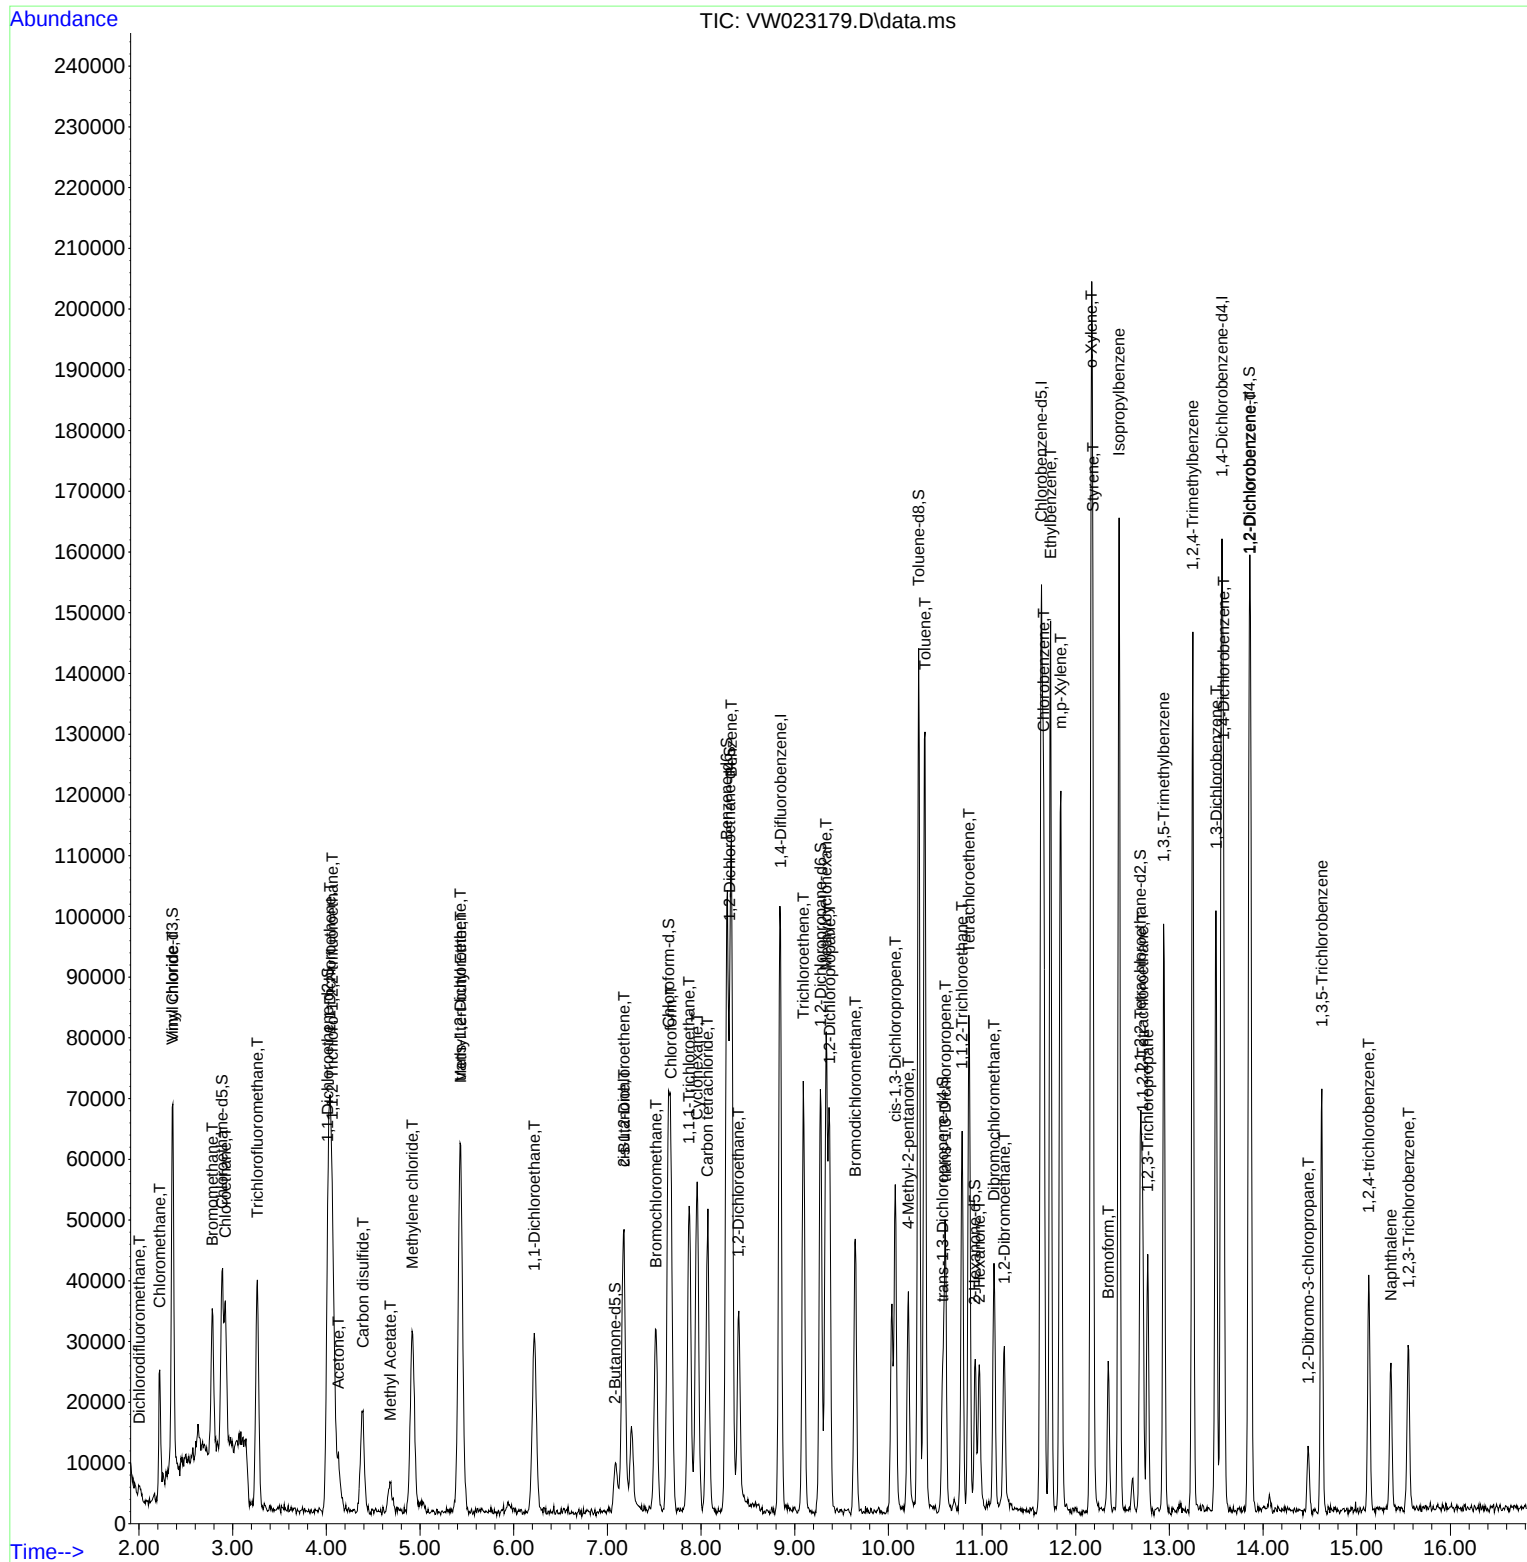



#2  
Dichlorodifluoromethane  
Concen: 3.754 ug/L  
RT: 2.001 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS



Tgt Ion: 85 Resp: 1774  
Ion Ratio Lower Upper  
85 100  
87 29.9 27.8 41.8




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022



#3  
Chloromethane  
Concen: 17.511 ug/L  
RT: 2.221 min Scan# 52  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Tgt Ion: 50 Resp: 15990  
Ion Ratio Lower Upper  
50 100  
52 29.3 23.1 42.9

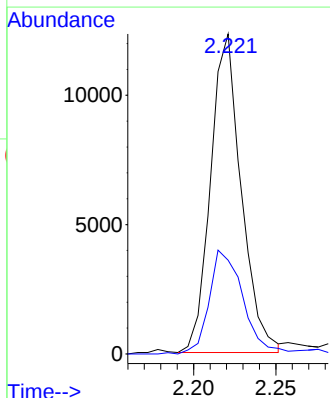







#5  
 Vinyl chloride  
 Concen: 16.764 ug/L  
 RT: 2.361 min Scan# 75  
 Delta R.T. 0.000 min  
 Lab File: VW023179.D  
 Acq: 19 May 2022 17:45

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 EXY11MS

Tgt Ion: 62 Resp: 3072  
 Ion Ratio Lower Upper  
 62 100  
 64 37.8 24.9 46.3




Manual Integrations  
 APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
 Supervised By :Mahesh Dadoda 05/26/2022



#6  
 Bromomethane  
 Concen: 14.409 ug/L  
 RT: 2.782 min Scan# 144  
 Delta R.T. 0.006 min  
 Lab File: VW023179.D  
 Acq: 19 May 2022 17:45


Tgt Ion: 94 Resp: 16954  
 Ion Ratio Lower Upper  
 94 100  
 96 96.1 61.7 114.5

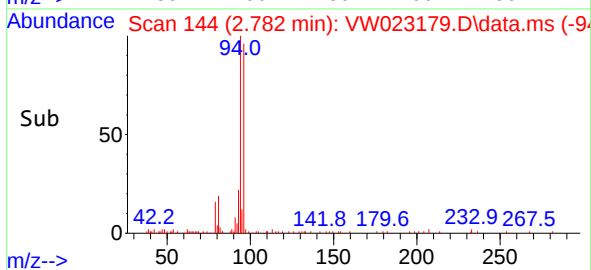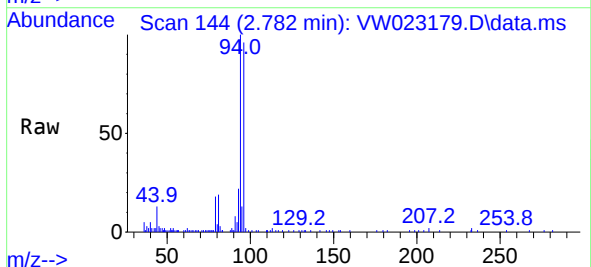



#8  
Chloroethane  
Concen: 24.258 ug/L  
RT: 2.922 min Scan# 167  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS



Tgt Ion: 64 Resp: 2144  
Ion Ratio Lower Upper  
64 100  
66 35.7 23.4 43.6




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

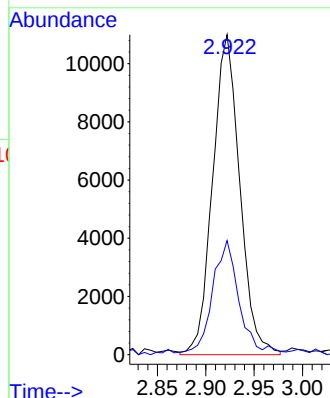

#9  
Trichlorofluoromethane  
Concen: 43.610 ug/L  
RT: 3.263 min Scan# 223  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Tgt Ion:101 Resp: 36528  
Ion Ratio Lower Upper  
101 100  
103 64.7 53.9 80.9

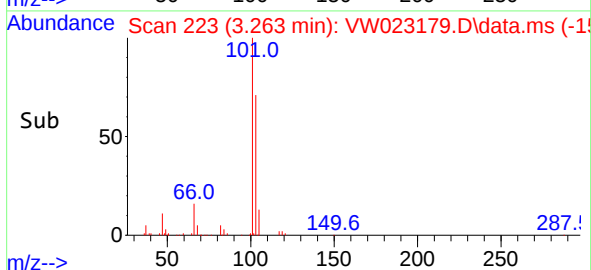







#10  
1,1,2-Trichloro-1,2,2-trifluoroethane  
Concen: 19.381 ug/L  
RT: 4.062 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

Tgt Ion:101 Resp: 2427  
Ion Ratio Lower Upper  
101 100  
85 46.2 34.3 51.5  
151 71.6 54.2 81.2




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

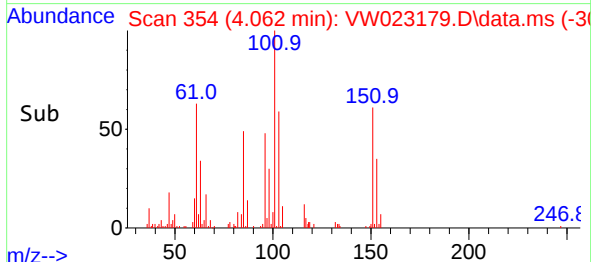

#12  
1,1-Dichloroethene  
Concen: 17.147 ug/L  
RT: 4.038 min Scan# 350  
Delta R.T. -0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Tgt Ion: 96 Resp: 19037  
Ion Ratio Lower Upper  
96 100  
61 155.5 125.7 233.5  
63 145.1 83.4 155.0

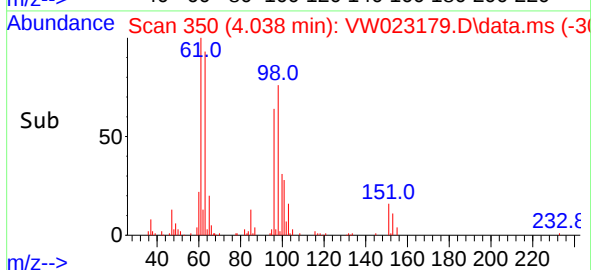







#13  
Acetone  
Concen: 50.141 ug/L  
RT: 4.129 min Scan# 365  
Delta R.T. 0.012 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

Tgt Ion: 43 Resp: 12694  
Ion Ratio Lower Upper  
43 100  
58 21.1 0.0 64.0




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022



#14  
Carbon disulfide  
Concen: 11.395 ug/L  
RT: 4.391 min Scan# 408  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Tgt Ion: 76 Resp: 34683  
Ion Ratio Lower Upper  
76 100  
78 10.3 7.7 11.5

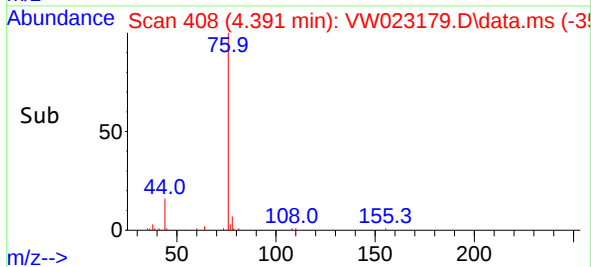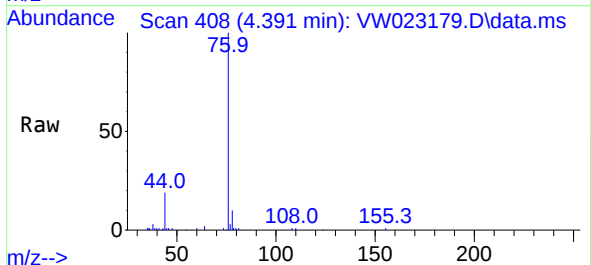







#15  
Methyl Acetate  
Concen: 18.564 ug/L m  
RT: 4.684 min Scan# 453  
Delta R.T. 0.018 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

Tgt Ion: 43 Resp: 944  
Ion Ratio Lower Upper  
43 100  
74 0.6 21.9 32.9




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022



#16  
Methylene chloride  
Concen: 18.212 ug/L  
RT: 4.916 min Scan# 494  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45


Tgt Ion: 84 Resp: 23100  
Ion Ratio Lower Upper  
84 100  
86 60.2 45.4 84.4  
49 105.7 82.5 153.1

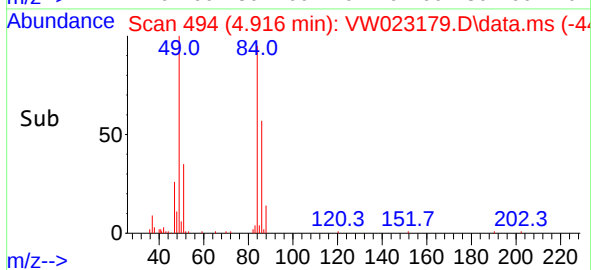



#17  
trans-1,2-Dichloroethene  
Concen: 15.705 ug/L  
RT: 5.428 min Scan# 51  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

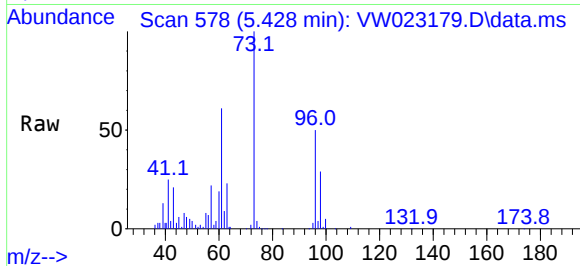


Tgt Ion: 96 Resp: 1962  
Ion Ratio Lower Upper  
96 100  
61 121.9 92.2 171.2  
98 57.7 42.9 79.7

Manual Integrations  
APPROVED



Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022




#18  
Methyl tert-butyl Ether  
Concen: 24.735 ug/L  
RT: 5.434 min Scan# 579  
Delta R.T. 0.012 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

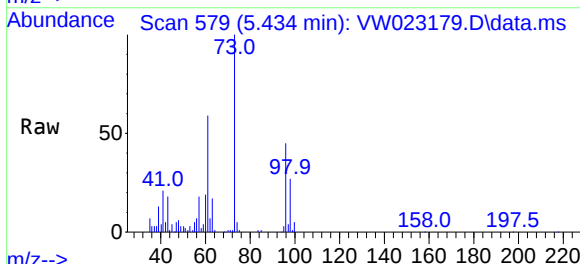

Tgt Ion: 73 Resp: 47176  
Ion Ratio Lower Upper  
73 100  
43 21.3 15.9 23.9  
57 15.8 16.5 24.7#

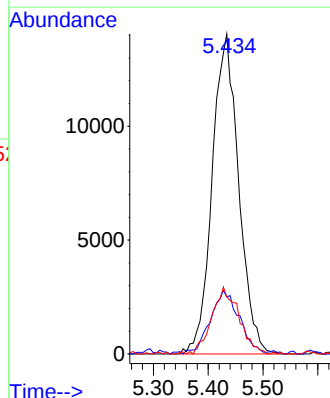



#19

1,1-Dichloroethane

Concen: 18.972 ug/L

RT: 6.220 min Scan# 707

Delta R.T. 0.006 min

Lab File: VW023179.D

Acq: 19 May 2022 17:45

Instrument :

MSVOA\_W

ClientSampleId :





EXY11MS

|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 63    | Resp: | 4017 |
| Ion Ratio | Lower | Upper |      |
| 63        | 100   |       |      |
| 65        | 31.1  | 23.3  | 43.3 |
| 83        | 13.6  | 11.1  | 20.5 |

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

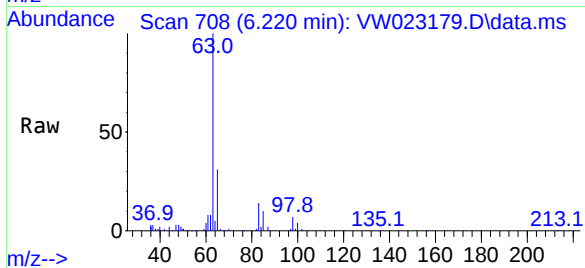

#20

cis-1,2-Dichloroethene

Concen: 16.932 ug/L




RT: 7.177 min Scan# 865


Delta R.T. 0.012 min

Lab File: VW023179.D

Acq: 19 May 2022 17:45


|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 96    | Resp: | 22722 |
| Ion Ratio | Lower | Upper |       |
| 96        | 100   |       |       |
| 61        | 125.1 | 84.2  | 156.4 |
| 68        | 1.2   | 0.1   | 0.1   |

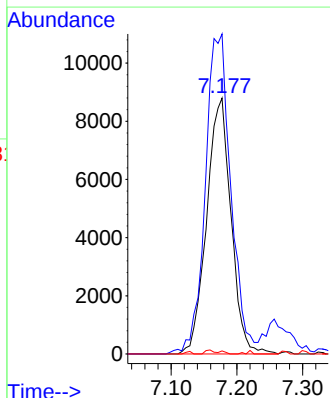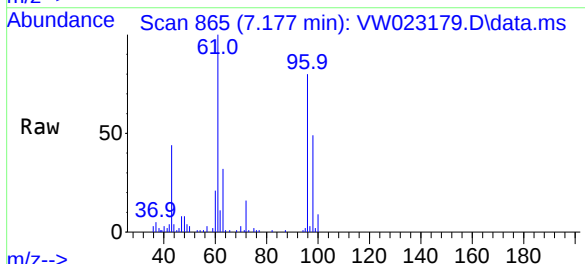



#22  
2-Butanone  
Concen: 33.639 ug/L  
RT: 7.177 min Scan# 864  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS



Tgt Ion: 43 Resp: 11910  
Ion Ratio Lower Upper  
43 100  
72 33.1 15.1 45.3




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022



#23  
Bromochloromethane  
Concen: 17.205 ug/L  
RT: 7.519 min Scan# 921  
Delta R.T. 0.012 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45


Tgt Ion:128 Resp: 10813  
Ion Ratio Lower Upper  
128 100  
49 148.4 110.0 204.4  
130 132.4 94.8 176.0  
51 53.4 40.2 60.2

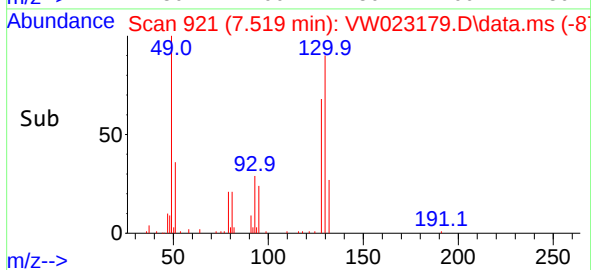



#25  
Chloroform  
Concen: 19.215 ug/L  
RT: 7.677 min Scan# 946  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS




Tgt Ion: 83 Resp: 4499  
Ion Ratio Lower Upper  
83 100  
85 59.0 46.6 86.6

Manual Integrations  
APPROVED



Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022




#27  
1,2-Dichloroethane  
Concen: 18.120 ug/L  
RT: 8.397 min Scan# 1065  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Tgt Ion: 62 Resp: 28282  
Ion Ratio Lower Upper  
62 100  
98 6.9 7.2 10.8#

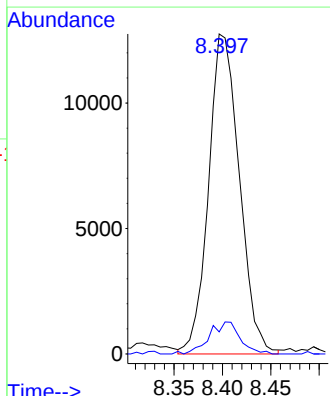



#29  
Cyclohexane  
Concen: 15.941 ug/L  
RT: 7.958 min Scan# 993  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
Client Sample Id :  
EXY11MS






Tgt Ion: 56 Resp: 27049

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 56  | 100   |       |       |
| 69  | 31.6  | 25.6  | 38.4  |
| 84  | 91.4  | 78.2  | 117.4 |

Manual Integrations  
APPROVED




Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

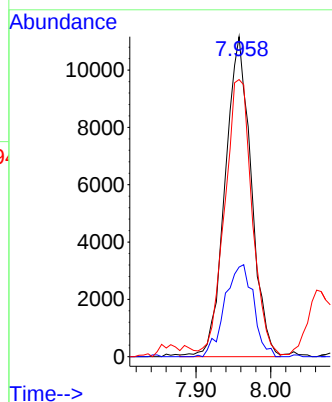


#30  
1,1,1-Trichloroethane  
Concen: 21.611 ug/L  
RT: 7.872 min Scan# 979  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Tgt Ion: 97 Resp: 40069

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 97  | 100   |       |       |
| 99  | 64.0  | 51.0  | 76.4  |
| 61  | 43.0  | 34.8  | 52.2  |

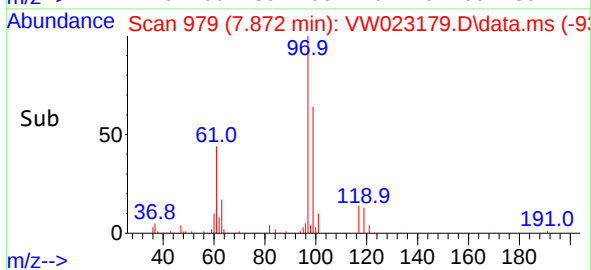







#31  
Carbon tetrachloride  
Concen: 19.861 ug/L  
RT: 8.067 min Scan# 1010  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

Tgt Ion:117 Resp: 3444  
Ion Ratio Lower Upper  
117 100  
119 92.7 76.6 115.0




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

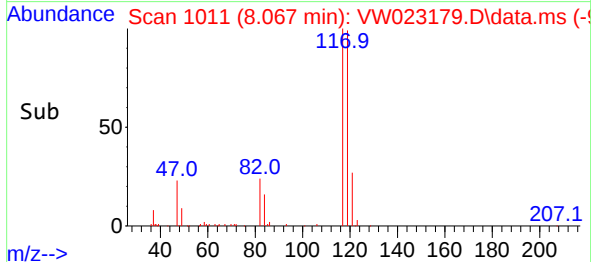

#33  
Benzene  
Concen: 19.569 ug/L  
RT: 8.323 min Scan# 1053  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45


Tgt Ion: 78 Resp: 90449

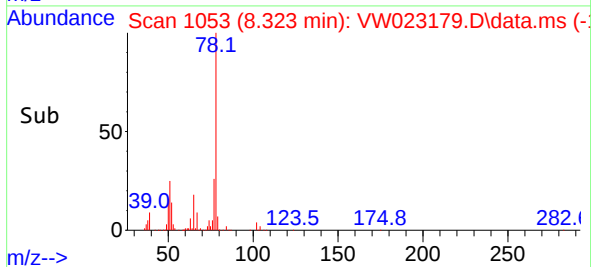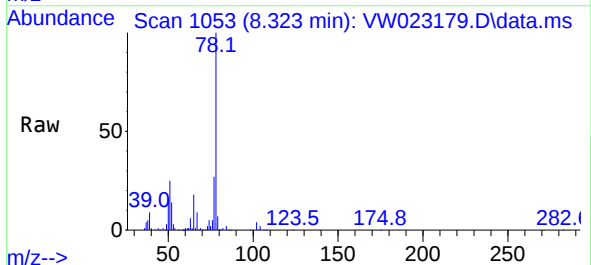

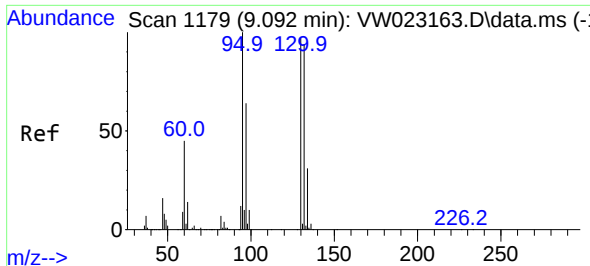

#34  
Trichloroethene  
Concen: 18.655 ug/L  
RT: 9.092 min Scan# 1179  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

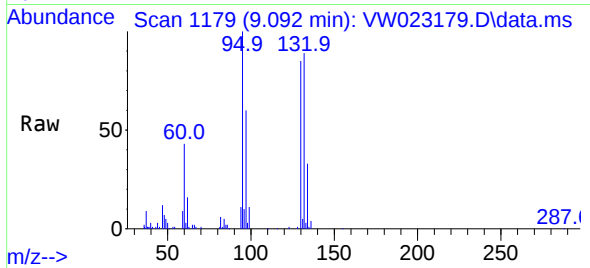

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 95      | 100   |       |       |
| 97      | 60.1  | 46.1  | 85.7  |
| 132     | 88.8  | 66.9  | 124.3 |
| 130     | 85.4  | 69.5  | 129.1 |




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

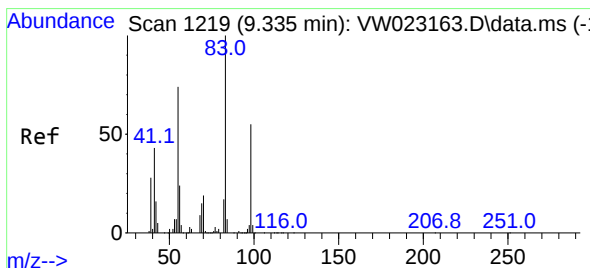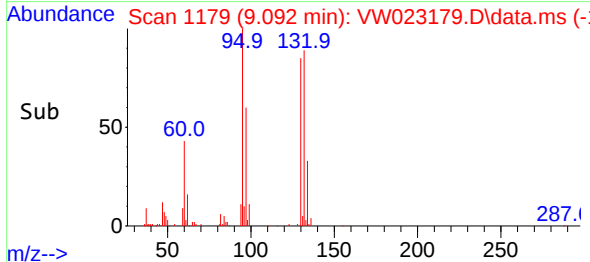

#35  
Methylcyclohexane  
Concen: 14.022 ug/L  
RT: 9.335 min Scan# 1219  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 83      | 100   |       |       |
| 55      | 70.7  | 55.1  | 82.7  |
| 98      | 49.5  | 40.4  | 60.6  |

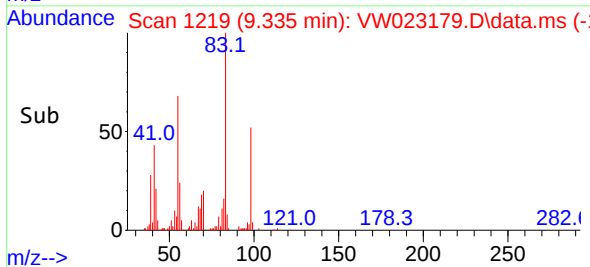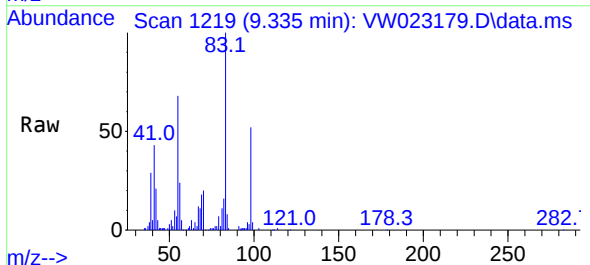

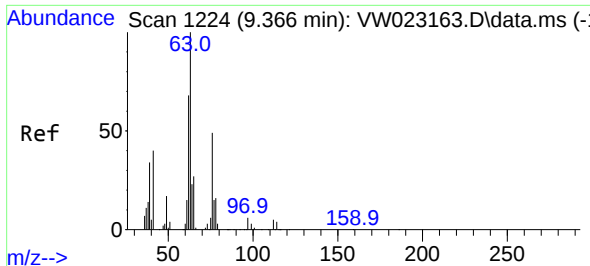

#37

1,2-Dichloropropane

Concen: 19.113 ug/L

RT: 9.372 min Scan# 11

Delta R.T. 0.006 min

Lab File: VW023179.D

Acq: 19 May 2022 17:45

Instrument :

MSVOA\_W

ClientSampleId :

EXY11MS

Tgt Ion: 63 Resp: 21378

Ion Ratio Lower Upper

63 100





112 5.4 3.8 5.8

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022

Supervised By :Mahesh Dadoda 05/26/2022

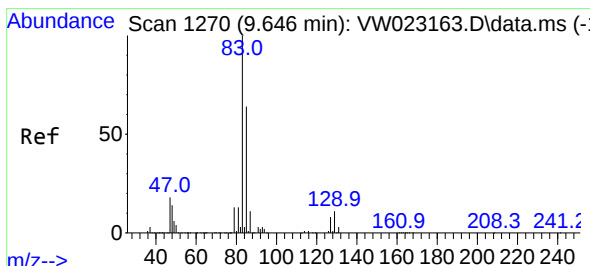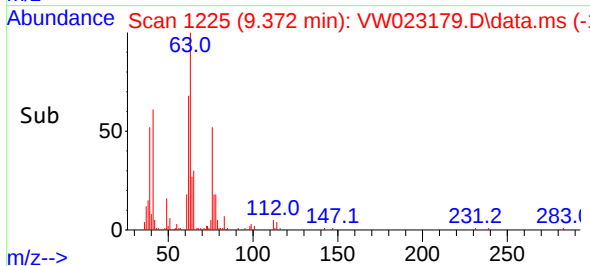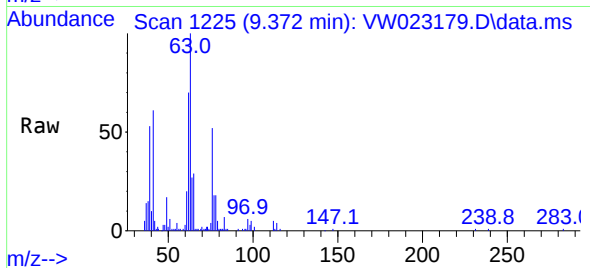

#38

Bromodichloromethane

Concen: 19.148 ug/L

RT: 9.646 min Scan# 1270

Delta R.T. 0.000 min

Lab File: VW023179.D

Acq: 19 May 2022 17:45




Tgt Ion: 83 Resp: 30421


Ion Ratio Lower Upper

83 100

85 62.1 43.5 80.7

127 9.0 7.1 10.7

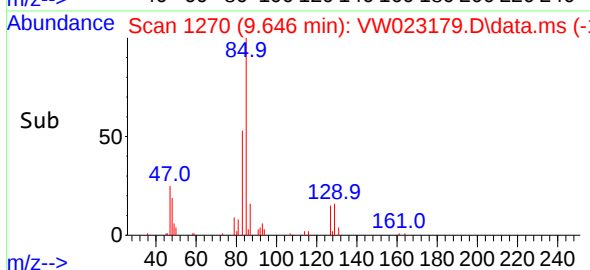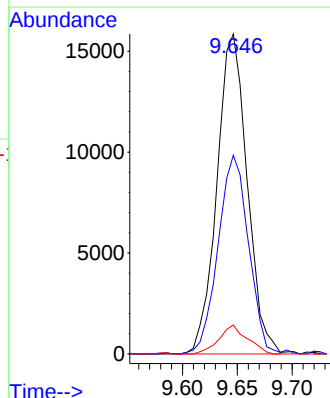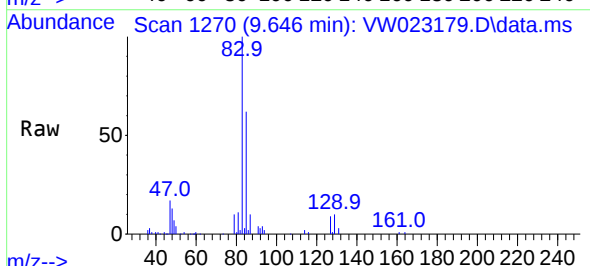







#39  
cis-1,3-Dichloropropene  
Concen: 16.338 ug/L  
RT: 10.073 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

Tgt Ion: 75 Resp: 28336  
Ion Ratio Lower Upper  
75 100  
77 31.9 22.1 41.1




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

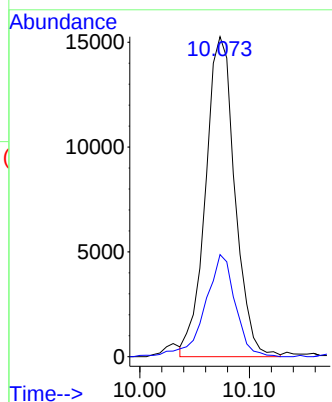

#40  
4-Methyl-2-pentanone  
Concen: 32.109 ug/L  
RT: 10.213 min Scan# 1363  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Tgt Ion: 43 Resp: 22637  
Ion Ratio Lower Upper  
43 100  
58 41.3 31.4 47.2  
100 18.7 14.2 21.4

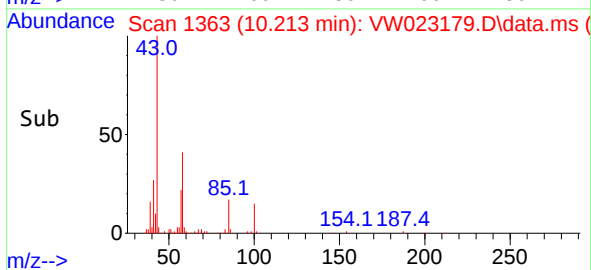







#42  
Toluene  
Concen: 18.589 ug/L  
RT: 10.390 min Scan# 11  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

Tgt Ion: 91 Resp: 9628  
Ion Ratio Lower Upper  
91 100  
92 55.5 41.6 77.2




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022



#44  
trans-1,3-Dichloropropene  
Concen: 15.809 ug/L  
RT: 10.610 min Scan# 1428  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45


Tgt Ion: 75 Resp: 24472  
Ion Ratio Lower Upper  
75 100  
77 31.6 22.0 40.8

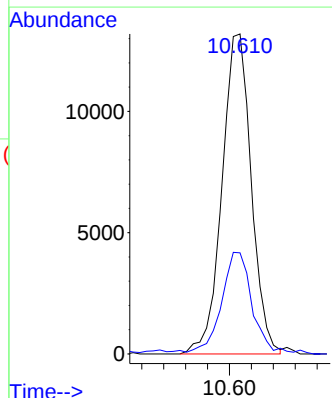

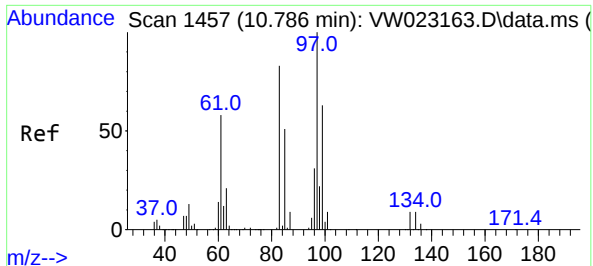

#45  
1,1,2-Trichloroethane  
Concen: 20.337 ug/L  
RT: 10.786 min Scan# 1457  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

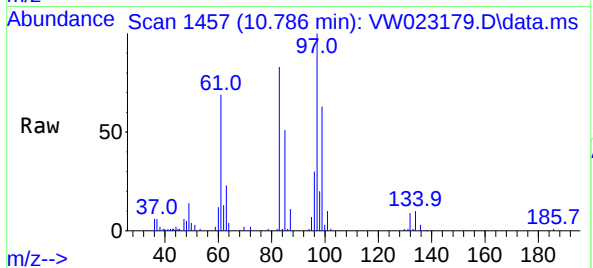


| Tgt Ion: | 97    | Resp: | 19010 |
|----------|-------|-------|-------|
| Ion      | Ratio | Lower | Upper |
| 97       | 100   |       |       |
| 99       | 62.8  | 44.7  | 82.9  |
| 83       | 82.7  | 58.4  | 108.4 |
| 85       | 50.8  | 38.7  | 71.9  |

Manual Integrations  
APPROVED



Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

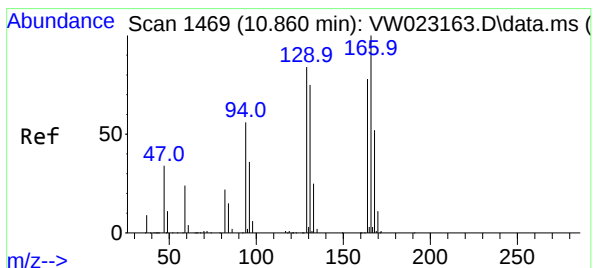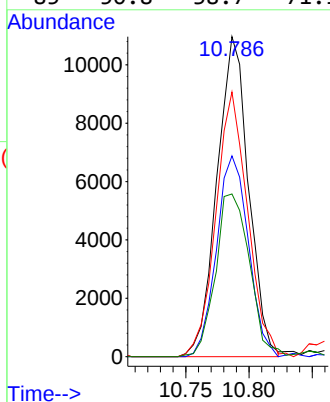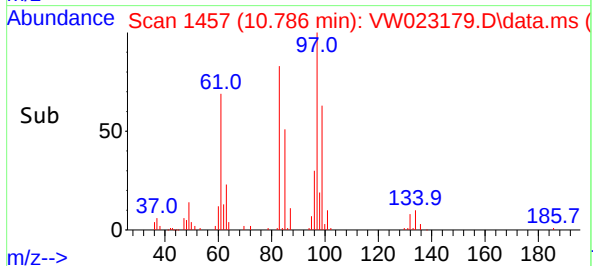


#46  
Tetrachloroethene  
Concen: 18.348 ug/L  
RT: 10.860 min Scan# 1469  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

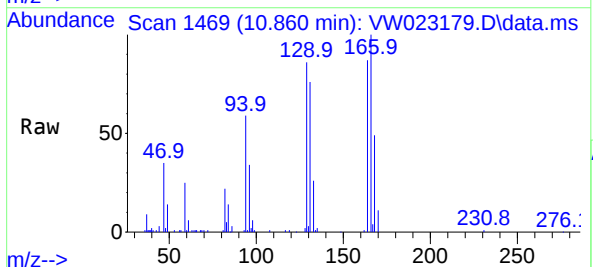


| Tgt Ion: | 164   | Resp: | 17527 |
|----------|-------|-------|-------|
| Ion      | Ratio | Lower | Upper |
| 164      | 100   |       |       |
| 129      | 99.2  | 76.9  | 142.7 |
| 131      | 87.3  | 75.1  | 139.5 |
| 166      | 114.9 | 96.0  | 178.2 |

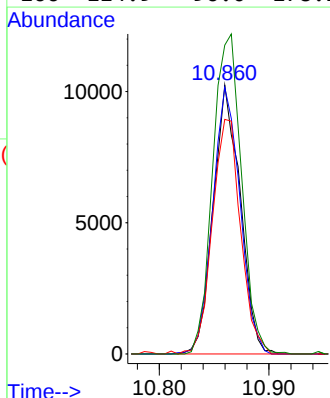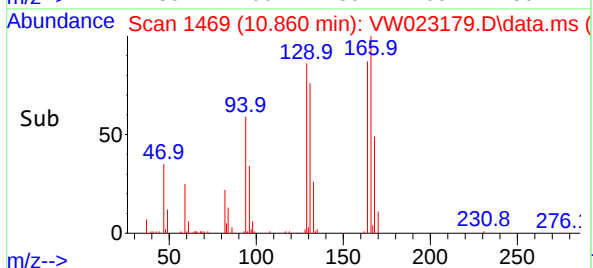

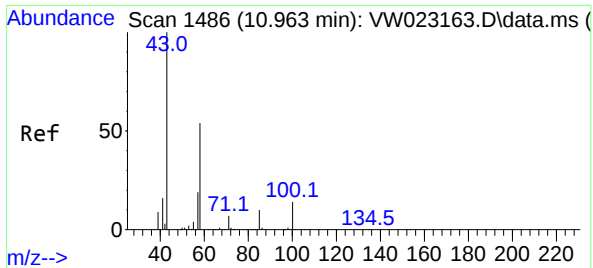

#48  
2-Hexanone  
Concen: 32.402 ug/L  
RT: 10.969 min Scan# 1487  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

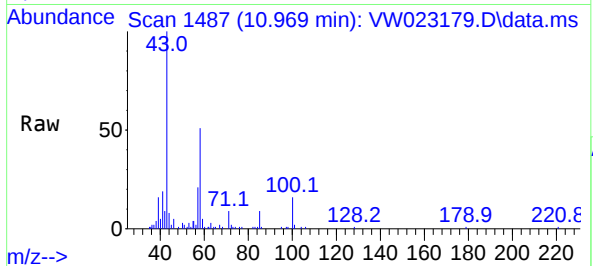


Tgt Ion: 43 Resp: 1526  
Ion Ratio Lower Upper  
43 100  
58 54.9 45.9 68.9  
57 21.0 16.2 24.2  
100 15.1 10.7 16.1

Manual Integrations  
APPROVED



Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

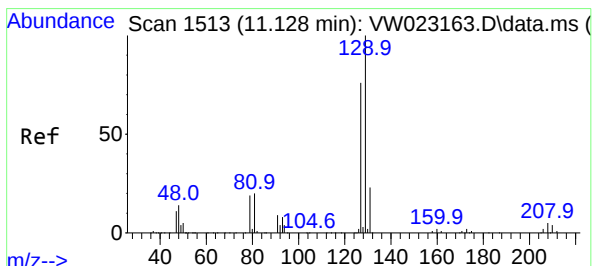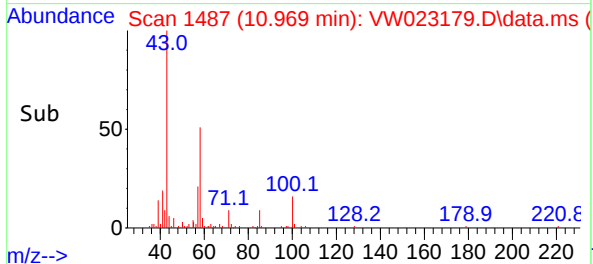


#49  
Dibromochloromethane  
Concen: 18.338 ug/L  
RT: 11.128 min Scan# 1513  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

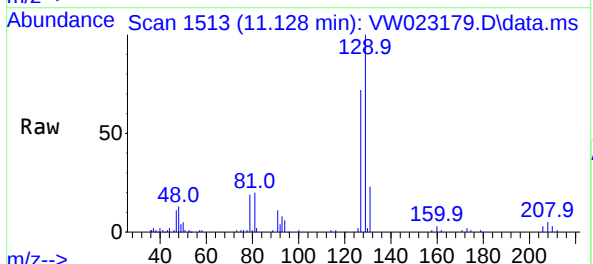

Tgt Ion:129 Resp: 20637  
Ion Ratio Lower Upper  
129 100  
127 71.6 53.8 100.0

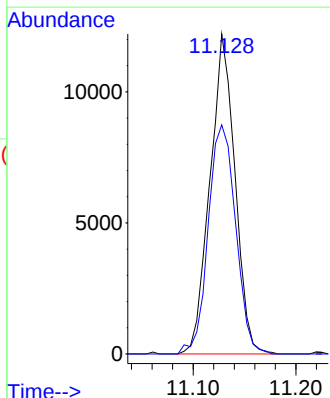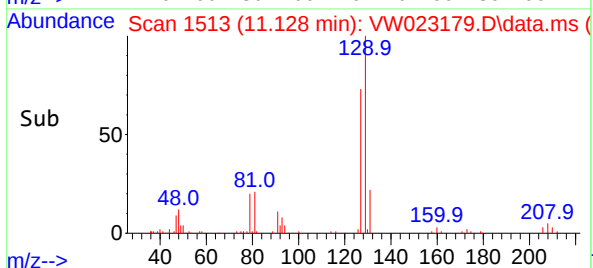







#50  
1,2-Dibromoethane  
Concen: 18.035 ug/L  
RT: 11.238 min Scan# 1531  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

Tgt Ion:107 Resp: 1693  
Ion Ratio Lower Upper  
107 100  
109 95.1 67.5 125.4  
188 3.4 2.9 4.3




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

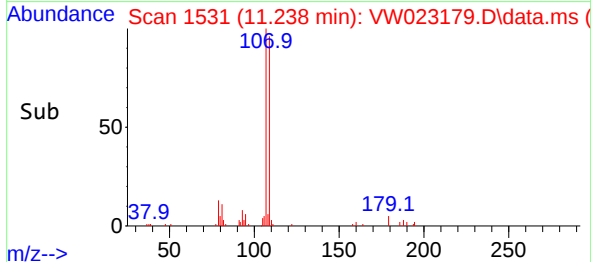

#51  
Chlorobenzene  
Concen: 18.024 ug/L  
RT: 11.658 min Scan# 1600  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Tgt Ion:112 Resp: 61550  
Ion Ratio Lower Upper  
112 100  
114 33.2 22.0 41.0  
77 60.2 42.6 63.8

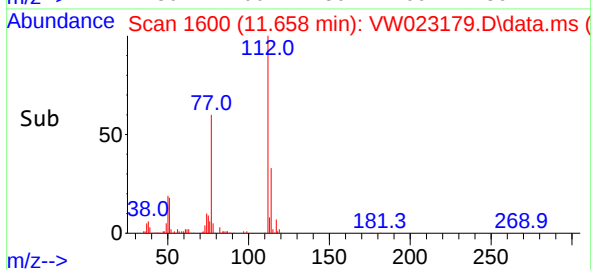



#52

Ethylbenzene

Concen: 17.245 ug/L

RT: 11.731 min Scan# 1

Delta R.T. 0.006 min

Lab File: VW023179.D

Acq: 19 May 2022 17:45

Instrument :

MSVOA\_W

ClientSampleId :

EXY11MS

Tgt Ion: 91 Resp: 9938

Ion Ratio Lower Upper

91 100





106 33.4 22.3 41.3

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022

Supervised By :Mahesh Dadoda 05/26/2022

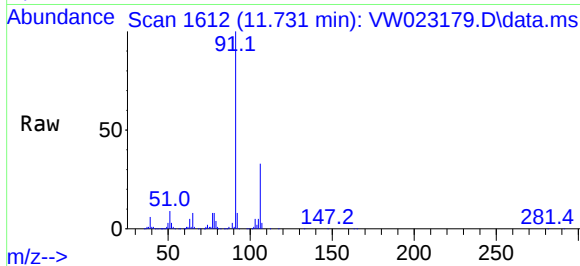

#53

m,p-Xylene

Concen: 17.163 ug/L

RT: 11.841 min Scan# 1630

Delta R.T. 0.006 min

Lab File: VW023179.D




Acq: 19 May 2022 17:45


Tgt Ion:106 Resp: 38971

Ion Ratio Lower Upper

106 100

91 196.6 136.8 254.0

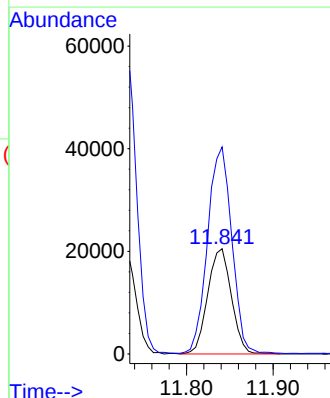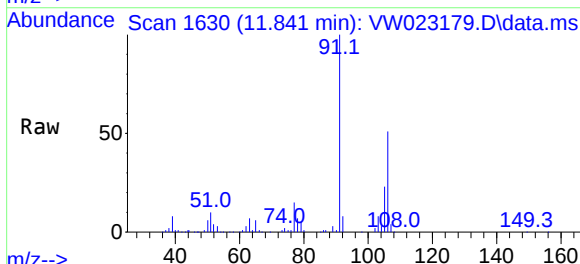







#54  
o-Xylene  
Concen: 17.531 ug/L  
RT: 12.164 min Scan# 1683  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

Tgt Ion:106 Resp: 38200  
Ion Ratio Lower Upper  
106 100  
91 215.6 147.2 273.4




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022



#55  
Styrene  
Concen: 16.845 ug/L  
RT: 12.183 min Scan# 1686  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Tgt Ion:104 Resp: 62370  
Ion Ratio Lower Upper  
104 100  
78 42.9 32.3 59.9

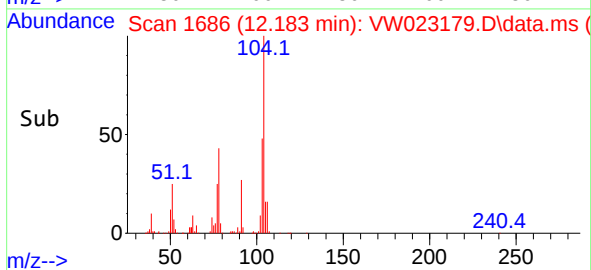

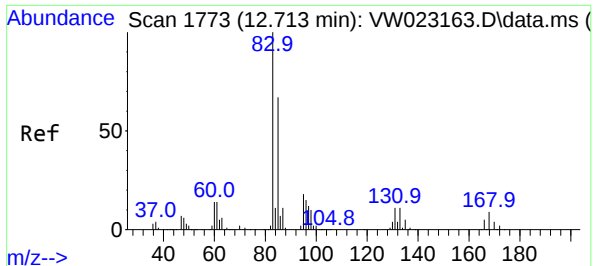





#57  
1,1,2,2-Tetrachloroethane  
Concen: 18.685 ug/L  
RT: 12.713 min Scan# 1773  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 83    | Resp: | 2182 |
| Ion Ratio | Lower | Upper |      |
| 83        | 100   |       |      |
| 85        | 69.0  | 47.5  | 88.1 |
| 131       | 11.6  | 8.7   | 13.1 |




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

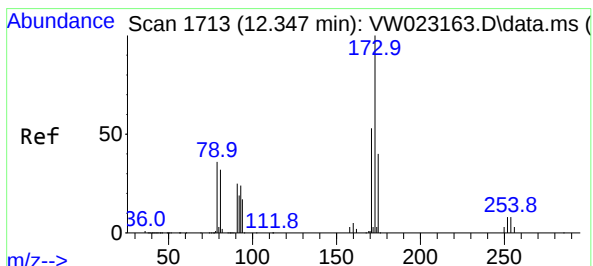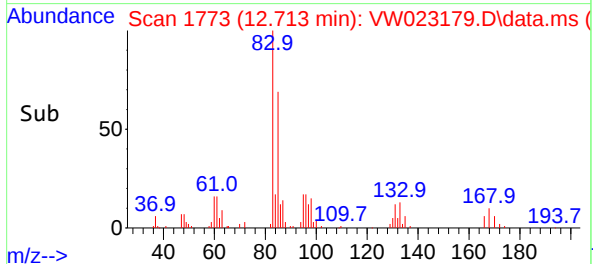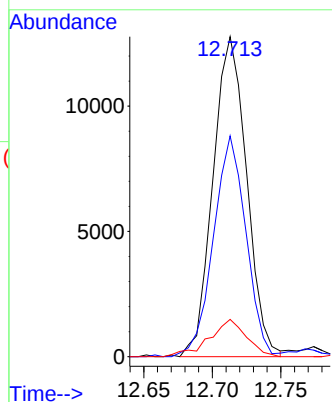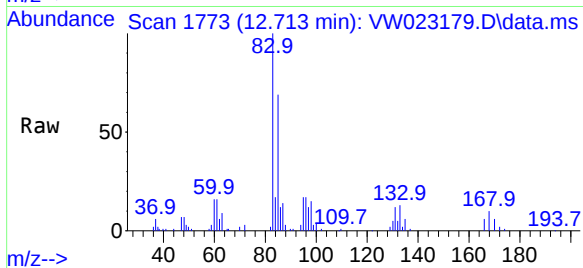

#59  
Bromoform  
Concen: 18.414 ug/L  
RT: 12.347 min Scan# 1713  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45


|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 173   | Resp: | 9163 |
| Ion Ratio | Lower | Upper |      |
| 173       | 100   |       |      |
| 175       | 53.9  | 38.1  | 57.1 |
| 254       | 8.0   | 6.5   | 9.7  |

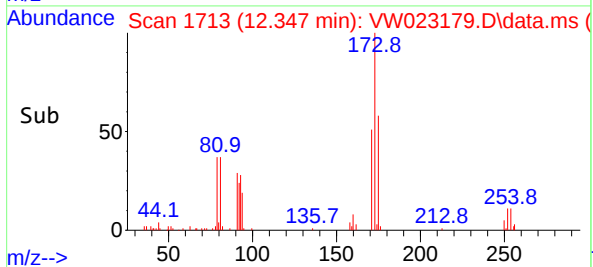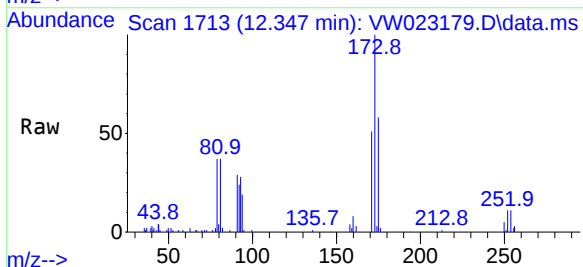



#60  
Isopropylbenzene  
Concen: 21.558 ug/L  
RT: 12.463 min Scan# 1732  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS




Tgt Ion: 105 Resp: 103698  
Ion Ratio Lower Upper  
105 100  
120 26.3 21.3 31.9  
77 15.7 12.6 19.0

Manual Integrations  
APPROVED



Reviewed By : Semsettin Yesilyurt 05/20/2022  
Supervised By : Mahesh Dadoda 05/26/2022




#61  
1,2,3-Trichloropropane  
Concen: 22.722 ug/L  
RT: 12.768 min Scan# 1782  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Tgt Ion: 75 Resp: 15941  
Ion Ratio Lower Upper  
75 100  
77 33.8 26.2 39.2  
110 41.4 34.1 51.1

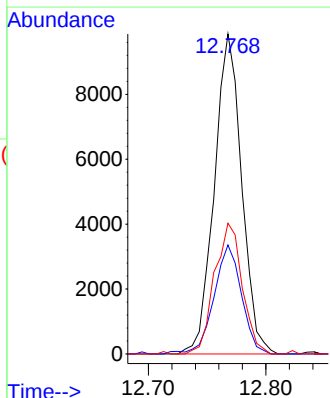



#62  
1,3,5-Trimethylbenzene  
Concen: 18.522 ug/L  
RT: 12.938 min Scan# 1810  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS




Tgt Ion:105 Resp: 4956  
Ion Ratio Lower Upper  
105 100  
120 48.8 38.9 58.3

Manual Integrations  
APPROVED



Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022




#63  
1,2,4-Trimethylbenzene  
Concen: 18.548 ug/L  
RT: 13.249 min Scan# 1861  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45



Tgt Ion:105 Resp: 74530  
Ion Ratio Lower Upper  
105 100  
120 45.0 37.4 56.2

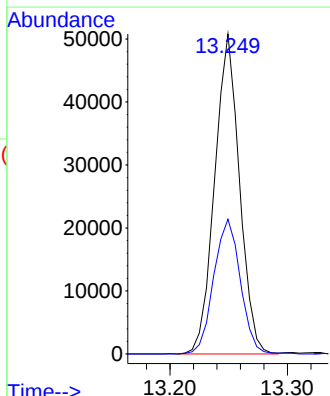

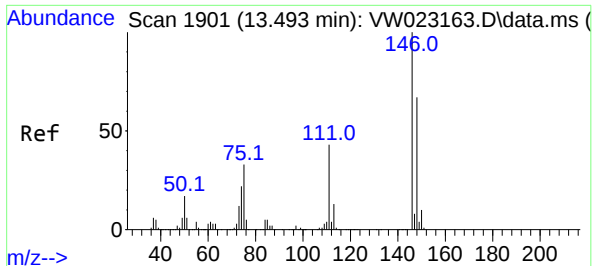





#64  
1,3-Dichlorobenzene  
Concen: 17.818 ug/L  
RT: 13.499 min Scan# 1901  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS

Tgt Ion:146 Resp: 38260  
Ion Ratio Lower Upper  
146 100  
111 46.3 29.5 54.9  
148 66.5 48.6 90.2




Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

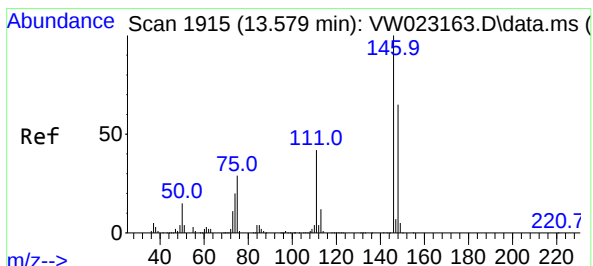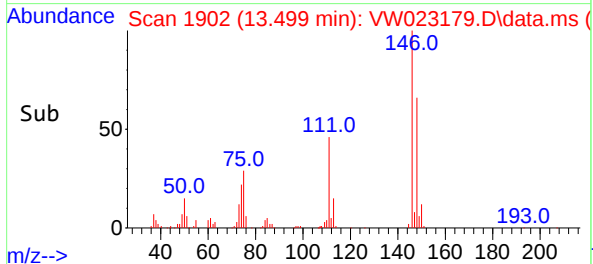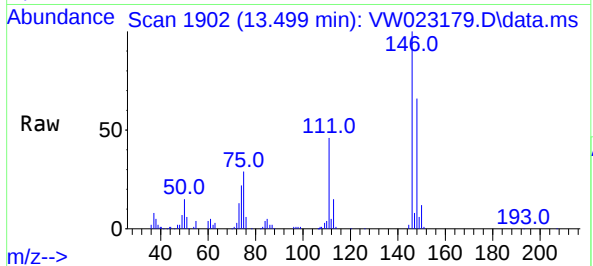

#65  
1,4-Dichlorobenzene  
Concen: 18.121 ug/L  
RT: 13.579 min Scan# 1915  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45


Tgt Ion:146 Resp: 40198  
Ion Ratio Lower Upper  
146 100  
111 38.1 27.2 50.4  
148 66.0 44.0 81.6

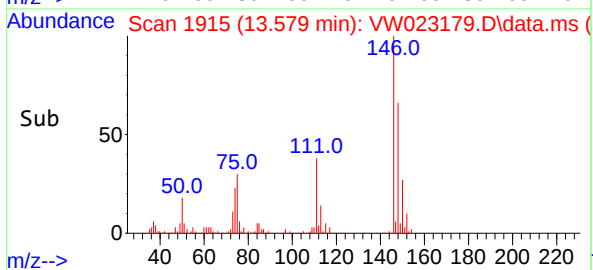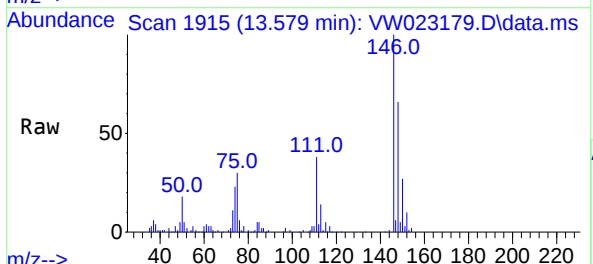



#67  
1,2-Dichlorobenzene  
Concen: 19.661 ug/L  
RT: 13.865 min Scan# 1962  
Delta R.T. 0.000 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS




Tgt Ion:146 Resp: 38638  
Ion Ratio Lower Upper  
146 100  
111 42.8 35.7 53.5  
148 66.7 52.6 79.0

Manual Integrations  
APPROVED



Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022

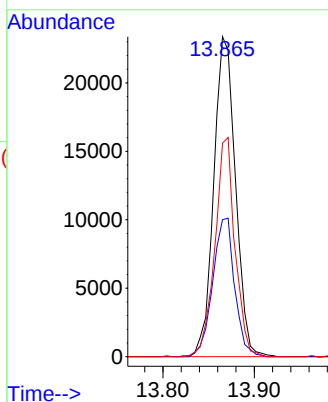


#68  
1,2-Dibromo-3-chloropropane  
Concen: 16.416 ug/L  
RT: 14.481 min Scan# 2063  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45

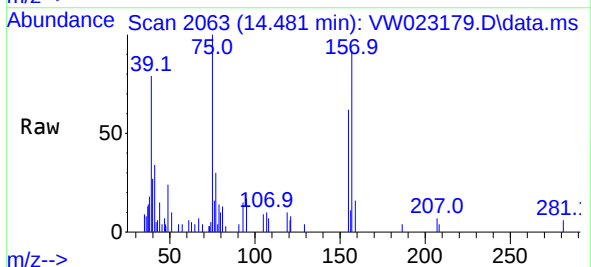

Tgt Ion: 75 Resp: 2517  
Ion Ratio Lower Upper  
75 100  
155 61.5 59.3 88.9  
157 91.8 89.8 134.8

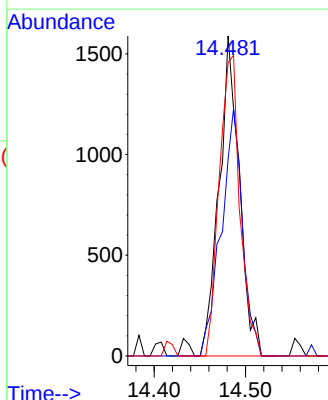



#69

1,3,5-Trichlorobenzene

Concen: 13.355 ug/L

RT: 14.627 min Scan# 2087

Delta R.T. 0.000 min

Lab File: VW023179.D

Acq: 19 May 2022 17:45

Instrument :

MSVOA\_W

ClientSampleId :

EXY11MS

Tgt Ion:180 Resp: 19039

Ion Ratio Lower Upper

180 100

182 95.8 74.8 112.2

184 31.8 23.4 35.2





145 34.8 26.5 39.7

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022

Supervised By :Mahesh Dadoda 05/26/2022

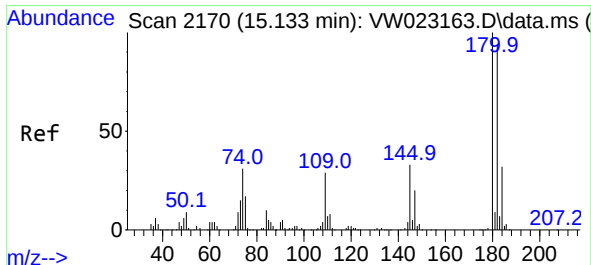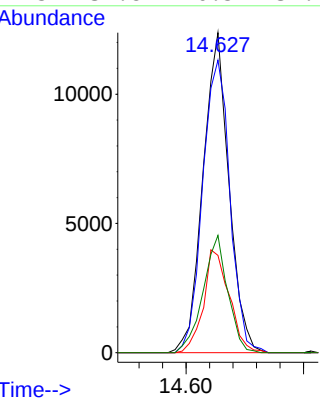

#70

1,2,4-trichlorobenzene

Concen: 9.814 ug/L

RT: 15.127 min Scan# 2169

Delta R.T. -0.006 min

Lab File: VW023179.D

Acq: 19 May 2022 17:45




Tgt Ion:180 Resp: 11254


Ion Ratio Lower Upper

180 100

182 88.1 74.9 112.3


145 34.8 26.6 39.8

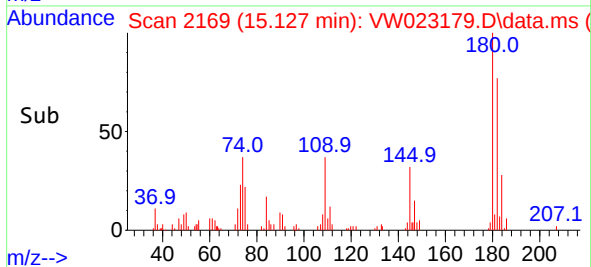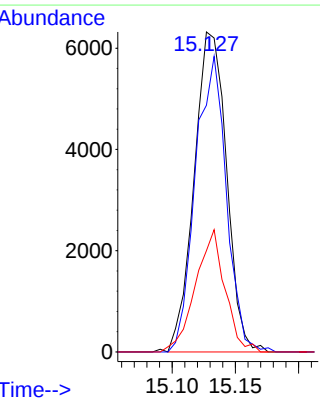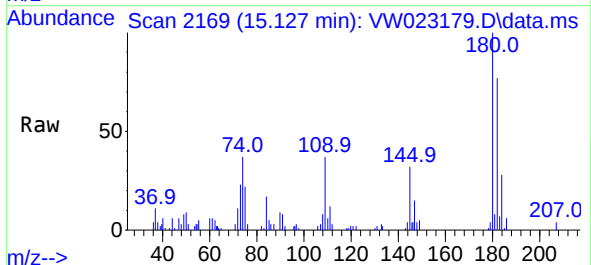



#71  
Naphthalene  
Concen: 8.067 ug/L  
RT: 15.365 min Scan# 2107  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45




Instrument :  
MSVOA\_W  
ClientSampleId :  
EXY11MS




| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 128     | 100   |       |       |
| 127     | 14.2  | 10.6  | 16.0  |
| 129     | 11.8  | 8.7   | 13.1  |

Manual Integrations  
APPROVED

Reviewed By :Semsettin Yesilyurt 05/20/2022  
Supervised By :Mahesh Dadoda 05/26/2022



#72  
1,2,3-Trichlorobenzene  
Concen: 7.967 ug/L  
RT: 15.554 min Scan# 2239  
Delta R.T. 0.006 min  
Lab File: VW023179.D  
Acq: 19 May 2022 17:45



| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 180     | 100   |       |       |
| 182     | 87.2  | 73.5  | 110.3 |
| 145     | 35.6  | 27.9  | 41.9  |

