




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051923\
 Data File : VW026001.D
 Acq On : 19 May 2023 13:24
 Operator : SY/MD
 Sample : 02859-02
 Misc : 6.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11G0

Manual IntegrationsAPPROVED

Quant Time: May 20 05:07:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 20 04:57:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/22/2023
 Supervised By :Mahesh Dadoda 05/22/2023

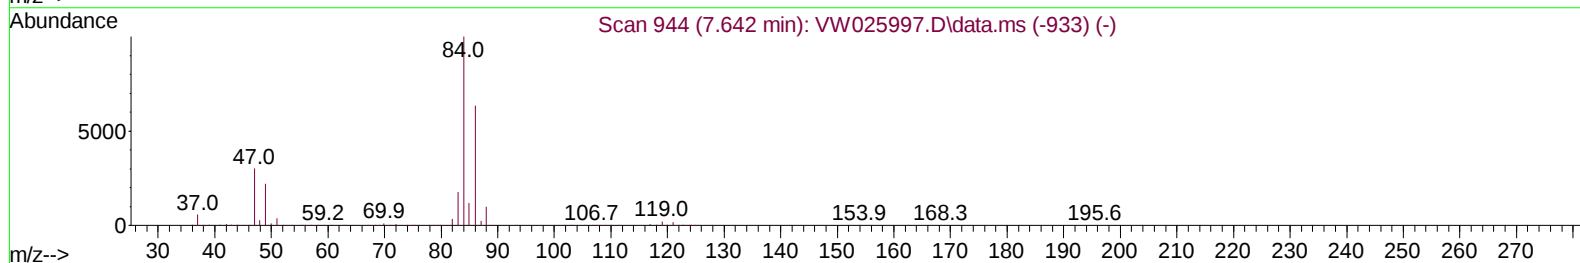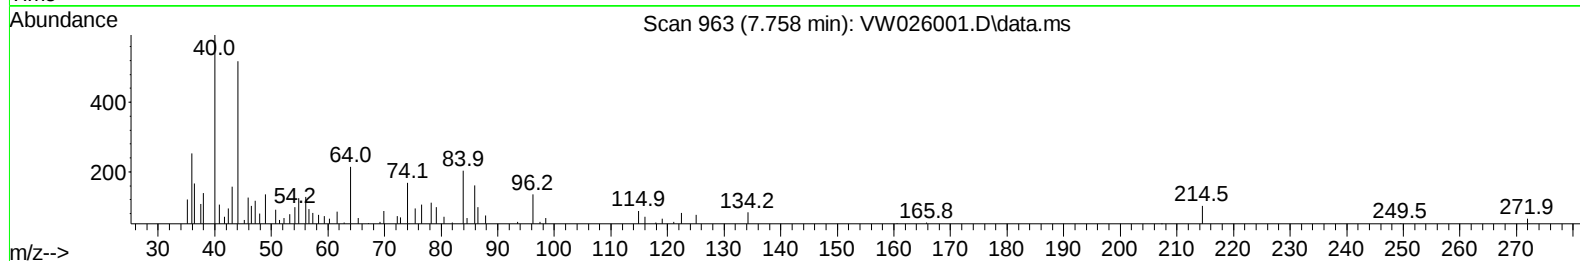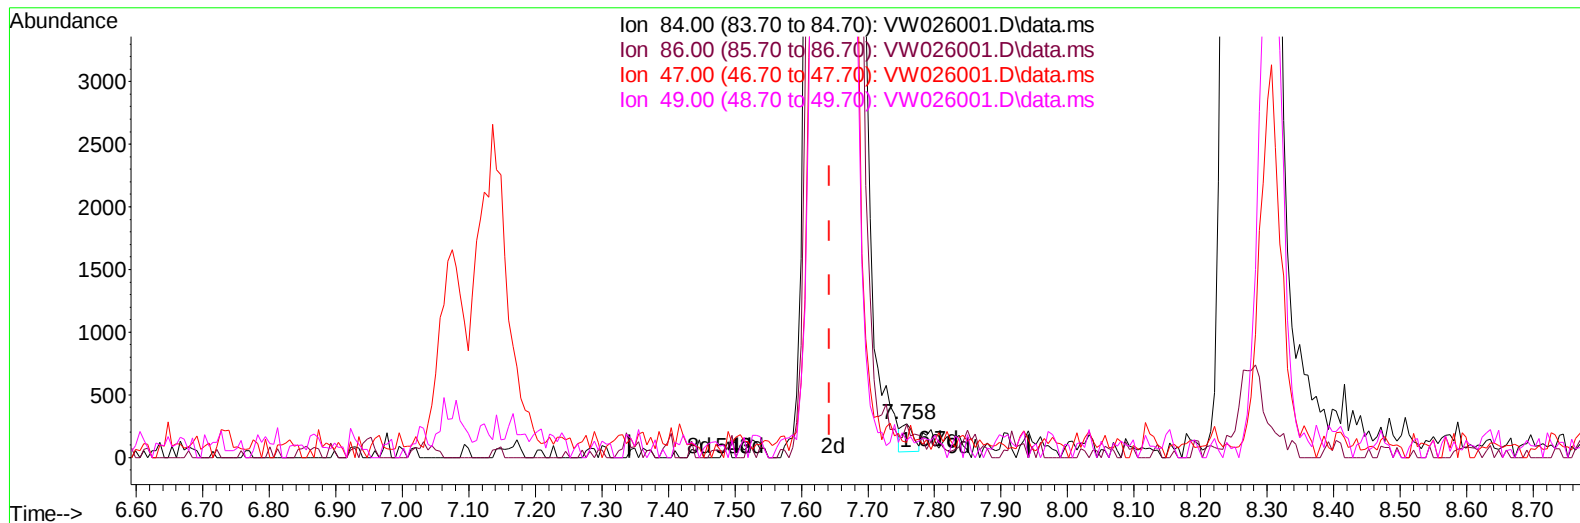

TIC: VW026001.D\data.ms

(24) Chloroform-d (S)

7.758min (+ 0.115) 0.01 ug/L

response 275

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.70	57.82
47.00	50.20	49.09
49.00	28.70	30.55




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051923\
 Data File : VW026001.D
 Acq On : 19 May 2023 13:24
 Operator : SY/MD
 Sample : 02859-02
 Misc : 6.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11G0

Manual IntegrationsAPPROVED

Quant Time: May 20 05:07:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 20 04:57:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/22/2023
 Supervised By :Mahesh Dadoda 05/22/2023

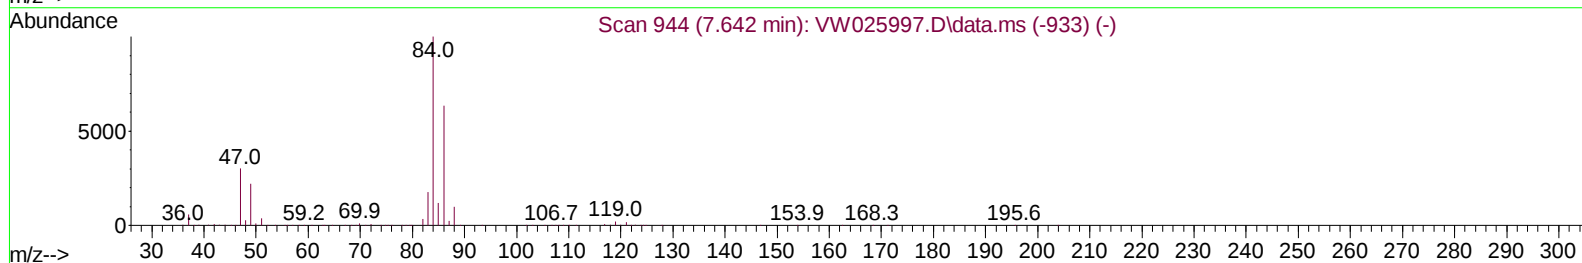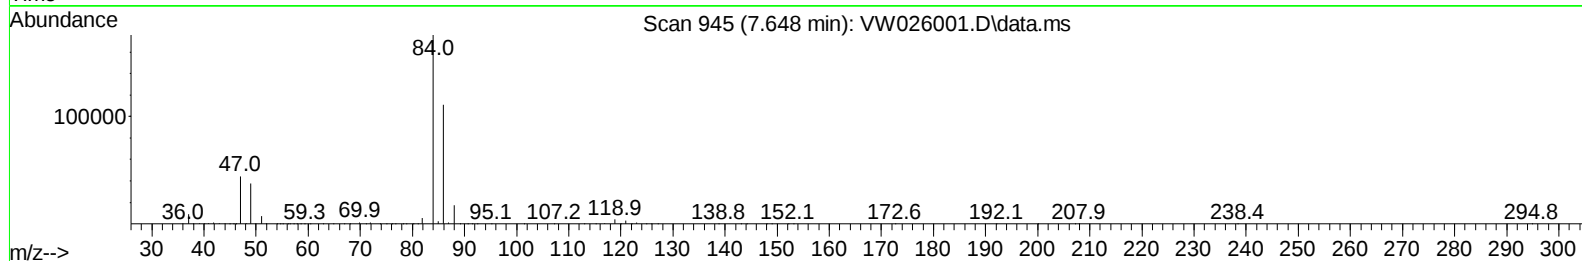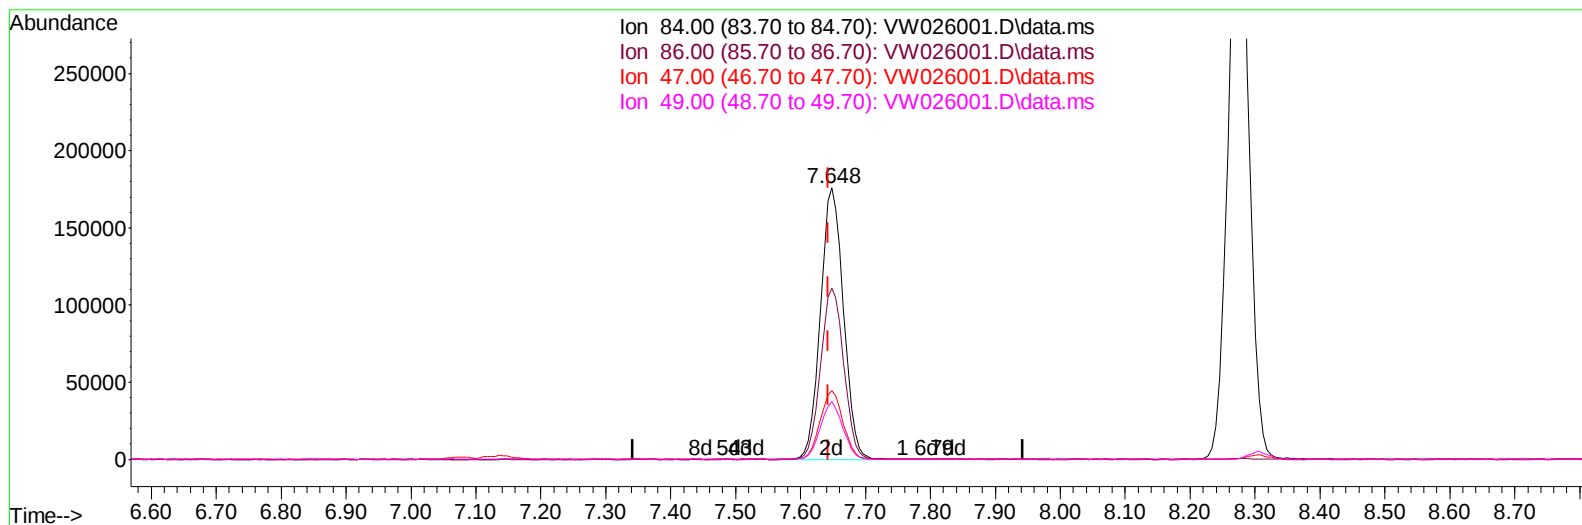

TIC: VW026001.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.006) 22.00 ug/L m

response 434886

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.70	0.04#
47.00	50.20	0.03#
49.00	28.70	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051923\
 Data File : VW026001.D
 Acq On : 19 May 2023 13:24
 Operator : SY/MD
 Sample : 02859-02
 Misc : 6.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11G0

Manual IntegrationsAPPROVED

Quant Time: May 20 05:07:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 20 04:57:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/22/2023
 Supervised By :Mahesh Dadoda 05/22/2023

Compound	R.T.	Q Ion	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	685615	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	642492	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	284158	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	189034	19.457	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.840%	
7) Chloroethane-d5	2.899	69	159867	22.195	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	88.760%	
11) 1,1-Dichloroethene-d2	4.021	65	93860	19.293	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	77.160%	
21) 2-Butanone-d5	7.075	46	163646	50.950	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	101.900%	
24) Chloroform-d	7.648	84	434886m	21.997	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.000%	
26) 1,2-Dichloroethane-d4	8.306	65	253809	22.703	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.800%	
32) Benzene-d6	8.276	84	855670	20.382	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	81.520%	
36) 1,2-Dichloropropane-d6	9.276	67	291533	21.704	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	86.800%	
41) Toluene-d8	10.324	98	727590	19.436	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	77.760%	
43) trans-1,3-Dichloroprop...	10.574	79	107840	19.806	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	79.240%	
47) 2-Hexanone-d5	10.922	63	108955	47.569	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	95.140%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	247817	24.206	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	96.840%	
66) 1,2-Dichlorobenzene-d4	13.848	152	253049	24.429	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.720%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051923\
Data File : VW026001.D
Acq On : 19 May 2023 13:24
Operator : SY/MD
Sample : 02859-02
Misc : 6.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C11G0

Manual IntegrationsAPPROVED

Quant Time: May 20 05:07:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 20 04:57:36 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/22/2023
Supervised By :Mahesh Dadoda 05/22/2023

