

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023188.D
 Acq On : 20 May 2022 10:56
 Operator : SY/VA
 Sample : N2848-05
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: May 20 23:02:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	348053	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	338010	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	170869	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	151612	21.232	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.920%
7) Chloroethane-d5	2.885	69	92133	19.832	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.320%
11) 1,1-Dichloroethene-d2	4.013	63	165678	17.956	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.840%
21) 2-Butanone-d5	7.074	46	60535	44.587	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.180%
24) Chloroform-d	7.647	84	249033	24.422	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.680%
26) 1,2-Dichloroethane-d4	8.488	65	96	0.017	ug/L	0.18
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.275	84	504184	25.879	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.520%
36) 1,2-Dichloropropane-d6	9.275	67	143849	26.285	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.120%
41) Toluene-d8	10.323	98	484419	25.739	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.960%
43) trans-1,3-Dichloroprop...	10.579	79	57856	22.960	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.840%
47) 2-Hexanone-d5	10.921	63	47403	45.373	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.740%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	120330	23.590	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	161355	27.014	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.040%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.031	75	4983	0.667	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023188.D
Acq On : 20 May 2022 10:56
Operator : SY/VA
Sample : N2848-05
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: May 20 23:02:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 20 23:01:40 2022
Response via : Initial Calibration

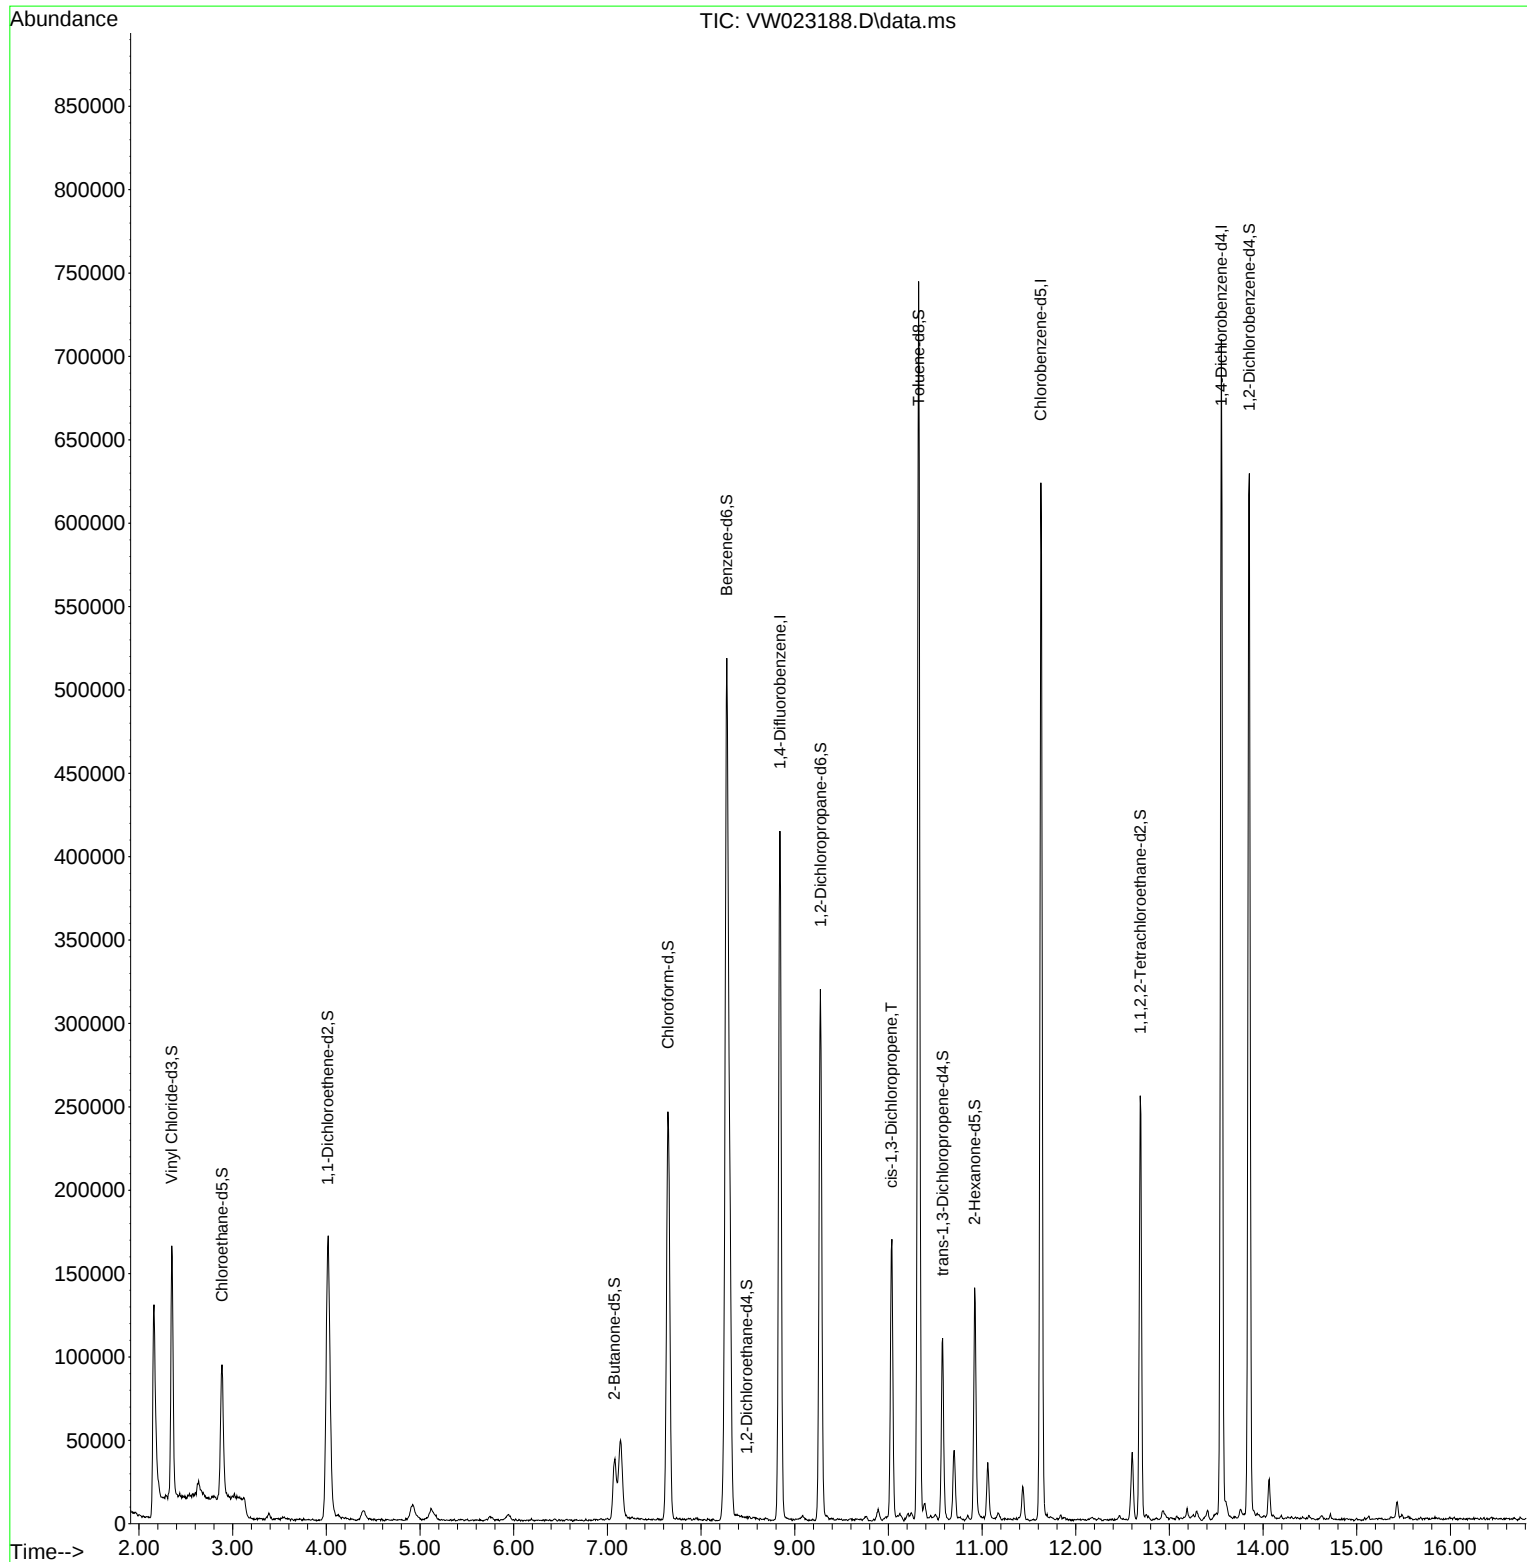

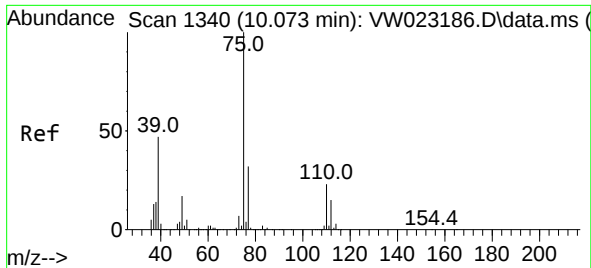

#39

cis-1,3-Dichloropropene

Concen: 0.667 ug/L

RT: 10.031 min Scan# 11

Delta R.T. -0.043 min

Lab File: VW023188.D


Acq: 20 May 2022 10:56

Instrument :

MSVOA_W

ClientSampleId :

VHBLK001

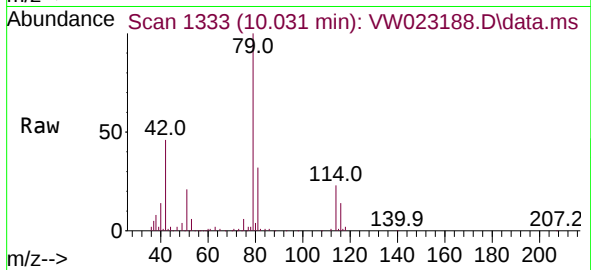

Tgt Ion: 75 Resp: 4983

Ion Ratio Lower Upper

75 100

77 40.9 22.1 41.1

