

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023209.D
 Acq On : 20 May 2022 19:23
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK470

Quant Time: May 20 23:06:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	287264	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	287282	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	142529	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	132239	22.438	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.760%
7) Chloroethane-d5	2.885	69	83952	21.895	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.600%
11) 1,1-Dichloroethene-d2	4.013	63	125880	16.530	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.120%
21) 2-Butanone-d5	7.074	46	56878	50.758	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.520%
24) Chloroform-d	7.647	84	212275	25.222	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.880%
26) 1,2-Dichloroethane-d4	8.305	65	122965	26.639	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.560%
32) Benzene-d6	8.275	84	417111	25.190	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.760%
36) 1,2-Dichloropropane-d6	9.275	67	122173	26.266	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.080%
41) Toluene-d8	10.323	98	397384	24.843	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.360%
43) trans-1,3-Dichloroprop...	10.579	79	50588	23.621	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.480%
47) 2-Hexanone-d5	10.921	63	44162	49.735	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.480%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	107406	24.774	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.080%
66) 1,2-Dichlorobenzene-d4	13.853	152	137383	27.574	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.280%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4434	0.698	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023209.D
Acq On : 20 May 2022 19:23
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK470

Quant Time: May 20 23:06:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 20 23:01:40 2022
Response via : Initial Calibration

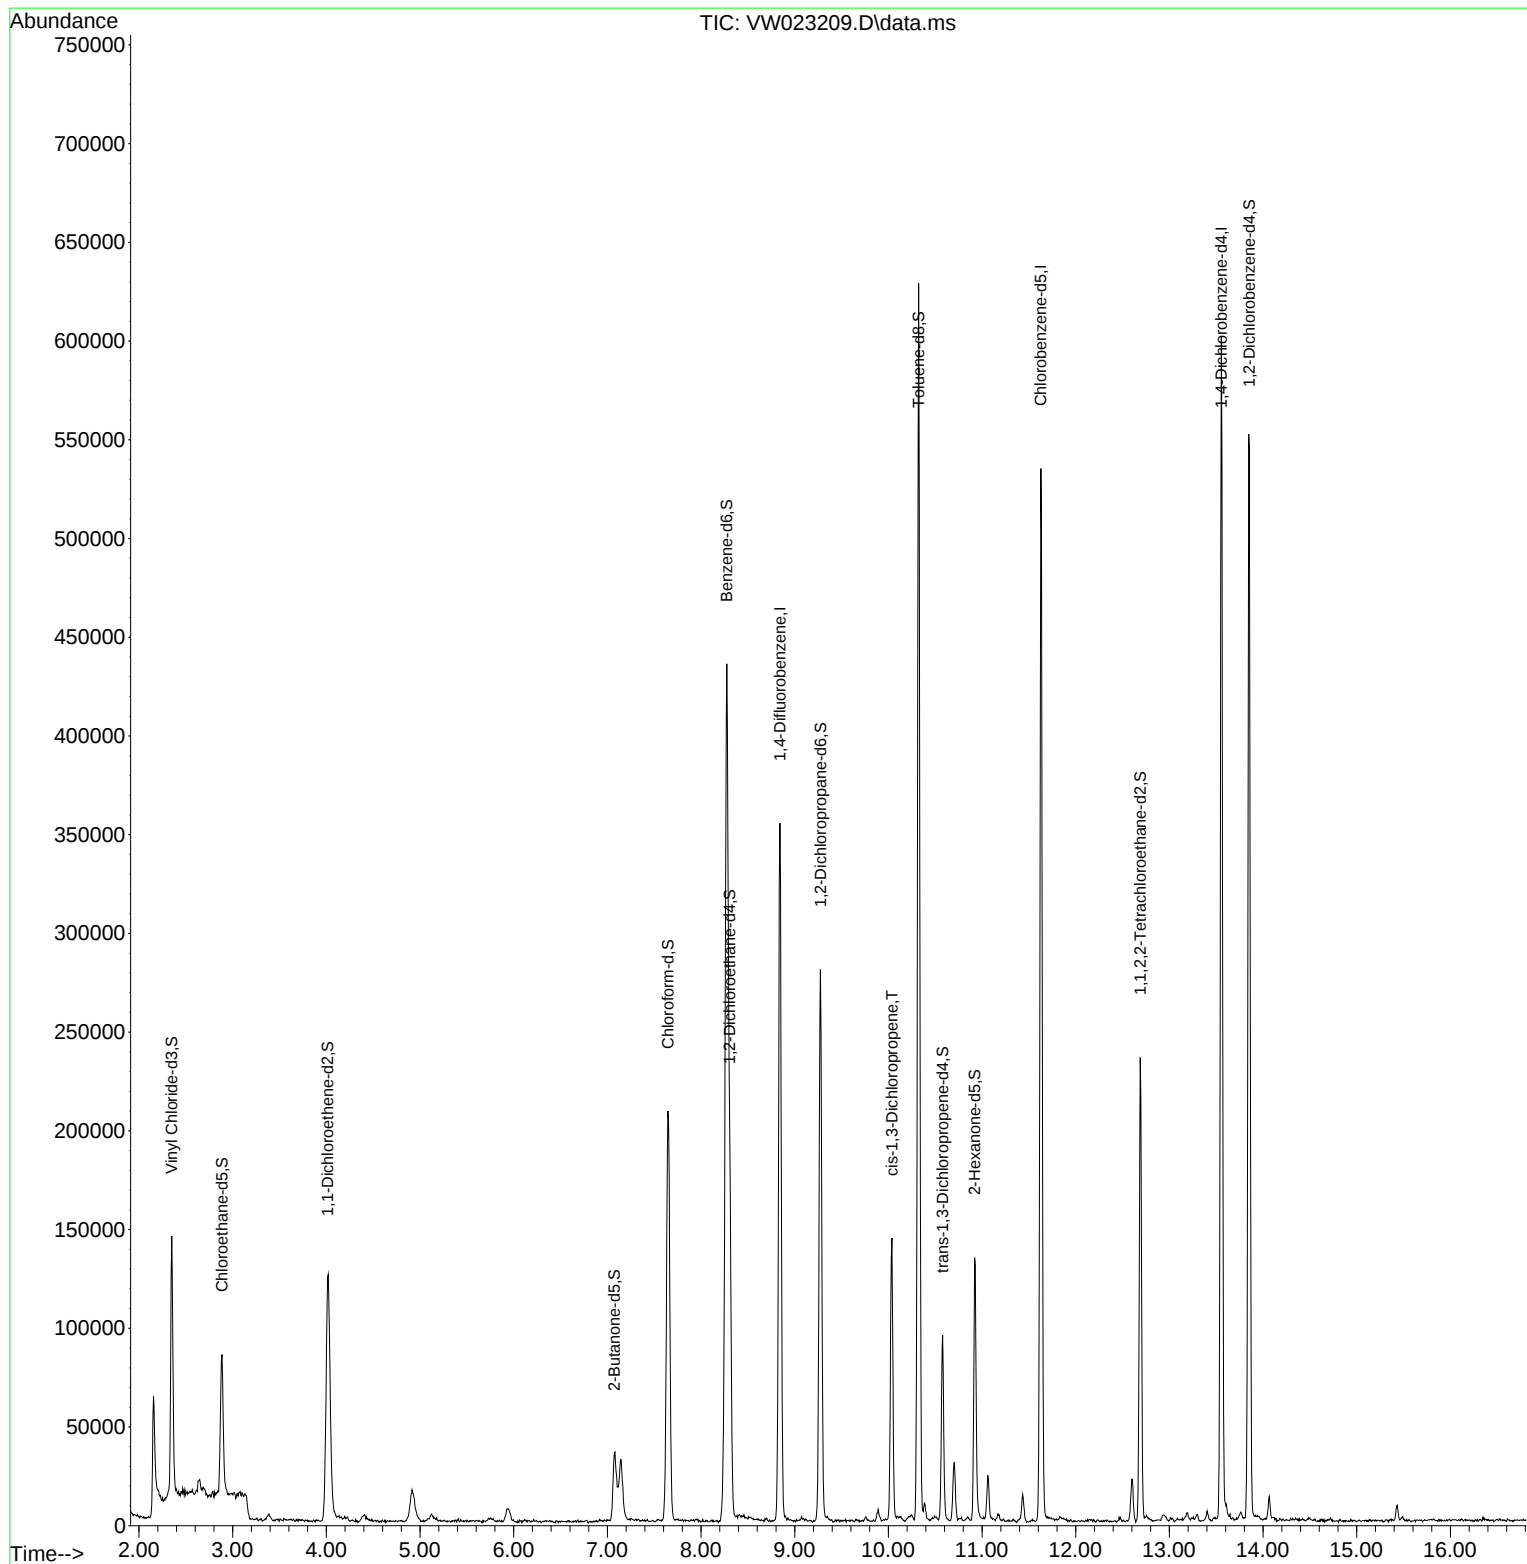

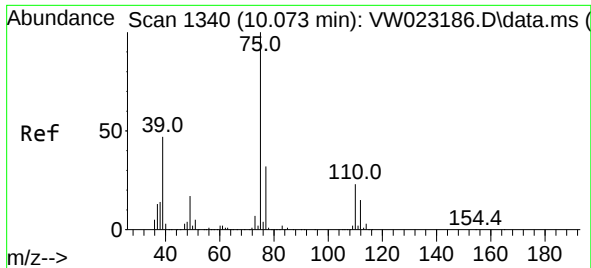

#39

cis-1,3-Dichloropropene

Concen: 0.698 ug/L

RT: 10.037 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW023209.D

Acq: 20 May 2022 19:23

Instrument :

MSVOA_W

ClientSampleId :

VIBLK470

Tgt Ion: 75 Resp: 4434

Ion Ratio Lower Upper

75 100

77 49.3 22.1 41.1#

