

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023216.D
 Acq On : 20 May 2022 23:00
 Operator : SY/VA
 Sample : N2925-19RE
 Misc : 4.76g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXZ6

Quant Time: May 21 01:50:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	358112	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	361789	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	177136	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	126104	17.164	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.640%
7) Chloroethane-d5	2.879	69	76525	16.010	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.040%
11) 1,1-Dichloroethene-d2	4.013	63	119917	12.632	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.520%
21) 2-Butanone-d5	7.080	46	65169	46.651	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.300%
24) Chloroform-d	7.647	84	232197	22.131	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.520%
26) 1,2-Dichloroethane-d4	8.305	65	134583	23.388	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.560%
32) Benzene-d6	8.275	84	432002	20.716	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.880%
36) 1,2-Dichloropropane-d6	9.275	67	133588	22.805	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.240%
41) Toluene-d8	10.323	98	395263	19.622	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.480%
43) trans-1,3-Dichloroprop...	10.579	79	52481	19.458	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.840%
47) 2-Hexanone-d5	10.921	63	54841	49.043	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.080%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	126182	23.111	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	140690	22.721	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.880%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4965	0.621	ug/L	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023216.D
Acq On : 20 May 2022 23:00
Operator : SY/VA
Sample : N2925-19RE
Misc : 4.76g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXXZ6

Quant Time: May 21 01:50:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 21 01:30:17 2022
Response via : Initial Calibration

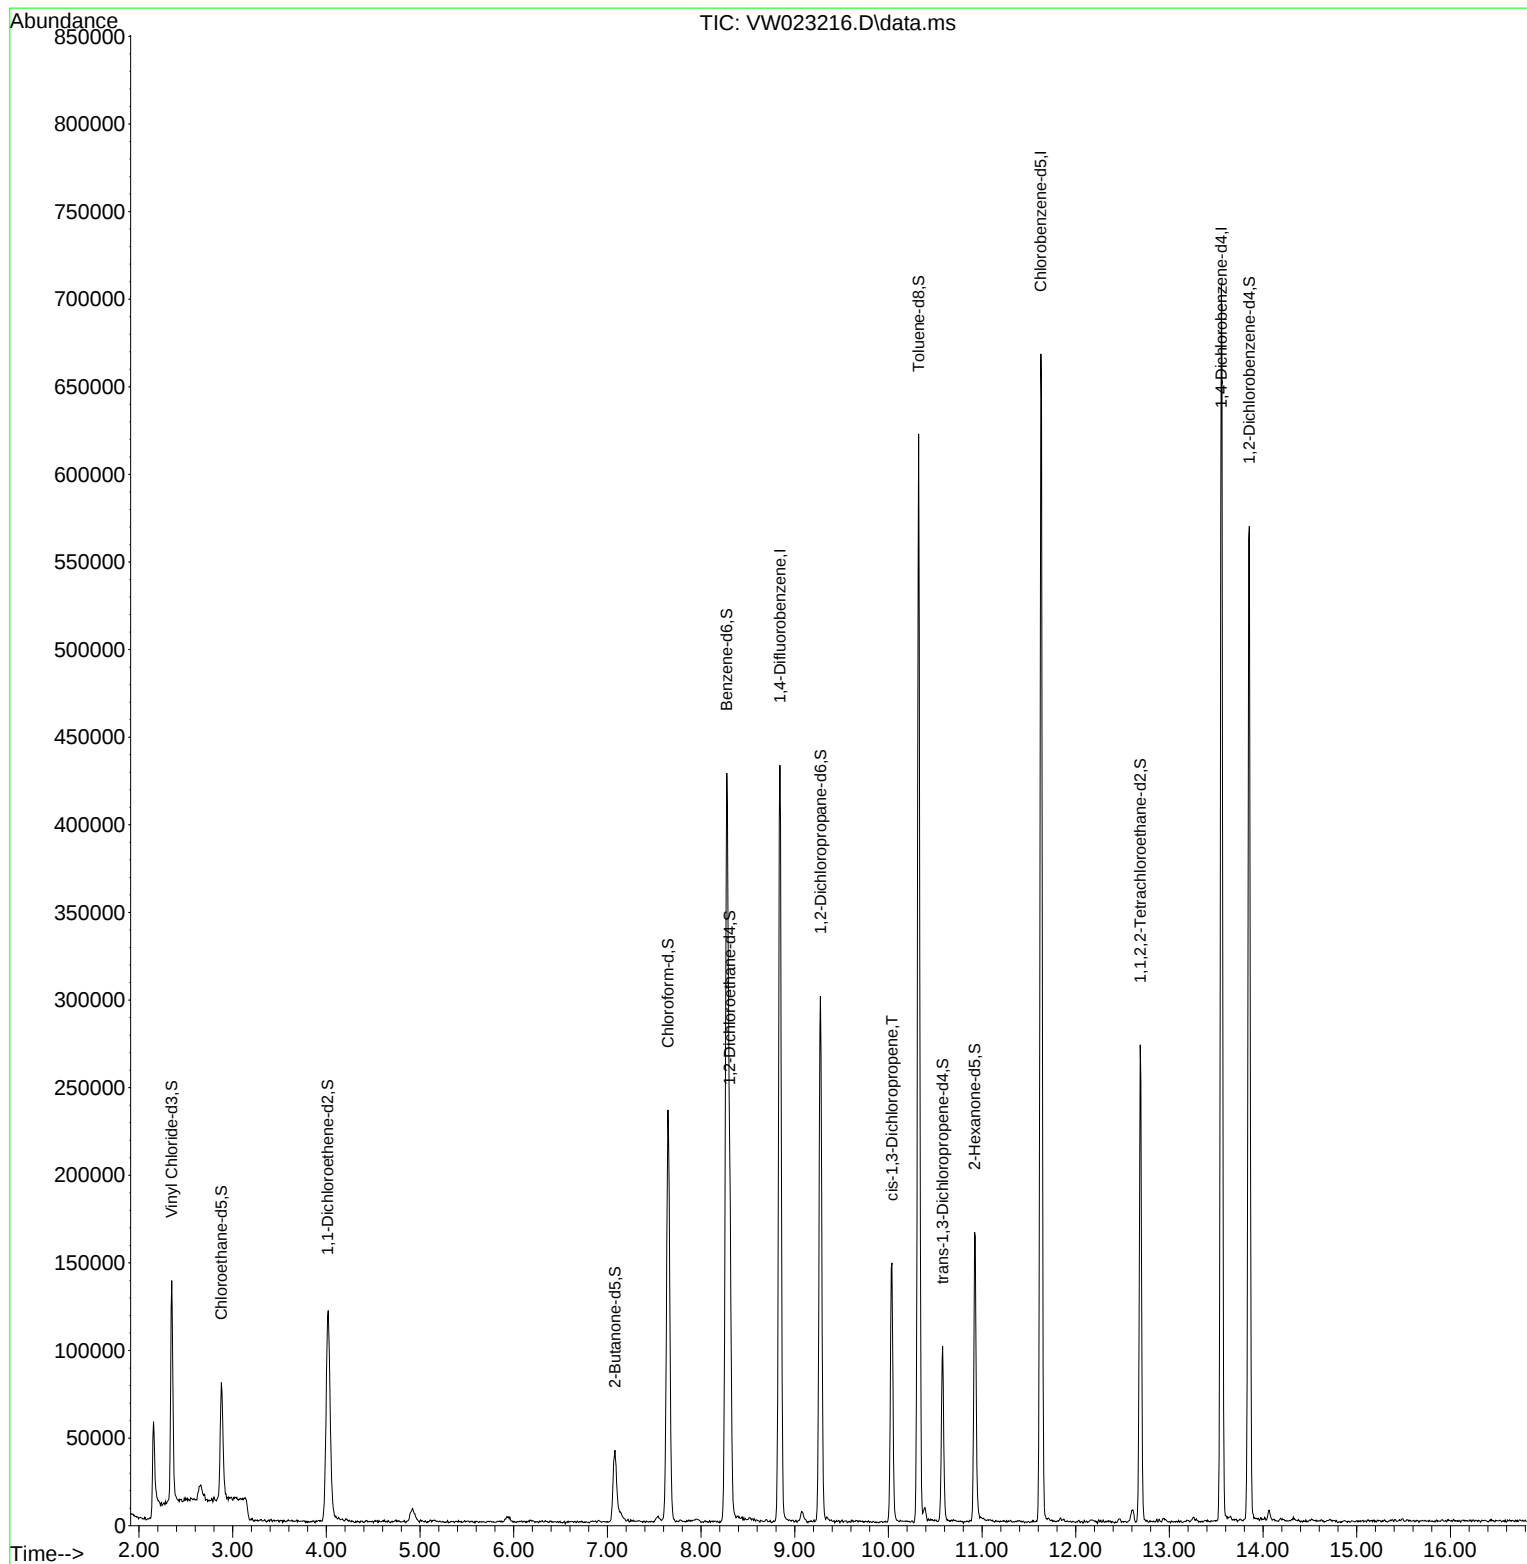

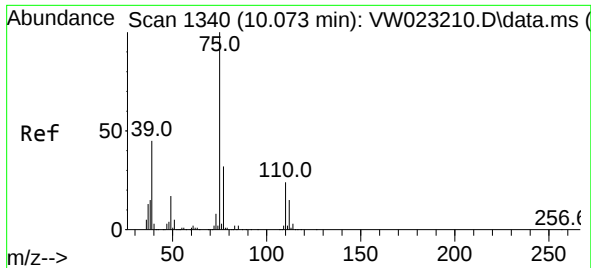

#39
 cis-1,3-Dichloropropene
 Concen: 0.621 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW023216.D
 Acq: 20 May 2022 23:00

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXZ6

Tgt Ion: 75 Resp: 4965
 Ion Ratio Lower Upper
 75 100
 77 45.1 22.1 41.1#

