




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023191.D
 Acq On : 20 May 2022 12:09
 Operator : SY/VA
 Sample : N2929-08
 Misc : 7.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBTG2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 20 23:03:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

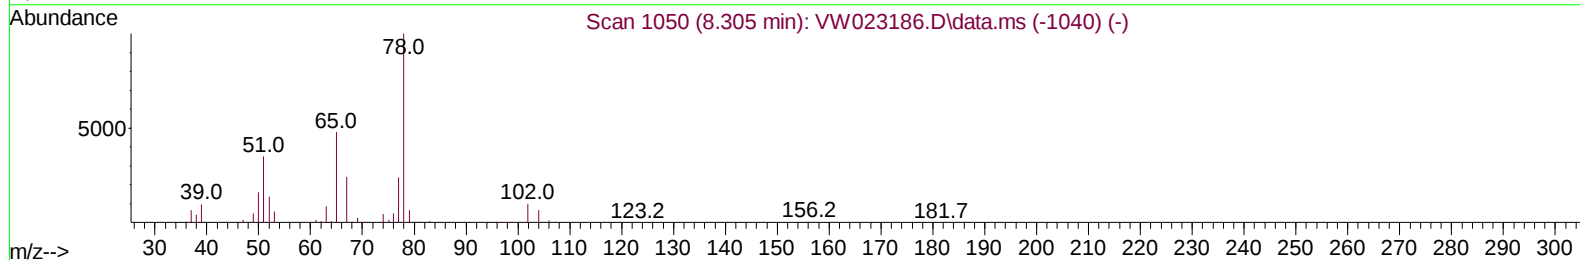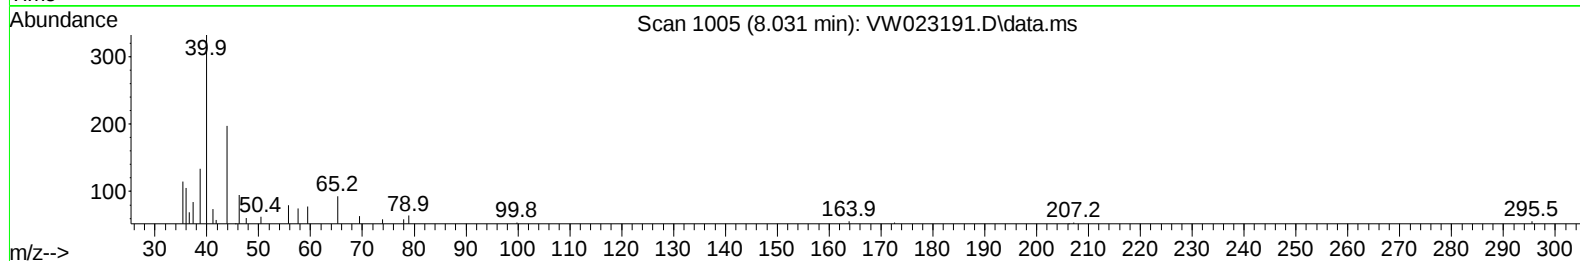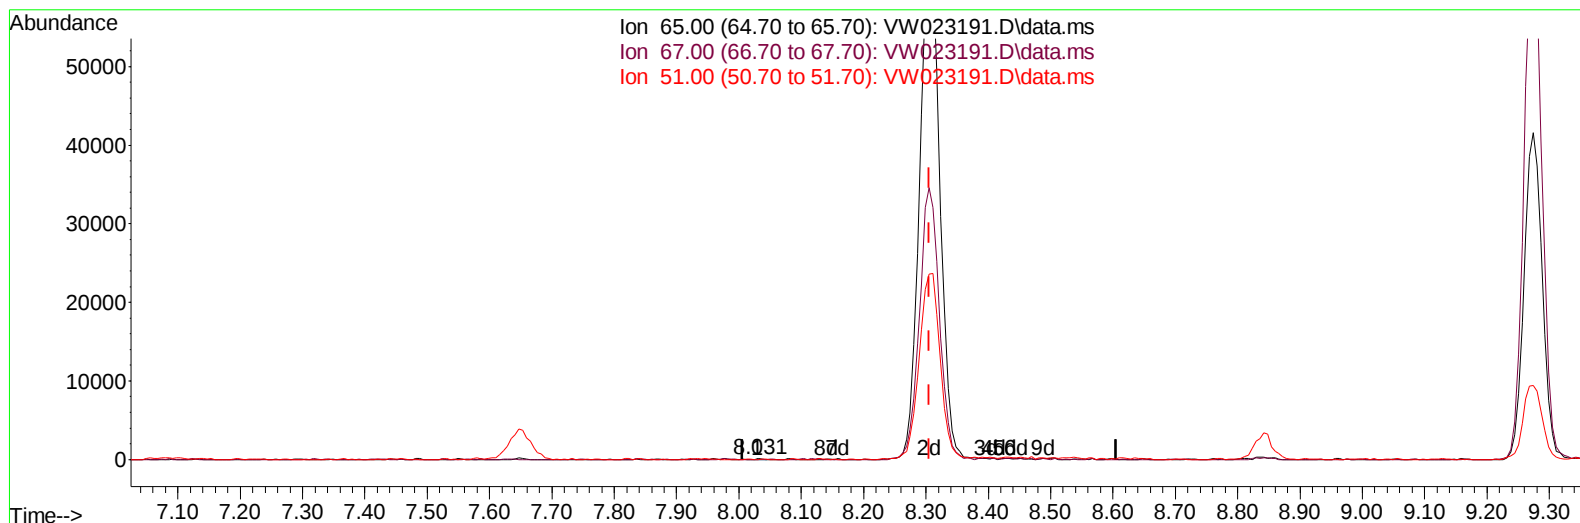

TIC: VW023191.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.031min (-0.274) 0.01 ug/L

response 67

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	65.67
51.00	92.30	85.07
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023191.D
 Acq On : 20 May 2022 12:09
 Operator : SY/VA
 Sample : N2929-08
 Misc : 7.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBTG2

Manual IntegrationsAPPROVED

Quant Time: May 20 23:03:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

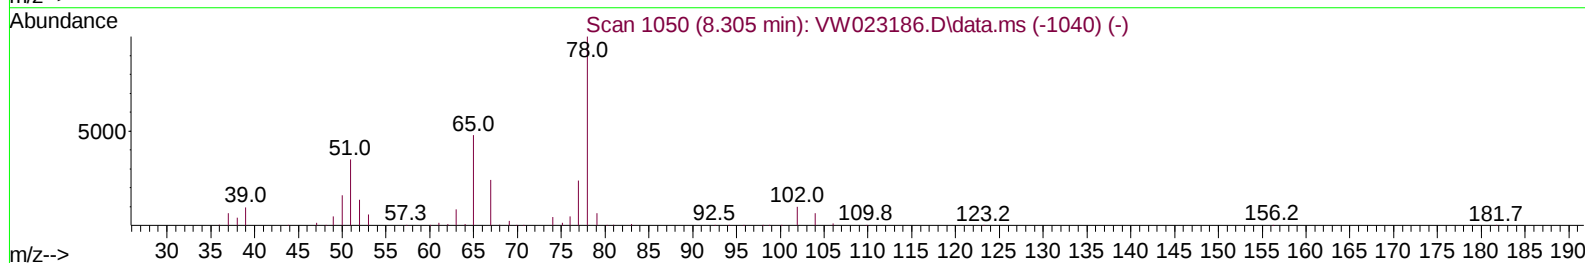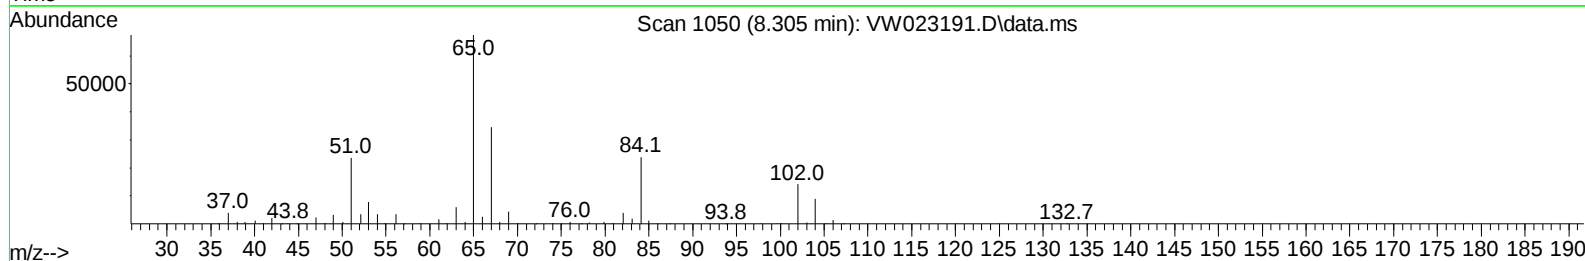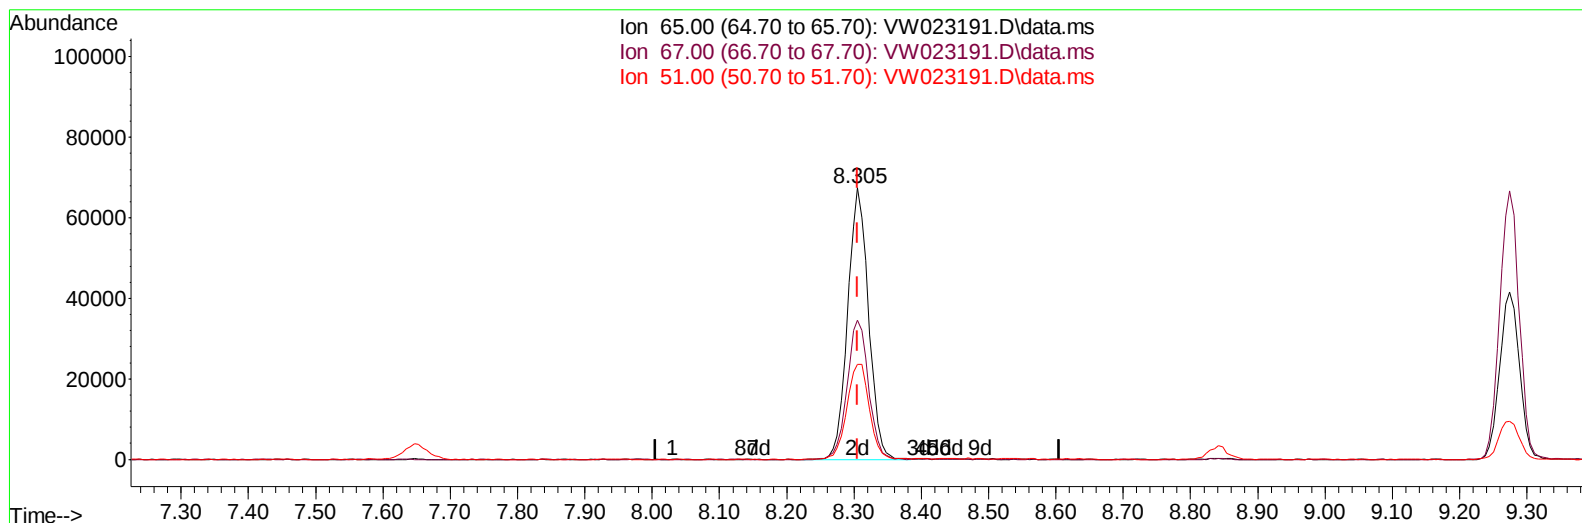

TIC: VW023191.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 26.99 ug/L m

response 144685

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.03#
51.00	92.30	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023191.D
 Acq On : 20 May 2022 12:09
 Operator : SY/VA
 Sample : N2929-08
 Misc : 7.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBTG2

Manual IntegrationsAPPROVED

Quant Time: May 20 23:03:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		333642	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		328714	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		171568	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		135292	19.765	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	79.040%	
7) Chloroethane-d5	2.885	69		78790	17.692	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	70.760%	
11) 1,1-Dichloroethene-d2	4.019	63		142294	16.088	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	64.360%	
21) 2-Butanone-d5	7.080	46		94434	72.559	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	145.120%#	
24) Chloroform-d	7.647	84		227710	23.295	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	93.200%	
26) 1,2-Dichloroethane-d4	8.305	65		144685m	26.988	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	107.960%	
32) Benzene-d6	8.275	84		451751	23.843	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	95.360%	
36) 1,2-Dichloropropane-d6	9.274	67		134424	25.257	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	101.040%	
41) Toluene-d8	10.323	98		435529	23.796	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	95.200%	
43) trans-1,3-Dichloroprop...	10.579	79		60372	24.636	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	98.560%	
47) 2-Hexanone-d5	10.921	63		84248	82.921	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	165.840%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		161775	32.611	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	130.440%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		161823	26.982	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	107.920%	
Target Compounds							
13) Acetone	4.129	43		9751	10.007	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023191.D
Acq On : 20 May 2022 12:09
Operator : SY/VA
Sample : N2929-08
Misc : 7.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBTG2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 20 23:03:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 20 23:01:40 2022
Response via : Initial Calibration

