




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023198.D
 Acq On : 20 May 2022 14:57
 Operator : SY/VA
 Sample : N2925-04
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY06

Manual IntegrationsAPPROVED

Quant Time: May 21 00:56:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

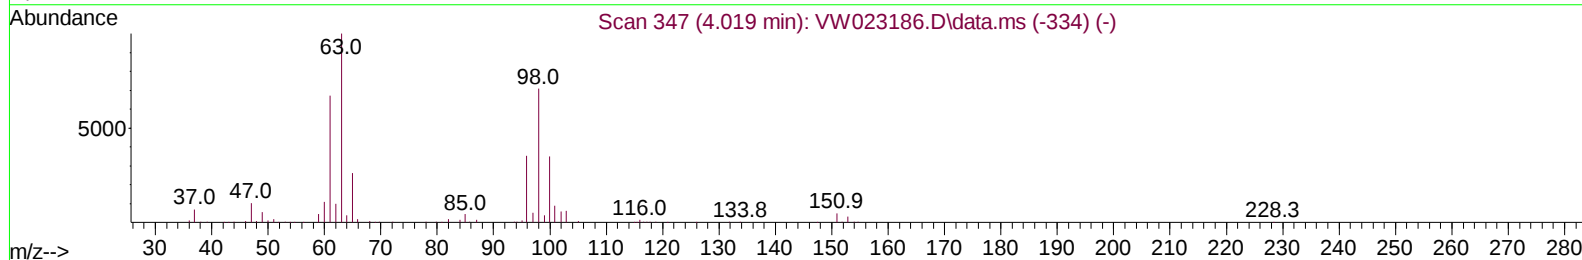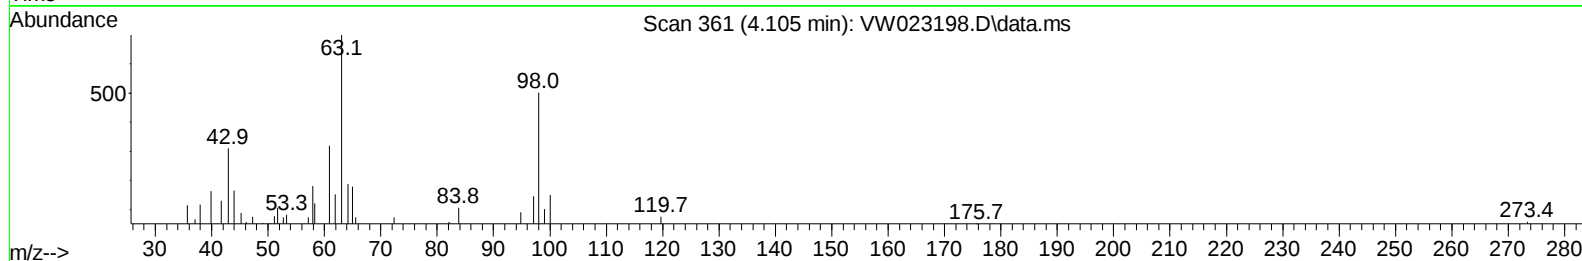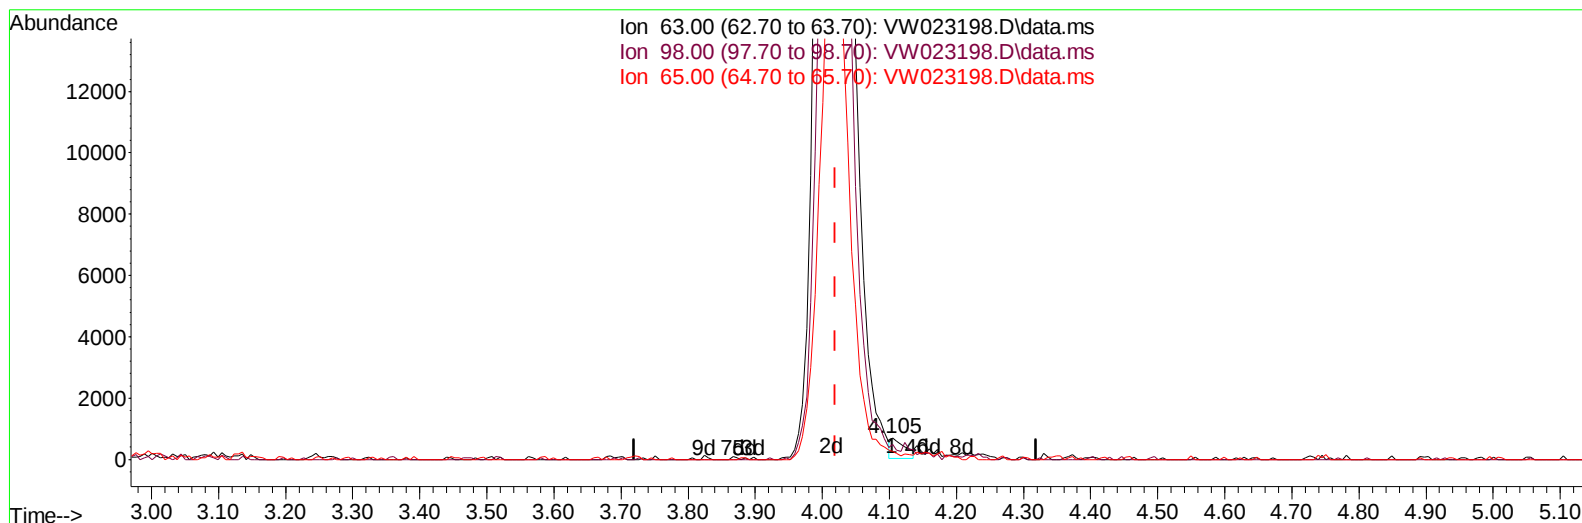

TIC: VW023198.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.105min (+ 0.085) 0.09 ug/L

response 962

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	51.14
65.00	23.30	17.36
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023198.D
Acq On : 20 May 2022 14:57
Operator : SY/VA
Sample : N2925-04
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY06

Manual IntegrationsAPPROVED

Quant Time: May 21 00:56:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 20 23:01:40 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
Supervised By :Mahesh Dadoda 05/25/2022

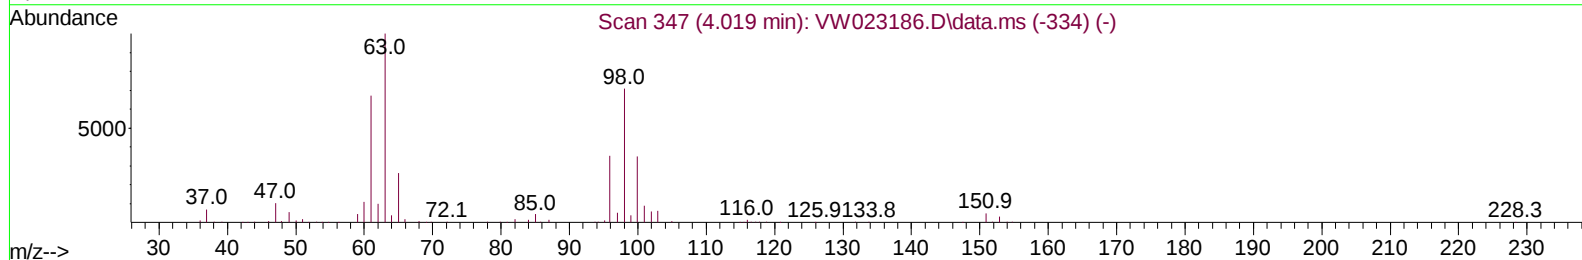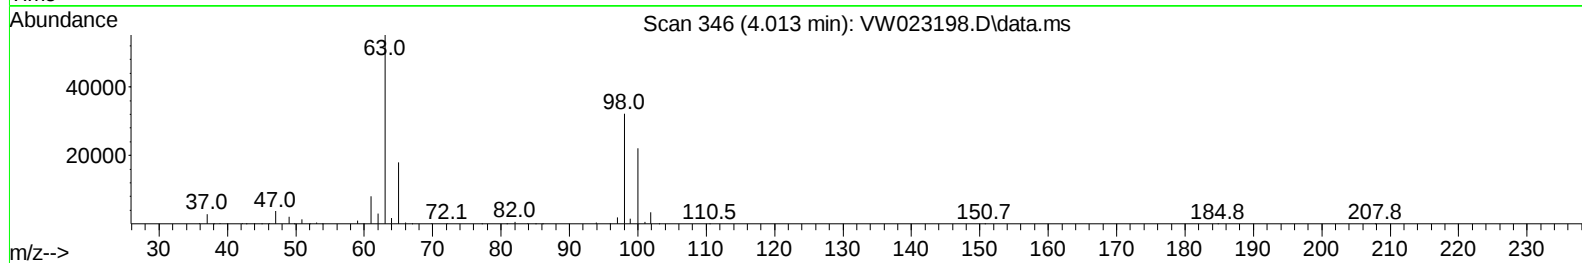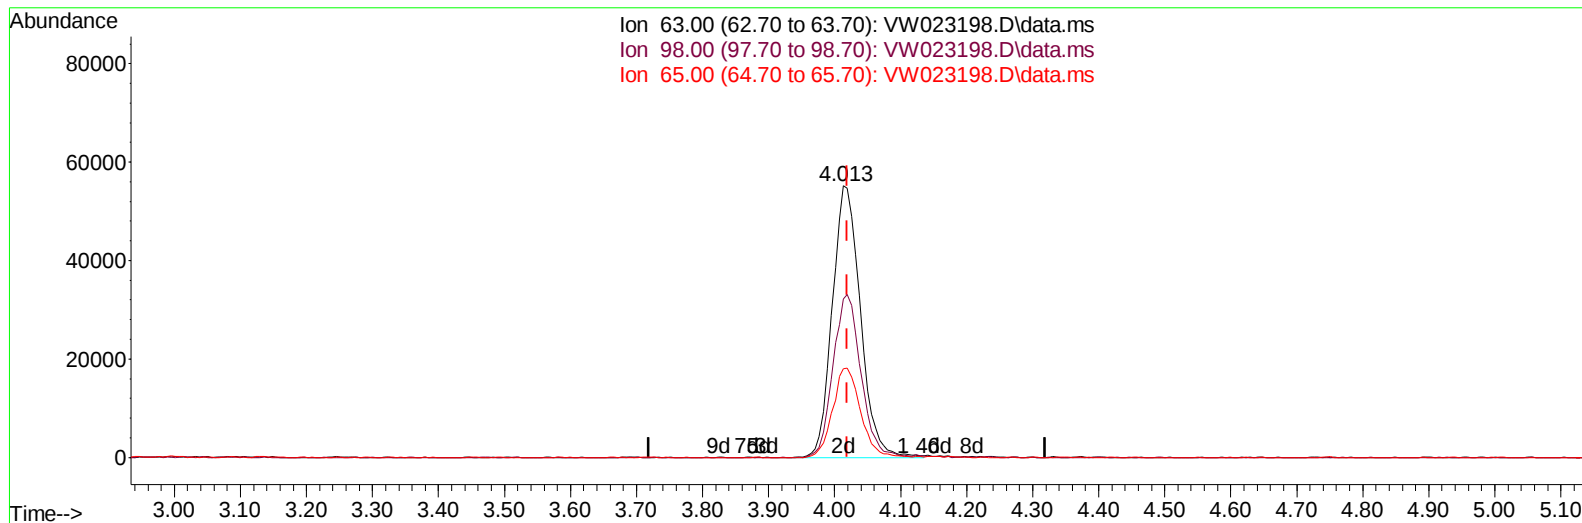

TIC: VW023198.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 14.53 ug/L m

response 163175

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.30#
65.00	23.30	0.10#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023198.D
 Acq On : 20 May 2022 14:57
 Operator : SY/VA
 Sample : N2925-04
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY06

Manual IntegrationsAPPROVED

Quant Time: May 21 00:56:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

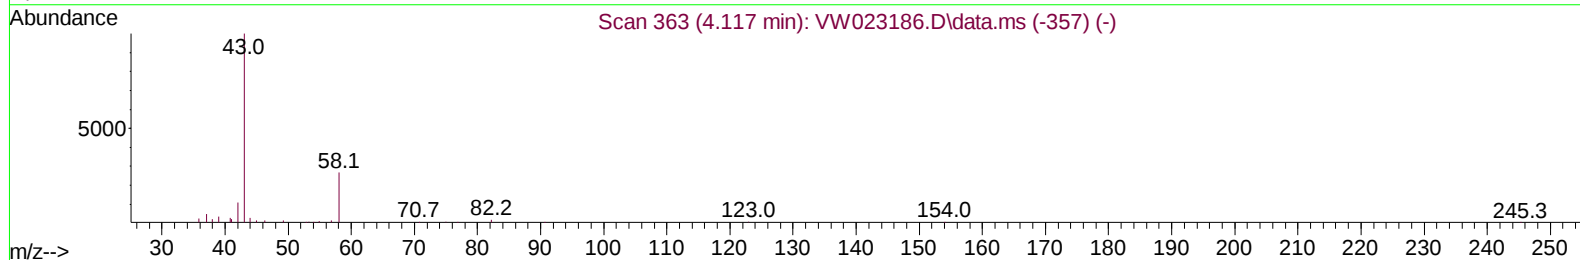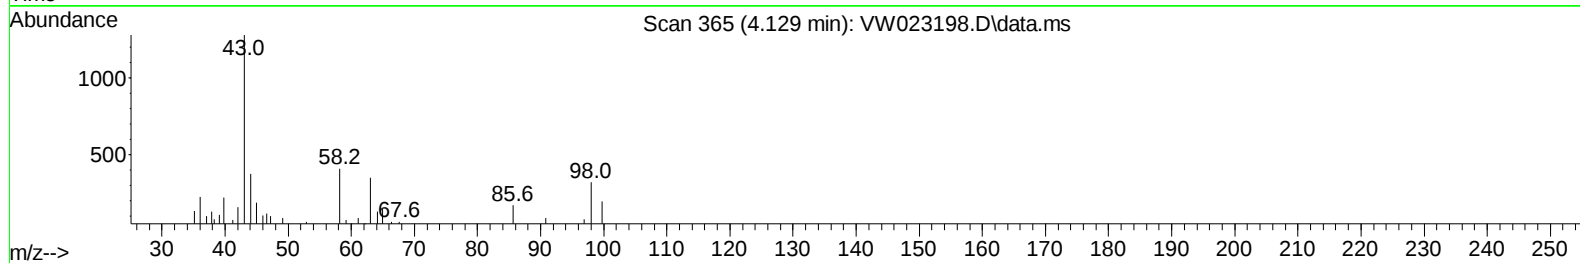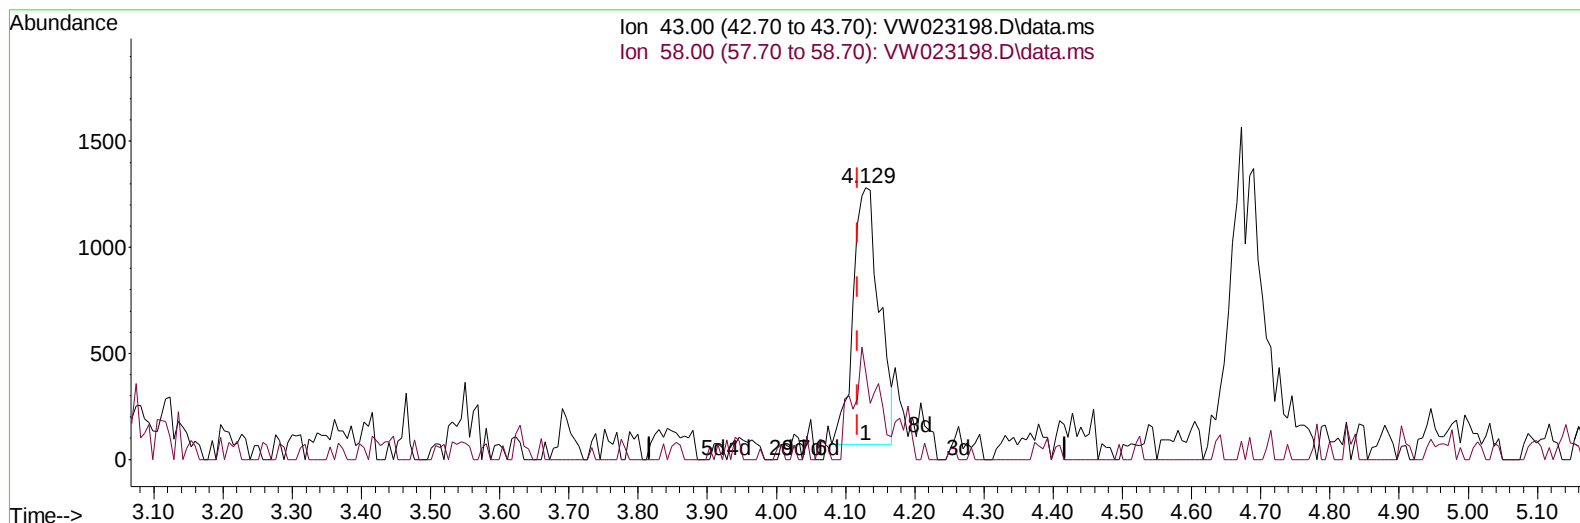

TIC: VW023198.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 2.57 ug/L

response 3179

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	17.14
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023198.D
 Acq On : 20 May 2022 14:57
 Operator : SY/VA
 Sample : N2925-04
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY06

Manual IntegrationsAPPROVED

Quant Time: May 21 00:56:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

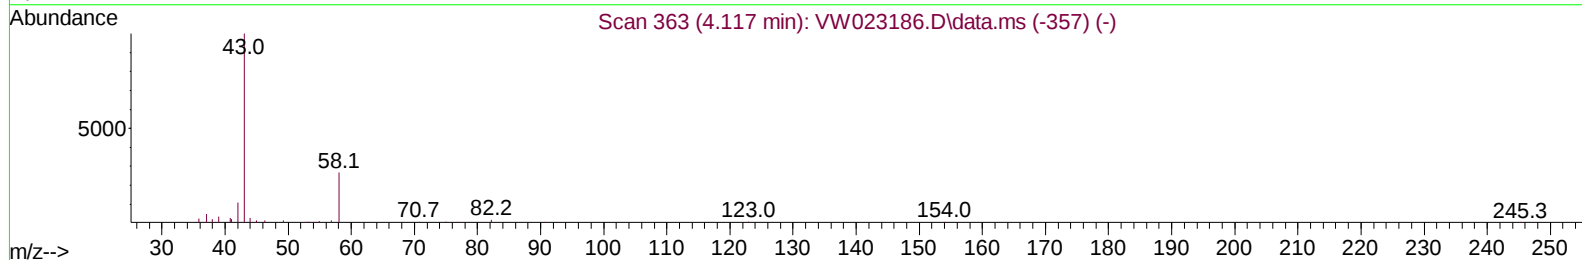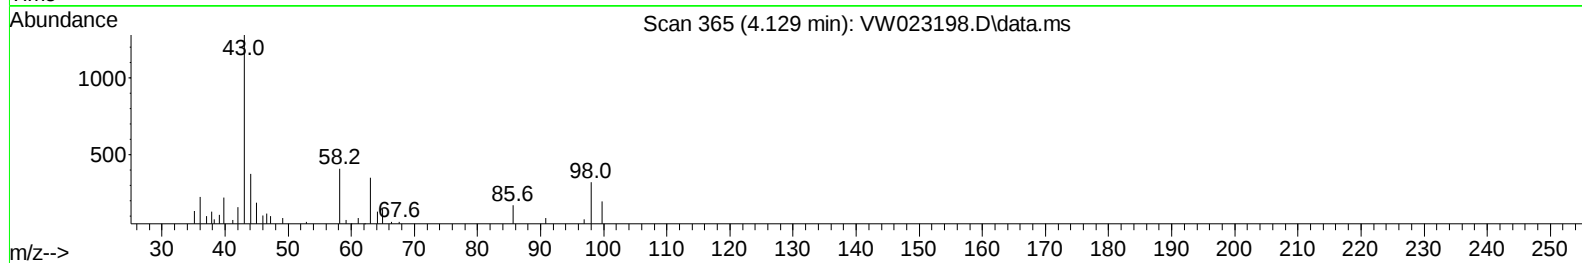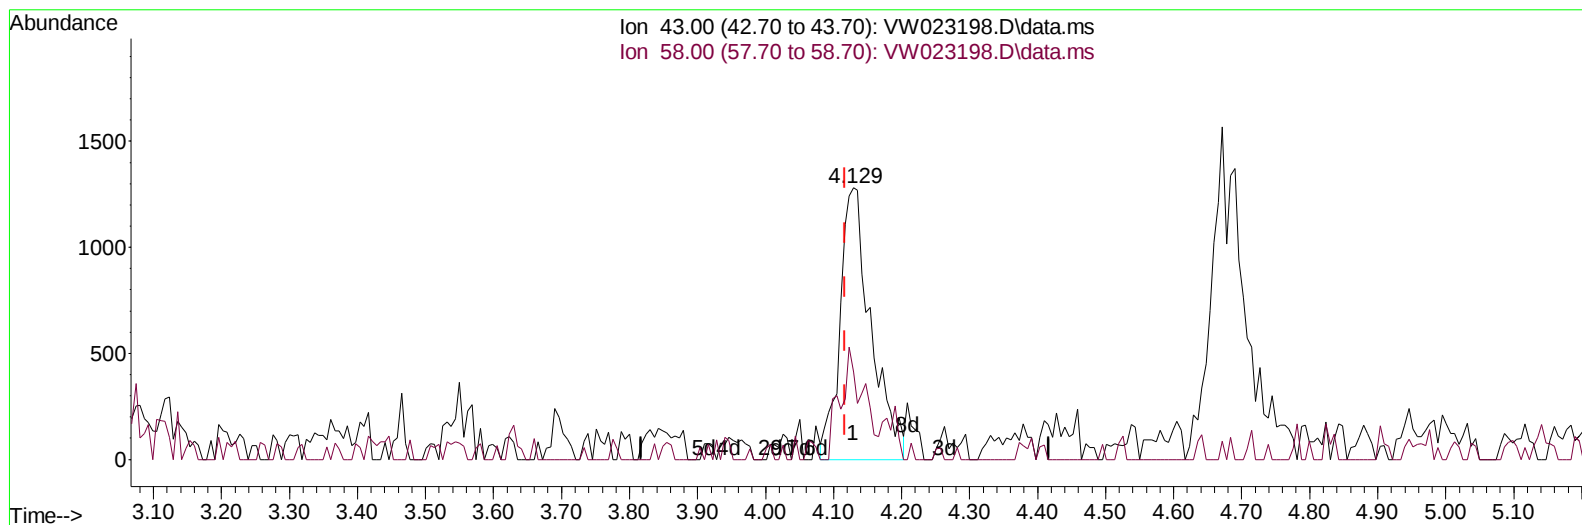

TIC: VW023198.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 3.26 ug/L m

response 4036

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	13.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023198.D
 Acq On : 20 May 2022 14:57
 Operator : SY/VA
 Sample : N2925-04
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY06

Manual IntegrationsAPPROVED

Quant Time: May 21 00:56:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

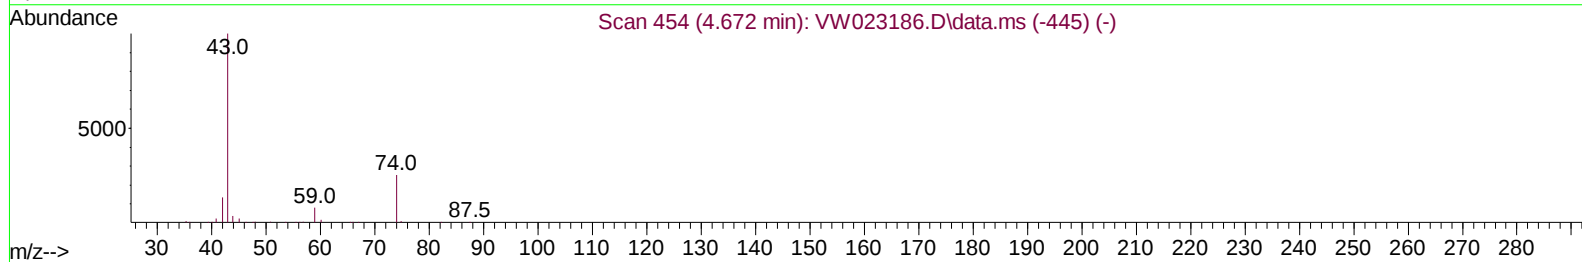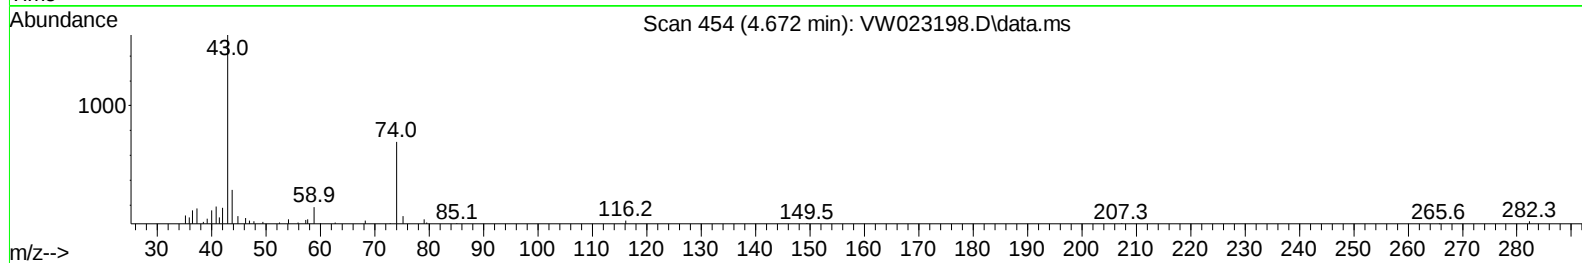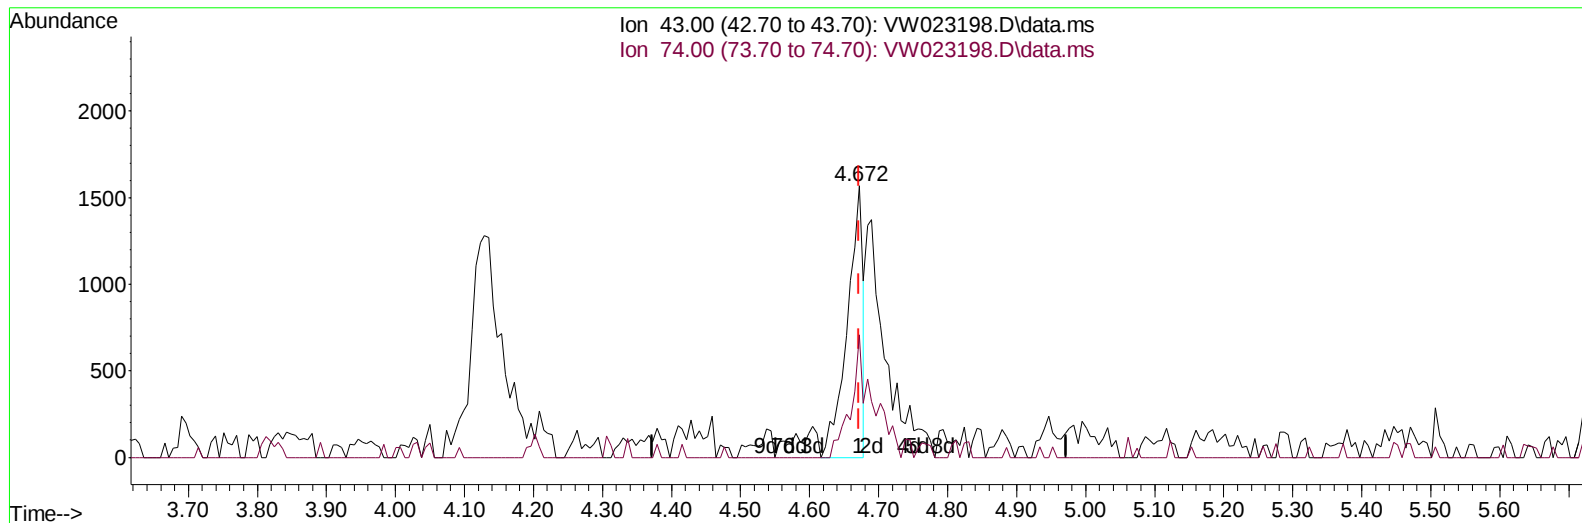

TIC: VW023198.D\data.ms

(15) Methyl Acetate (T)

4.672min (-0.000) 1.00 ug/L

response 2476

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.40	33.24#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023198.D
 Acq On : 20 May 2022 14:57
 Operator : SY/VA
 Sample : N2925-04
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY06

Manual IntegrationsAPPROVED

Quant Time: May 21 00:56:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

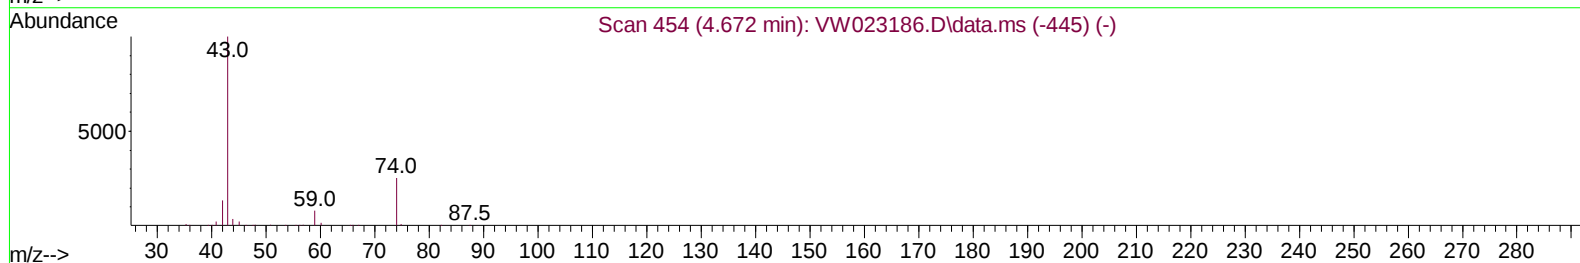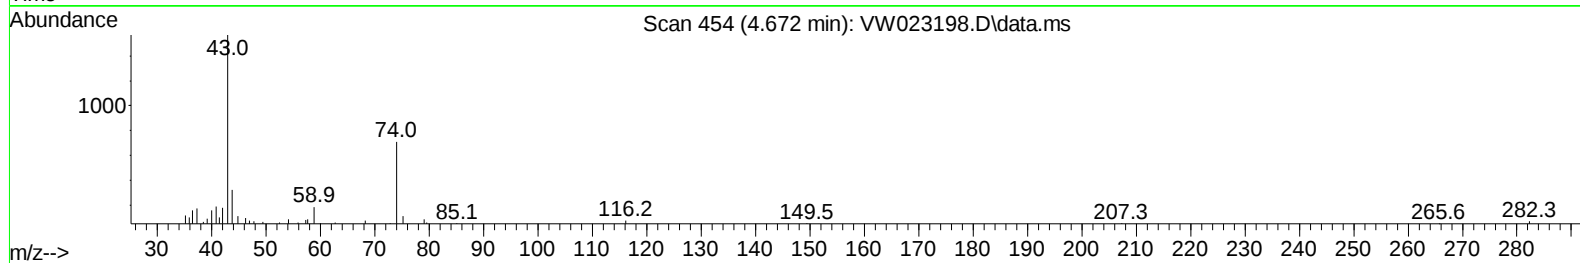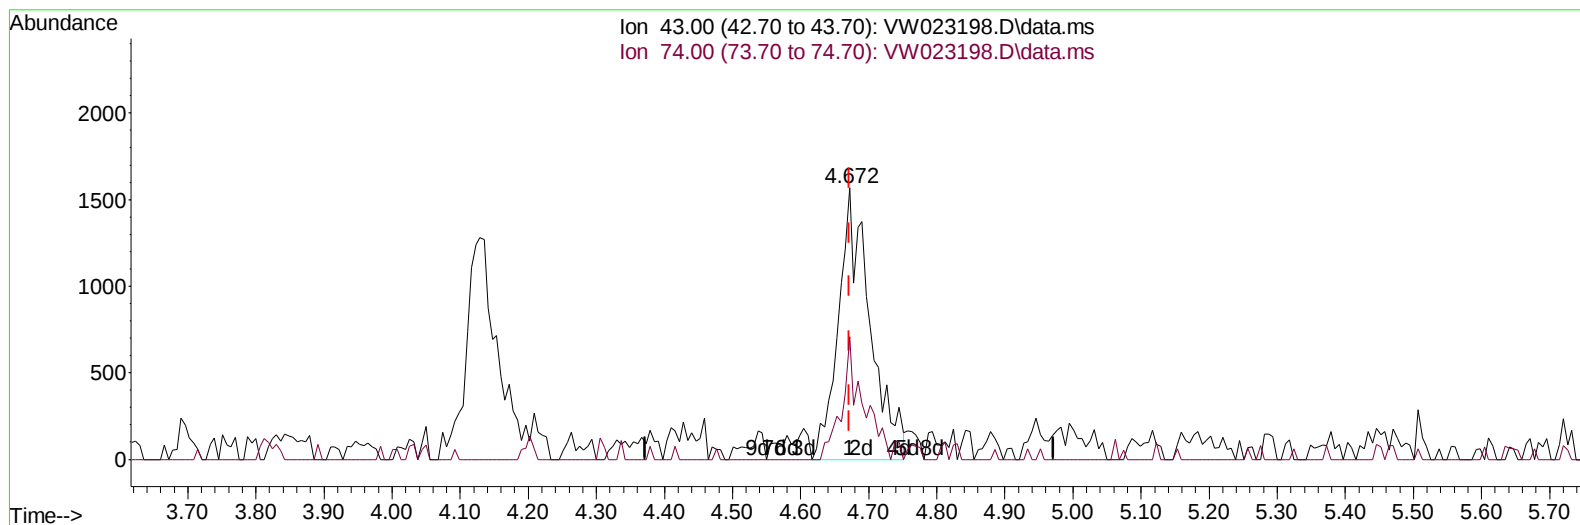

TIC: VW023198.D\data.ms

(15) Methyl Acetate (T)

4.672min (-0.000) 2.04 ug/L m

response 5067

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.40	16.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023198.D
 Acq On : 20 May 2022 14:57
 Operator : SY/VA
 Sample : N2925-04
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY06

Manual IntegrationsAPPROVED

Quant Time: May 21 00:56:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 20 23:01:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	423608	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	381198	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	151102	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	174728	20.105	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	80.400%	
7) Chloroethane-d5	2.885	69	105795	18.711	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.840%	
11) 1,1-Dichloroethene-d2	4.013	63	163175m	14.531	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	58.120%	
21) 2-Butanone-d5	7.074	46	60461	36.589	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	73.180%	
24) Chloroform-d	7.647	84	295041	23.773	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.080%	
26) 1,2-Dichloroethane-d4	8.305	65	166068	24.397	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.600%	
32) Benzene-d6	8.275	84	536795	24.431	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	97.720%	
36) 1,2-Dichloropropane-d6	9.275	67	169606	27.480	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	109.920%	
41) Toluene-d8	10.323	98	484180	22.812	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	91.240%	
43) trans-1,3-Dichloroprop...	10.579	79	59492	20.934	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	83.720%	
47) 2-Hexanone-d5	10.921	63	45986	39.030	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	78.060%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	137177	23.846	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4	13.853	152	140552	26.610	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	106.440%	
Target Compounds						
13) Acetone	4.129	43	4036m	3.262	ug/L	Qvalue
15) Methyl Acetate	4.672	43	5067m	2.039	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023198.D
Acq On : 20 May 2022 14:57
Operator : SY/VA
Sample : N2925-04
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY06

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 21 00:56:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 20 23:01:40 2022
Response via : Initial Calibration

