




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023215.D
 Acq On : 20 May 2022 22:35
 Operator : SY/VA
 Sample : N2925-18
 Misc : 4.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXZ5

Manual IntegrationsAPPROVED

Quant Time: May 21 01:50:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

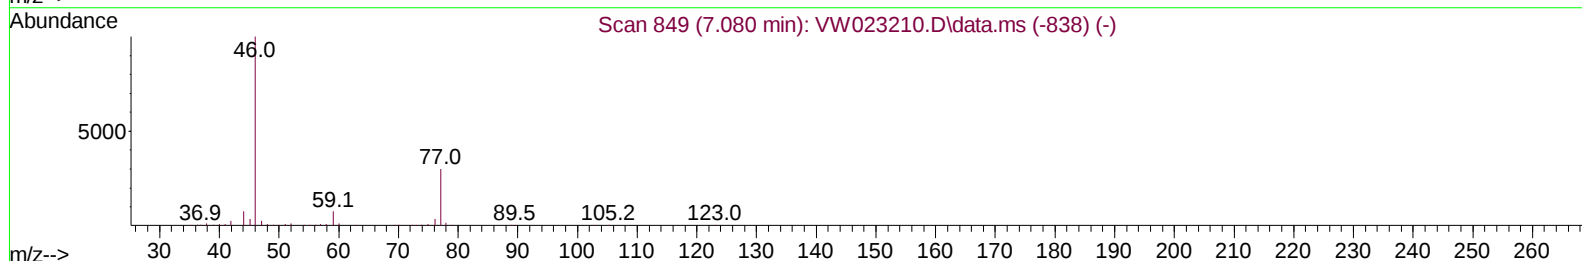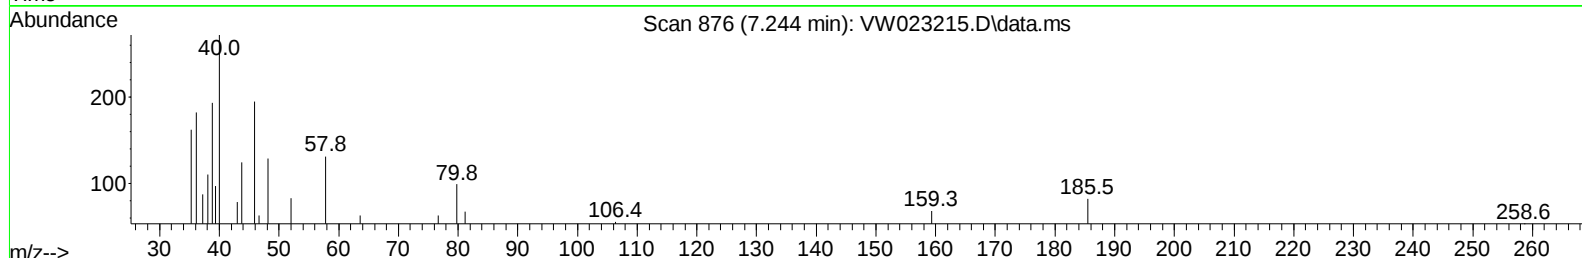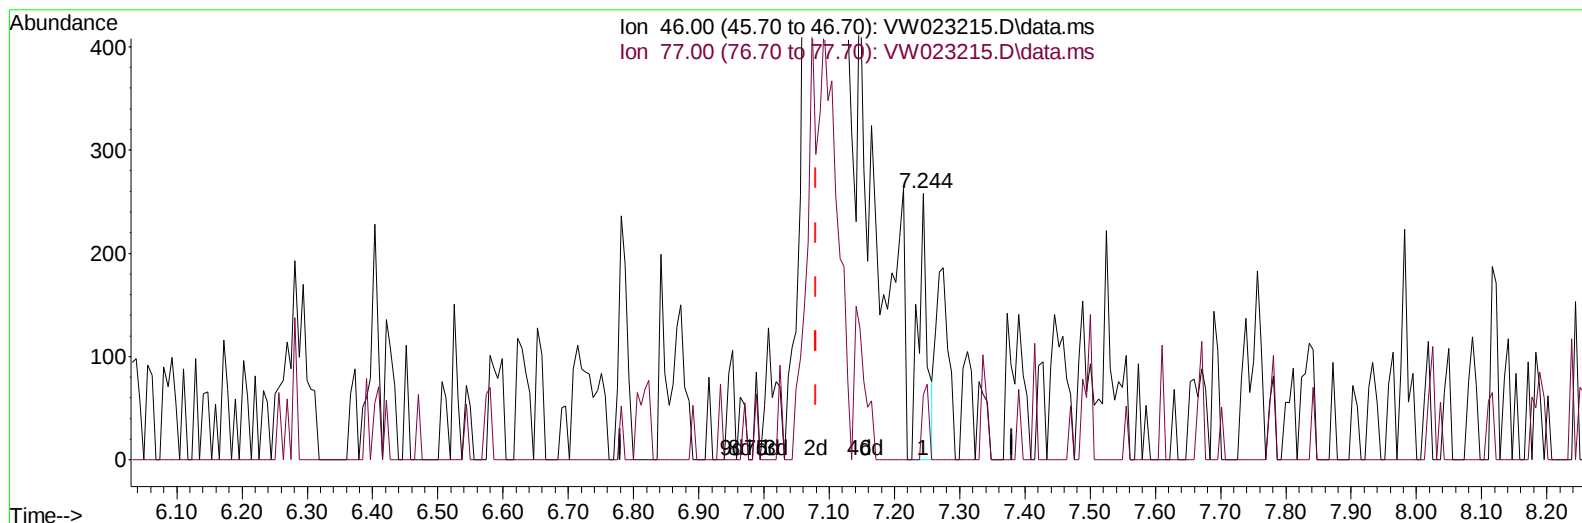

TIC: VW023215.D\data.ms

(21) 2-Butanone-d5 (S)

7.244min (+ 0.165) 2.61 ug/L

response 248

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	20.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023215.D
 Acq On : 20 May 2022 22:35
 Operator : SY/VA
 Sample : N2925-18
 Misc : 4.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXZ5

Manual IntegrationsAPPROVED

Quant Time: May 21 01:50:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

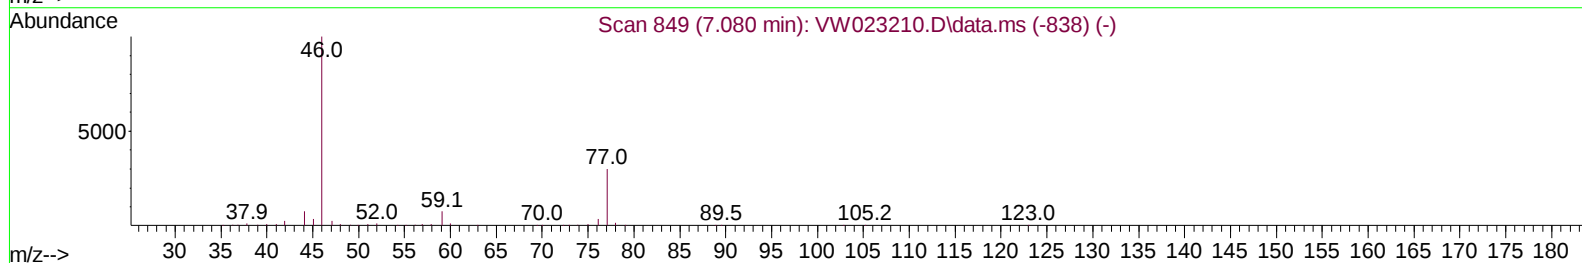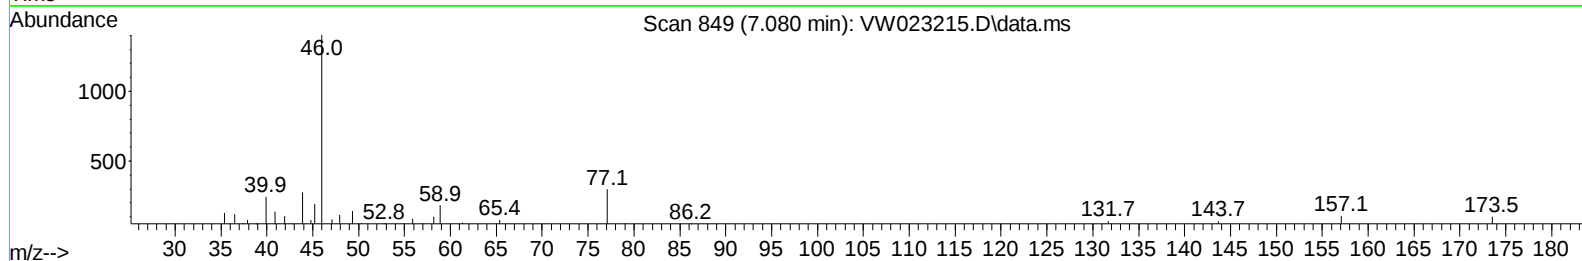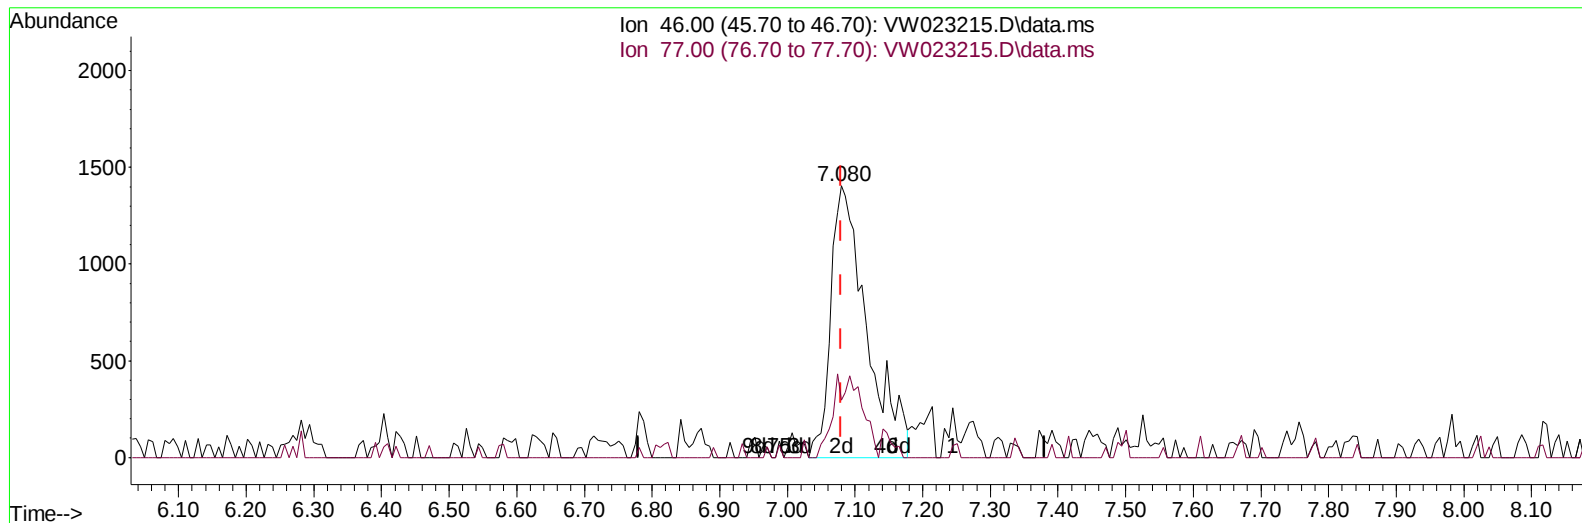

TIC: VW023215.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.000) 54.84 ug/L m

response 5209

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.96#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023215.D
 Acq On : 20 May 2022 22:35
 Operator : SY/VA
 Sample : N2925-18
 Misc : 4.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXXZ5

Manual IntegrationsAPPROVED

Quant Time: May 21 01:50:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	24348	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	21245	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	6914	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	13285	26.595	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	106.360%	
7) Chloroethane-d5	2.892	69	7884	24.259	ug/L	0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	97.040%	
11) 1,1-Dichloroethene-d2	4.032	63	12218	18.929	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	75.720%	
21) 2-Butanone-d5	7.080	46	5209m	54.845	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	109.680%	
24) Chloroform-d	7.653	84	20427	28.636	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	114.560%	
26) 1,2-Dichloroethane-d4	8.305	65	12310	31.464	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	125.840%	
32) Benzene-d6	8.281	84	34194	27.924	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	111.680%	
36) 1,2-Dichloropropane-d6	9.275	67	11985	34.842	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	139.360%#	
41) Toluene-d8	10.323	98	25792	21.804	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	87.200%	
43) trans-1,3-Dichloroprop...	10.579	79	3462	21.859	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	87.440%	
47) 2-Hexanone-d5	10.921	63	1710	26.041	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	52.080%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	9548	29.781	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	119.120%	
66) 1,2-Dichlorobenzene-d4	13.853	152	6640	27.473	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	109.880%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023215.D
Acq On : 20 May 2022 22:35
Operator : SY/VA
Sample : N2925-18
Misc : 4.53g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXXZ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 21 01:50:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 21 01:30:17 2022
Response via : Initial Calibration

