




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023227.D
 Acq On : 21 May 2022 03:24
 Operator : SY/VA
 Sample : N2929-06RE
 Misc : 7.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBTG0RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 21 04:08:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

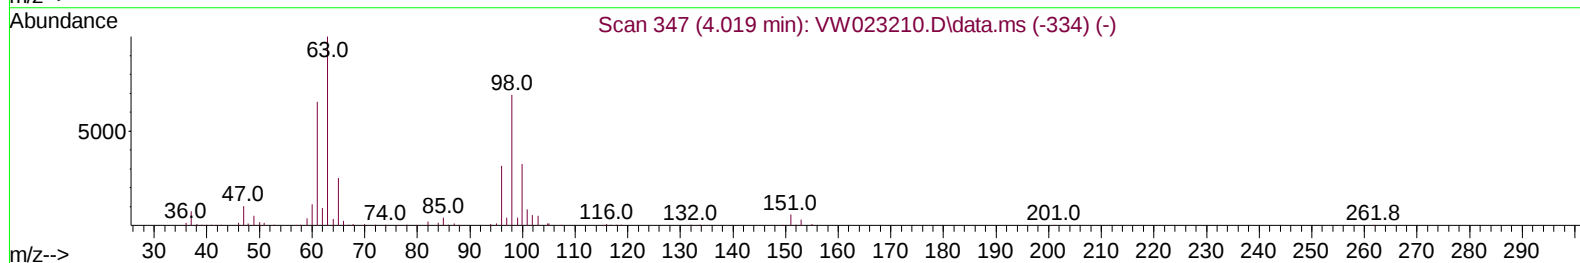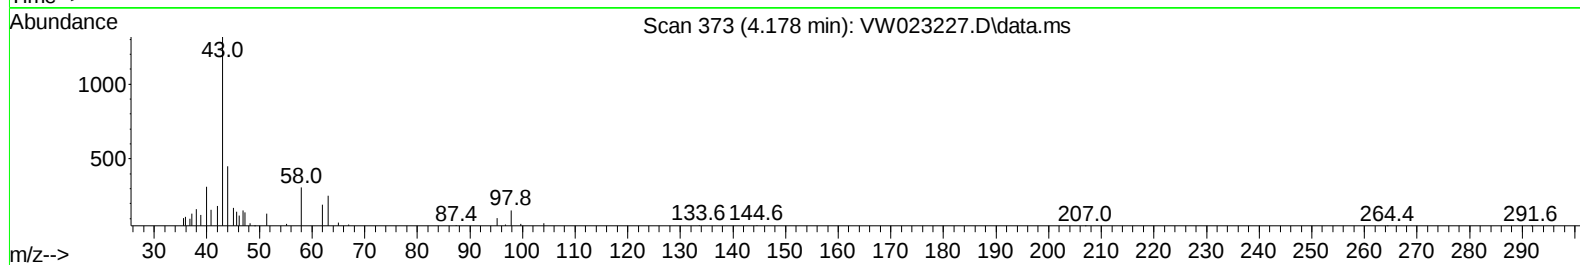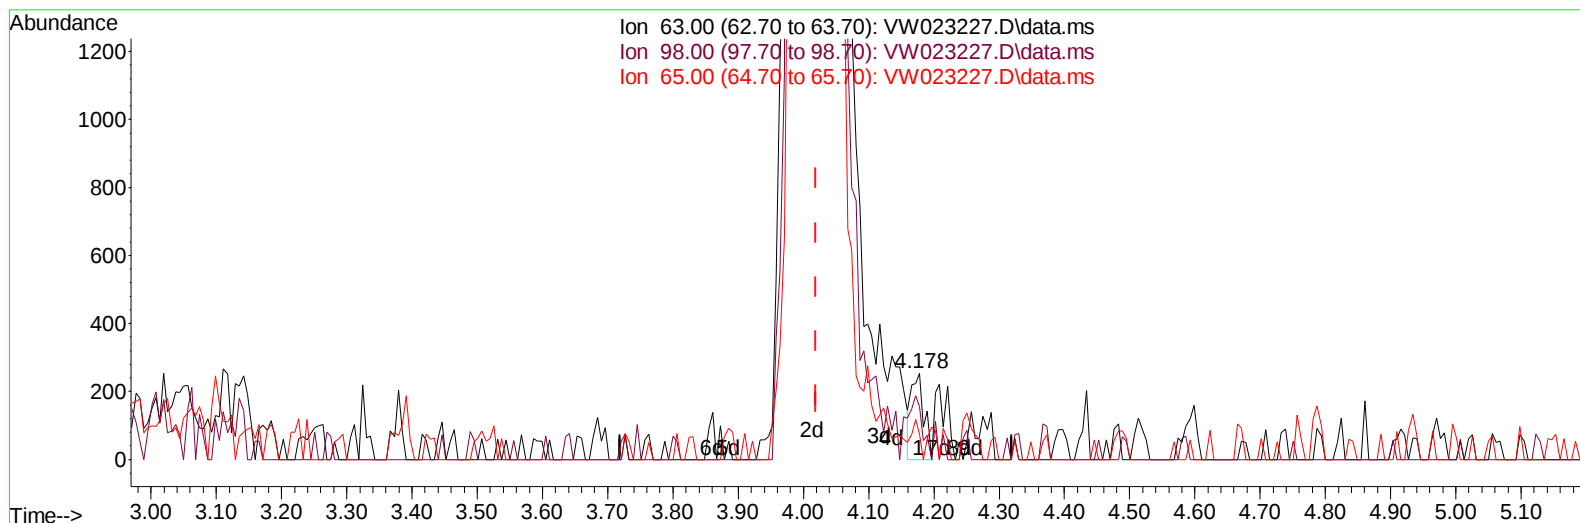

TIC: VW023227.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.178min (+ 0.159) 0.04 ug/L

response 342

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	92.40
65.00	23.30	28.36
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023227.D
Acq On : 21 May 2022 03:24
Operator : SY/VA
Sample : N2929-06RE
Misc : 7.33g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBTG0RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 21 04:08:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 21 01:30:17 2022
Response via : Initial Calibration

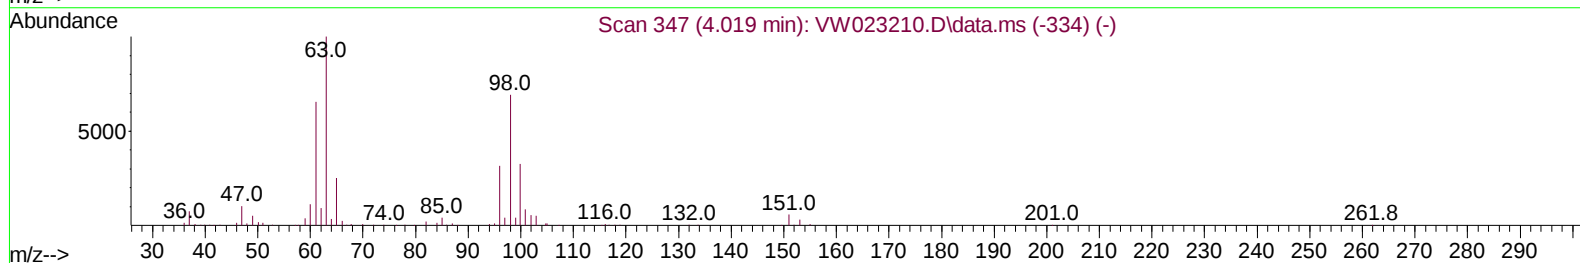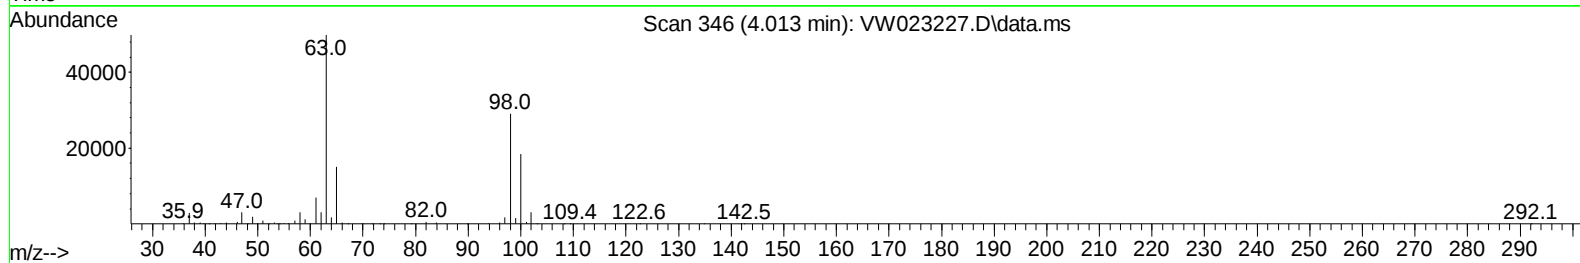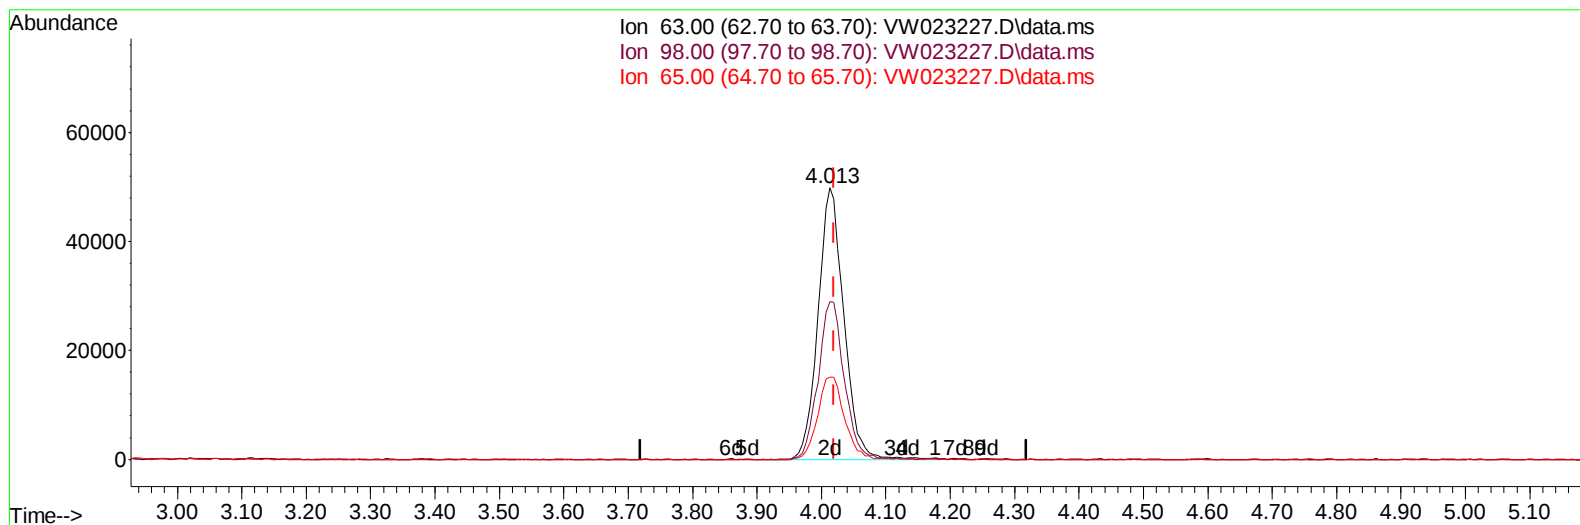

TIC: VW023227.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 14.98 ug/L m

response 139169

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.23#
65.00	23.30	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023227.D
 Acq On : 21 May 2022 03:24
 Operator : SY/VA
 Sample : N2929-06RE
 Misc : 7.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBTG0RE

Manual IntegrationsAPPROVED

Quant Time: May 21 04:08:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		350490	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		305545	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		101877	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		140215	19.499	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	78.000%	
7) Chloroethane-d5	2.879	69		86814	18.557	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	74.240%	
11) 1,1-Dichloroethene-d2	4.013	63		139169m	14.978	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	59.920%	
21) 2-Butanone-d5	7.080	46		99831	73.018	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	146.040%#	
24) Chloroform-d	7.647	84		252454	24.585	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	98.360%	
26) 1,2-Dichloroethane-d4	8.305	65		156895	27.858	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	111.440%	
32) Benzene-d6	8.275	84		465169	26.413	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	105.640%	
36) 1,2-Dichloropropane-d6	9.274	67		147644	29.845	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	119.360%	
41) Toluene-d8	10.323	98		415354	24.414	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	97.640%	
43) trans-1,3-Dichloroprop...	10.579	79		55792	24.493	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	97.960%	
47) 2-Hexanone-d5	10.920	63		84980	89.984	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	179.960%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		132880	28.818	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	115.280%	
66) 1,2-Dichlorobenzene-d4	13.853	152		83871	23.551	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	94.200%	
Target Compounds							
						Qvalue	
13) Acetone	4.123	43		56361	55.061	ug/L	96
22) 2-Butanone	7.177	43		12216	8.534	ug/L	99
33) Benzene	8.323	78		17793	0.989	ug/L	100
34) Trichloroethene	9.085	95		6590	1.331	ug/L	92
42) Toluene	10.384	91		27053	1.341	ug/L	95
46) Tetrachloroethene	10.860	164		78686	21.152	ug/L	92
52) Ethylbenzene	11.725	91		18485	0.824	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023227.D
Acq On : 21 May 2022 03:24
Operator : SY/VA
Sample : N2929-06RE
Misc : 7.33g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBTG0RE

Manual IntegrationsAPPROVED

Quant Time: May 21 04:08:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 21 01:30:17 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/22/2022
Supervised By :Mahesh Dadoda 05/25/2022

