




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023229.D
 Acq On : 21 May 2022 04:13
 Operator : SY/VA
 Sample : VIBLK474
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK474

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 21 05:21:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

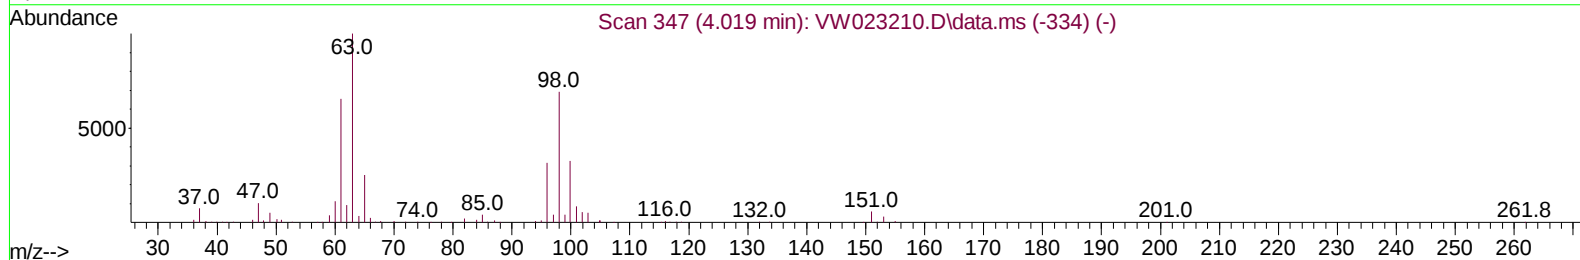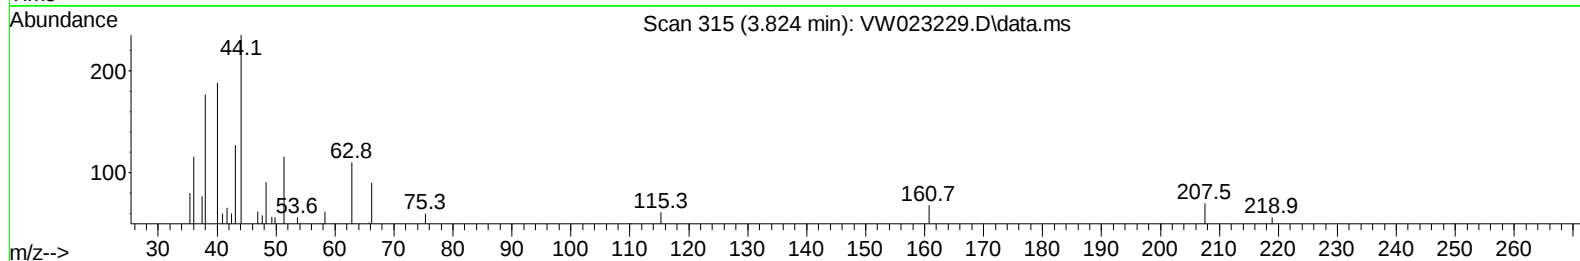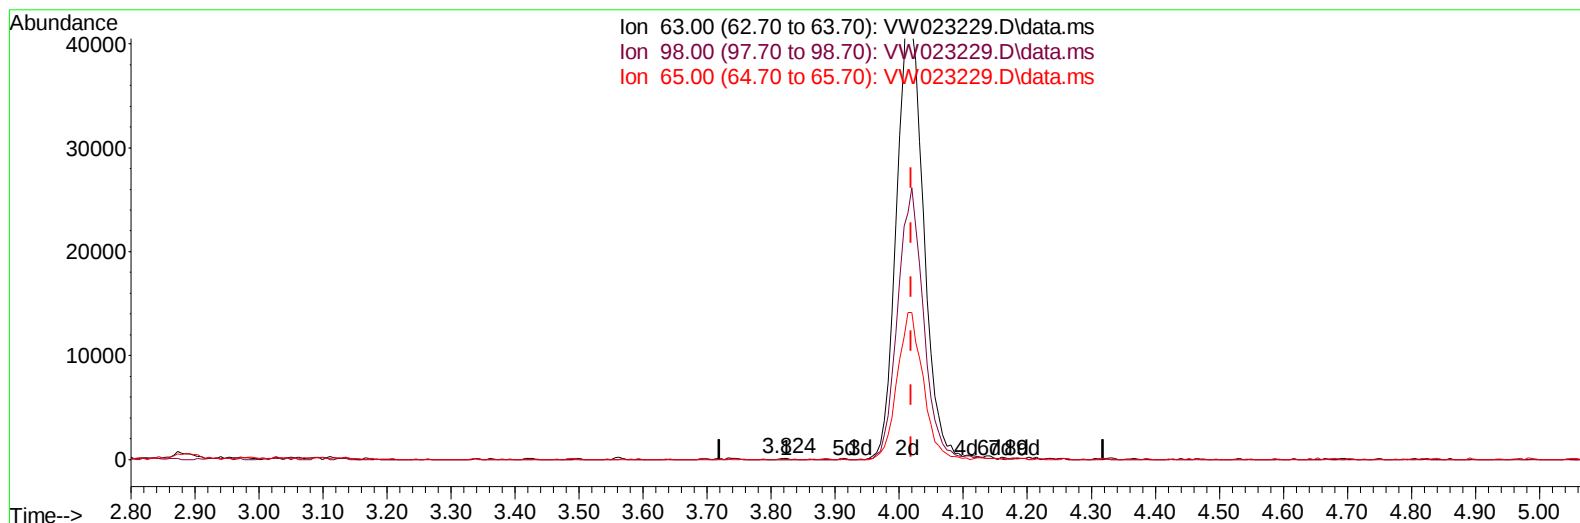

TIC: VW023229.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.824min (-0.195) 0.01 ug/L

response 93

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	93.55
65.00	23.30	24.73
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023229.D
 Acq On : 21 May 2022 04:13
 Operator : SY/VA
 Sample : VIBLK474
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK474

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 21 05:21:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

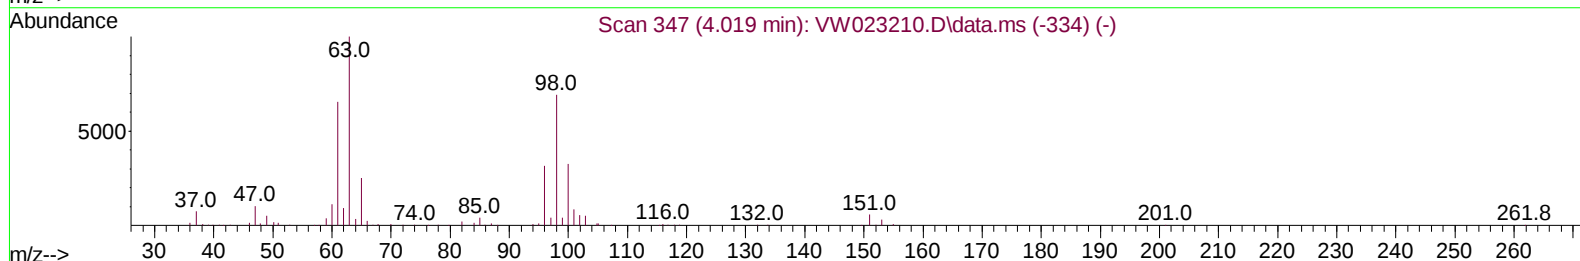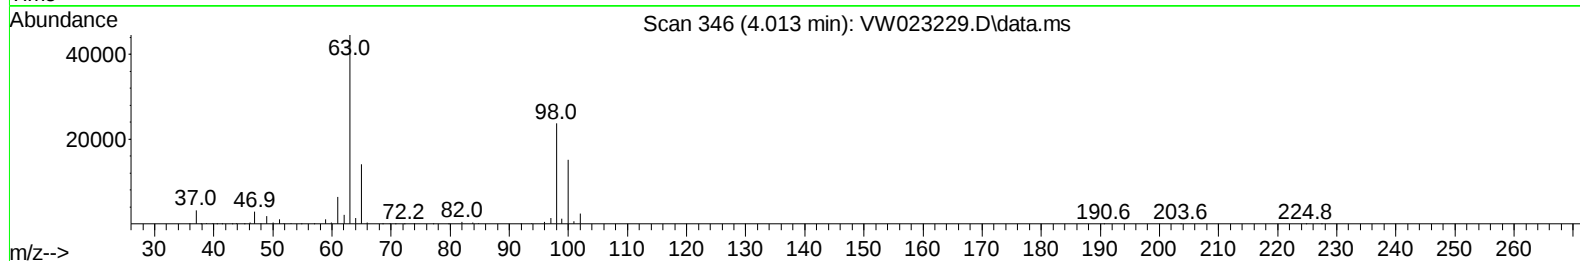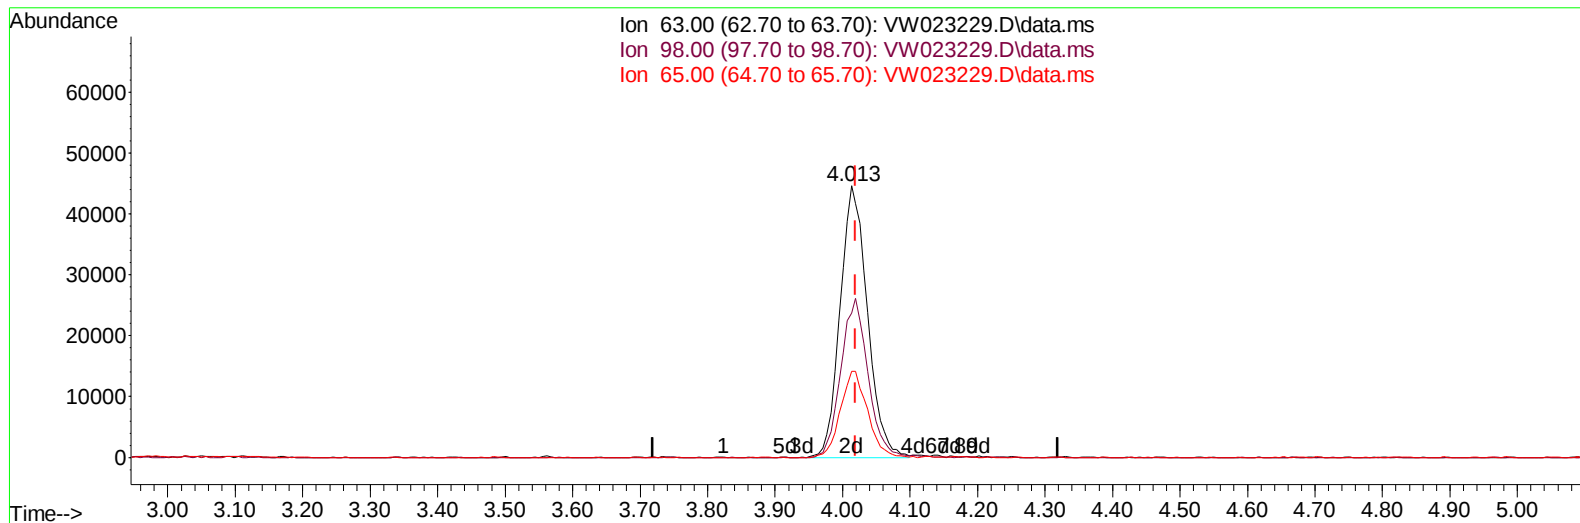

TIC: VW023229.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 15.70 ug/L m

response 125079

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.07#
65.00	23.30	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023229.D
 Acq On : 21 May 2022 04:13
 Operator : SY/VA
 Sample : VIBLK474
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK474

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 21 05:21:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	300584	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	298793	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	140022	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	126819	20.564	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	82.240%	
7) Chloroethane-d5	2.885	69	74264	18.510	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.040%	
11) 1,1-Dichloroethene-d2	4.013	63	125079m	15.697	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.800%	
21) 2-Butanone-d5	7.080	46	55438	47.281	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	94.560%	
24) Chloroform-d	7.647	84	216131	24.542	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	98.160%	
26) 1,2-Dichloroethane-d4	8.305	65	128081	26.518	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	106.080%	
32) Benzene-d6	8.275	84	426519	24.766	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	99.080%	
36) 1,2-Dichloropropane-d6	9.274	67	124186	25.670	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	102.680%	
41) Toluene-d8	10.323	98	409282	24.601	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	98.400%	
43) trans-1,3-Dichloroprop...	10.579	79	49886	22.395	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.600%	
47) 2-Hexanone-d5	10.927	63	46483	50.332	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.660%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	113960	25.273	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	101.080%	
66) 1,2-Dichlorobenzene-d4	13.853	152	135509	27.685	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	110.720%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023229.D
Acq On : 21 May 2022 04:13
Operator : SY/VA
Sample : VIBLK474
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK474

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 21 05:21:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 21 01:30:17 2022
Response via : Initial Calibration

