

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023232.D
 Acq On : 21 May 2022 05:25
 Operator : SY/VA
 Sample : N2926-07
 Misc : 4.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EXY16

Manual IntegrationsAPPROVED

Quant Time: May 21 06:03:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

05/22/2022
 Supervised By :Mahesh
 Dadoda

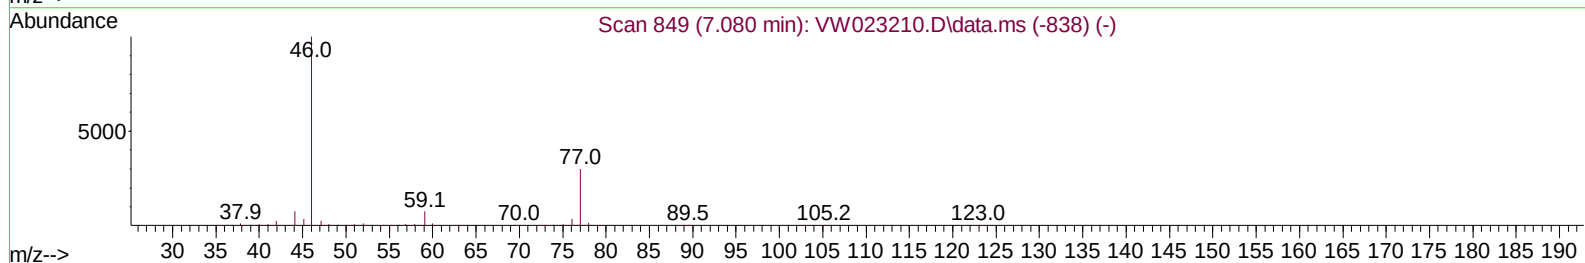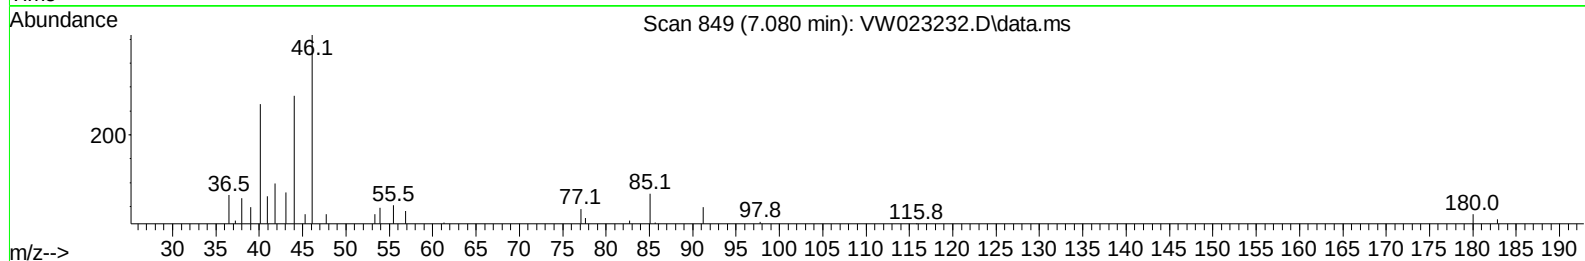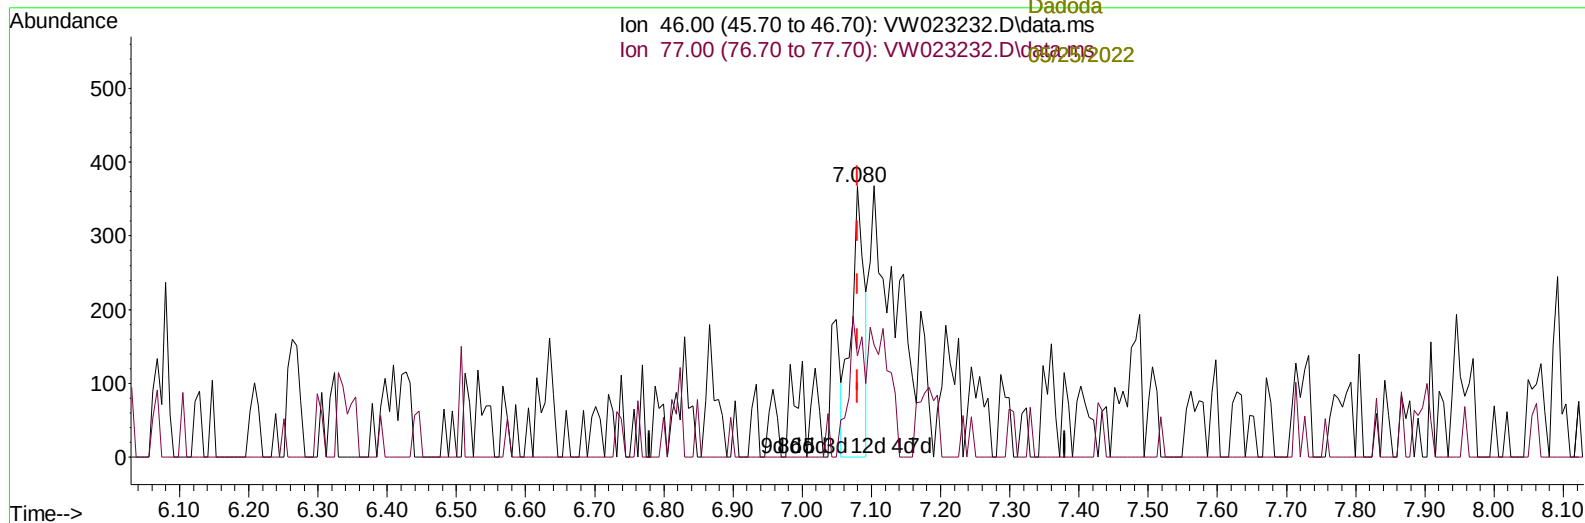

TIC: VW023232.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (-0.000) 12.36 ug/L

response 482

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	58.92#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023232.D
 Acq On : 21 May 2022 05:25
 Operator : SY/VA
 Sample : N2926-07
 Misc : 4.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY16




Manual IntegrationsAPPROVED

Quant Time: May 21 06:03:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

05/22/2022
 Supervised By :Mahesh
 Dadoda

05/23/2022

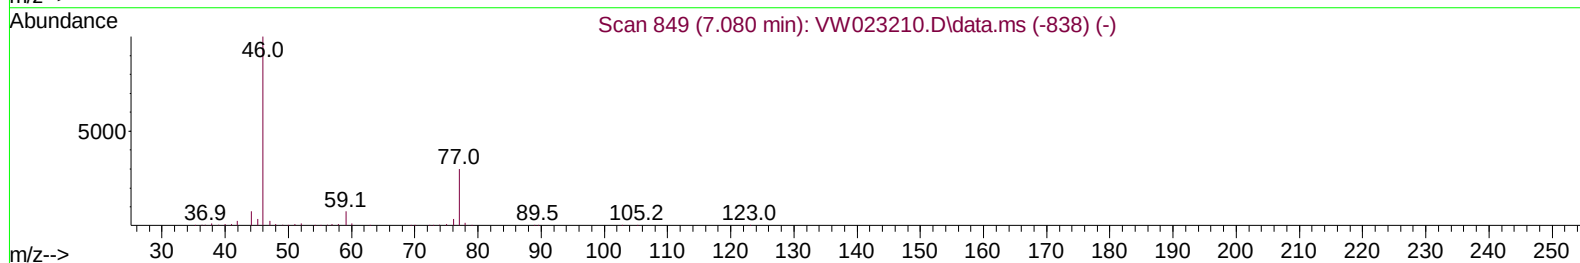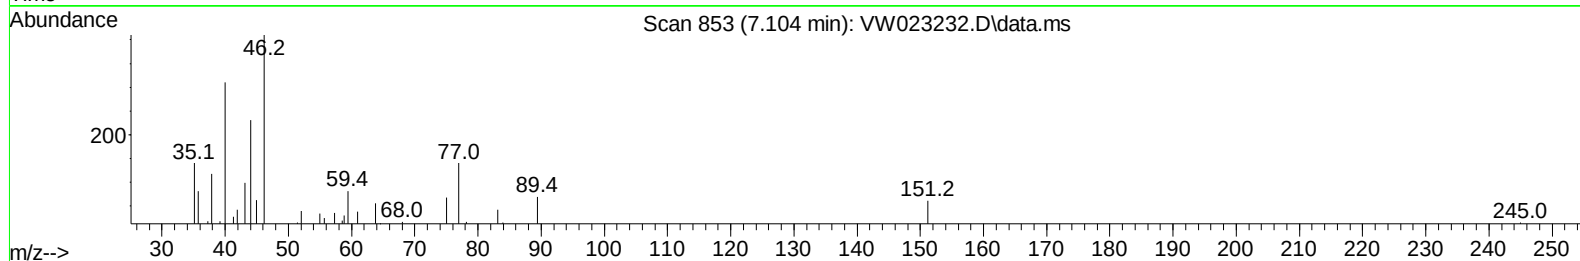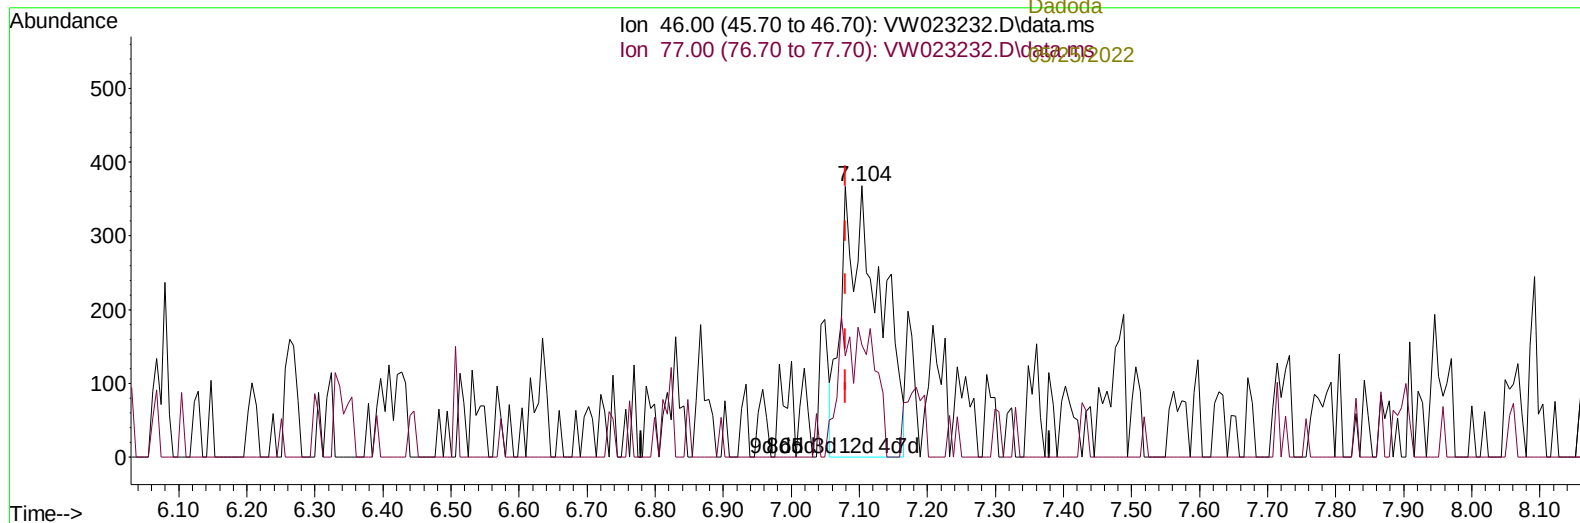

TIC: VW023232.D\data.ms

(21) 2-Butanone-d5 (S)

7.104min (+ 0.024) 36.43 ug/L m

response 1421

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	19.99
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023232.D
 Acq On : 21 May 2022 05:25
 Operator : SY/VA
 Sample : N2926-07
 Misc : 4.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY16

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

05/22/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: May 21 06:03:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----05/25/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	9999	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	10126	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	2089	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	4286	20.893	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.560%	
7) Chloroethane-d5	2.897	69	2895	21.691	ug/L	0.02
Spiked Amount 25.000	Range 30	- 150	Recovery	=	86.760%	
11) 1,1-Dichloroethene-d2	4.031	63	4536	17.112	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	68.440%	
21) 2-Butanone-d5	7.104	46	1421m	36.432	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	72.860%	
24) Chloroform-d	7.659	84	8225	28.077	ug/L	0.01
Spiked Amount 25.000	Range 40	- 150	Recovery	=	112.320%	
26) 1,2-Dichloroethane-d4	8.311	65	5118	31.854	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	127.400%	
32) Benzene-d6	8.275	84	14289	24.482	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	97.920%	
36) 1,2-Dichloropropane-d6	9.280	67	4673	28.502	ug/L	0.01
Spiked Amount 25.000	Range 70	- 120	Recovery	=	114.000%	
41) Toluene-d8	10.323	98	10768	19.098	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	76.400%	
43) trans-1,3-Dichloroprop...	10.579	79	1054	13.962	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	55.840%	
47) 2-Hexanone-d5	0.000	63	0d	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135	Recovery	=	0.000%#	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	3019	19.756	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	79.040%	
66) 1,2-Dichlorobenzene-d4	13.853	152	1787	24.471	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.880%	

Target Compounds Qvalue
 15) Methyl Acetate 4.678 43 8623 146.982 ug/L # 68

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023232.D
Acq On : 21 May 2022 05:25
Operator : SY/VA
Sample : N2926-07
Misc : 4.30g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY16

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

05/22/2022
Supervised By :Mahesh
Dadoda

05/25/2022

Quant Time: May 21 06:03:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 21 01:30:17 2022
Response via : Initial Calibration

